

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028835.D
 Acq On : 02 Nov 2022 12:44
 Operator : SY/MD
 Sample : N5353-10DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWU7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	109	rBV2	506418	586983	32.73%	4.400%
2	1.564	157	163	179	rVB	258401	293052	16.34%	2.197%
3	2.105	322	331	351	rVB	450101	642371	35.82%	4.815%
4	2.722	521	523	524	rBV2	1448	652	0.04%	0.005%
5	2.761	526	535	551	rVB	52739	94064	5.25%	0.705%
6	3.153	654	657	659	rBV4	1505	1099	0.06%	0.008%
7	3.169	659	662	663	rVV2	1032	500	0.03%	0.004%
8	3.201	669	672	676	rBV6	1914	1515	0.08%	0.011%
9	3.256	688	689	692	rBV3	1157	628	0.04%	0.005%
10	3.323	707	710	712	rVB4	1202	695	0.04%	0.005%
11	3.362	721	722	724	rBV2	1118	523	0.03%	0.004%
12	3.378	724	727	728	rVV2	1782	1104	0.06%	0.008%
13	3.400	731	734	736	rBV3	1411	833	0.05%	0.006%
14	3.439	742	746	748	rBV5	1234	960	0.05%	0.007%
15	3.568	781	786	787	rBV5	1215	1009	0.06%	0.008%
16	3.651	810	812	813	rBV2	1093	502	0.03%	0.004%
17	3.661	813	815	818	rVV3	1734	744	0.04%	0.006%
18	3.680	818	821	824	rVB5	1170	821	0.05%	0.006%
19	3.699	824	827	830	rBV4	1713	1197	0.07%	0.009%
20	3.719	830	833	835	rBV4	1367	861	0.05%	0.006%
21	3.767	846	848	852	rBV5	2304	1779	0.10%	0.013%
22	3.789	852	855	857	rBV4	1425	894	0.05%	0.007%
23	3.825	862	866	867	rBV4	919	533	0.03%	0.004%
24	3.879	873	883	923	rBV	160904	559009	31.17%	4.190%
25	4.342	1014	1027	1052	rVB	278974	669659	37.34%	5.019%
26	4.658	1122	1125	1127	rBV4	1476	817	0.05%	0.006%
27	4.738	1148	1150	1151	rBV2	1403	483	0.03%	0.004%
28	4.863	1185	1189	1192	rBV5	2521	2001	0.11%	0.015%
29	4.899	1198	1200	1201	rBV2	1714	669	0.04%	0.005%
30	5.040	1228	1244	1271	rBV2	688362	1793249	100.00%	13.441%
31	5.613	1411	1422	1454	rBV	445882	908355	50.65%	6.808%
32	6.066	1551	1563	1585	rBV	416458	849743	47.39%	6.369%
33	6.503	1697	1699	1701	rBV3	1631	955	0.05%	0.007%
34	6.535	1706	1709	1714	rVB6	1851	1473	0.08%	0.011%
35	6.629	1729	1738	1739	rBV9	3548	4124	0.23%	0.031%
36	6.905	1822	1824	1826	rBV3	2159	1227	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028835.D
 Acq On : 02 Nov 2022 12:44
 Operator : SY/MD
 Sample : N5353-10DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWU7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.918	1826	1828	1830	rVV3	1232	645	0.04%	0.005%
38	6.982	1838	1848	1872	rBV	190603	356638	19.89%	2.673%
39	7.310	1939	1950	1971	rBV	750988	1310646	73.09%	9.824%
40	7.619	2036	2046	2068	rBV	123048	224519	12.52%	1.683%
41	8.085	2181	2191	2228	rBV	488007	1002407	55.90%	7.513%
42	8.628	2356	2360	2363	rBV5	1441	1406	0.08%	0.011%
43	8.767	2400	2403	2405	rBV5	1111	722	0.04%	0.005%
44	8.847	2417	2428	2454	rVV	648346	1079225	60.18%	8.089%
45	9.056	2489	2493	2495	rBV5	2663	2232	0.12%	0.017%
46	9.448	2613	2615	2620	rBV5	1605	1256	0.07%	0.009%
47	9.529	2637	2640	2641	rBV3	1336	801	0.04%	0.006%
48	9.635	2670	2673	2674	rBV3	1709	760	0.04%	0.006%
49	9.799	2722	2724	2728	rVB4	1376	1075	0.06%	0.008%
50	9.825	2728	2732	2736	rBV5	1444	1537	0.09%	0.012%
51	9.972	2776	2778	2782	rVB5	1220	691	0.04%	0.005%
52	10.207	2840	2851	2871	rBV	529082	837920	46.73%	6.280%
53	10.484	2933	2937	2938	rBV5	2040	1305	0.07%	0.010%
54	10.522	2947	2949	2952	rBV4	1630	832	0.05%	0.006%
55	10.667	2993	2994	2997	rBV3	1041	509	0.03%	0.004%
56	10.683	2997	2999	3003	rVB3	1698	957	0.05%	0.007%
57	10.709	3003	3007	3009	rBV4	1258	981	0.05%	0.007%
58	10.757	3019	3022	3023	rBV3	1545	860	0.05%	0.006%
59	10.796	3031	3034	3038	rBV6	1449	1232	0.07%	0.009%
60	10.850	3045	3051	3053	rBV7	2477	2100	0.12%	0.016%
61	10.898	3062	3066	3069	rVB6	1598	1132	0.06%	0.008%
62	10.915	3069	3071	3072	rBV2	1397	628	0.04%	0.005%
63	10.940	3077	3079	3083	rVB4	2480	1270	0.07%	0.010%
64	11.079	3120	3122	3123	rBV2	1256	484	0.03%	0.004%
65	11.243	3162	3173	3195	rBV	585008	945017	52.70%	7.083%
66	11.387	3216	3218	3221	rVB3	2964	1518	0.08%	0.011%
67	11.410	3221	3225	3228	rVB6	2026	1508	0.08%	0.011%
68	11.615	3277	3289	3309	rBV	677032	1100340	61.36%	8.247%
69	11.934	3386	3388	3389	rBV2	1723	819	0.05%	0.006%
70	12.098	3434	3439	3445	rBV8	2476	3799	0.21%	0.028%
71	12.233	3479	3481	3483	rBV3	972	504	0.03%	0.004%
72	12.336	3510	3513	3516	rBV4	1203	768	0.04%	0.006%
73	12.423	3538	3540	3543	rVB3	1291	564	0.03%	0.004%
74	12.439	3543	3545	3546	rBV2	1075	483	0.03%	0.004%
75	12.670	3615	3617	3619	rBV3	1248	621	0.03%	0.005%
76	12.686	3620	3622	3625	rVB3	1641	708	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028835.D
 Acq On : 02 Nov 2022 12:44
 Operator : SY/MD
 Sample : N5353-10DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWU7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.760	3643	3645	3647	rVB3	1619	668	0.04%	0.005%
78	12.776	3647	3650	3652	rBV4	1436	899	0.05%	0.007%
79	12.799	3655	3657	3659	rBV2	1163	670	0.04%	0.005%
80	12.918	3690	3694	3698	rBV6	1667	1308	0.07%	0.010%
81	12.943	3698	3702	3703	rBV4	901	487	0.03%	0.004%
82	13.066	3737	3740	3741	rBV3	1194	683	0.04%	0.005%
83	13.114	3751	3755	3761	rBV10	1210	936	0.05%	0.007%
84	13.239	3789	3794	3795	rBV5	1988	1632	0.09%	0.012%
85	13.304	3811	3814	3819	rBV6	1762	1785	0.10%	0.013%
86	13.467	3863	3865	3871	rVB7	1441	933	0.05%	0.007%
87	13.635	3913	3917	3919	rBV4	1549	1096	0.06%	0.008%
88	13.767	3956	3958	3960	rVB3	1501	484	0.03%	0.004%
89	13.805	3966	3970	3972	rBV5	1609	1282	0.07%	0.010%
90	13.940	4010	4012	4016	rBV5	1945	1374	0.08%	0.010%
91	13.995	4025	4029	4031	rBV5	2364	1749	0.10%	0.013%
92	14.127	4068	4070	4072	rBV3	1465	869	0.05%	0.007%
93	14.358	4139	4142	4144	rBV3	1644	1113	0.06%	0.008%
94	14.384	4148	4150	4153	rVV4	1684	932	0.05%	0.007%
95	14.557	4202	4204	4205	rBV2	1554	688	0.04%	0.005%
96	14.631	4223	4227	4229	rBV6	1711	1294	0.07%	0.010%
97	15.017	4342	4347	4350	rBV8	2021	2159	0.12%	0.016%
98	15.049	4355	4357	4358	rBV2	1627	647	0.04%	0.005%
99	15.178	4395	4397	4399	rVB3	1611	502	0.03%	0.004%
100	15.313	4437	4439	4442	rBV4	1509	973	0.05%	0.007%




Sum of corrected areas: 13341665

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028835.D
Acq On : 02 Nov 2022 12:44
Operator : SY/MD
Sample : N5353-10DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWU7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

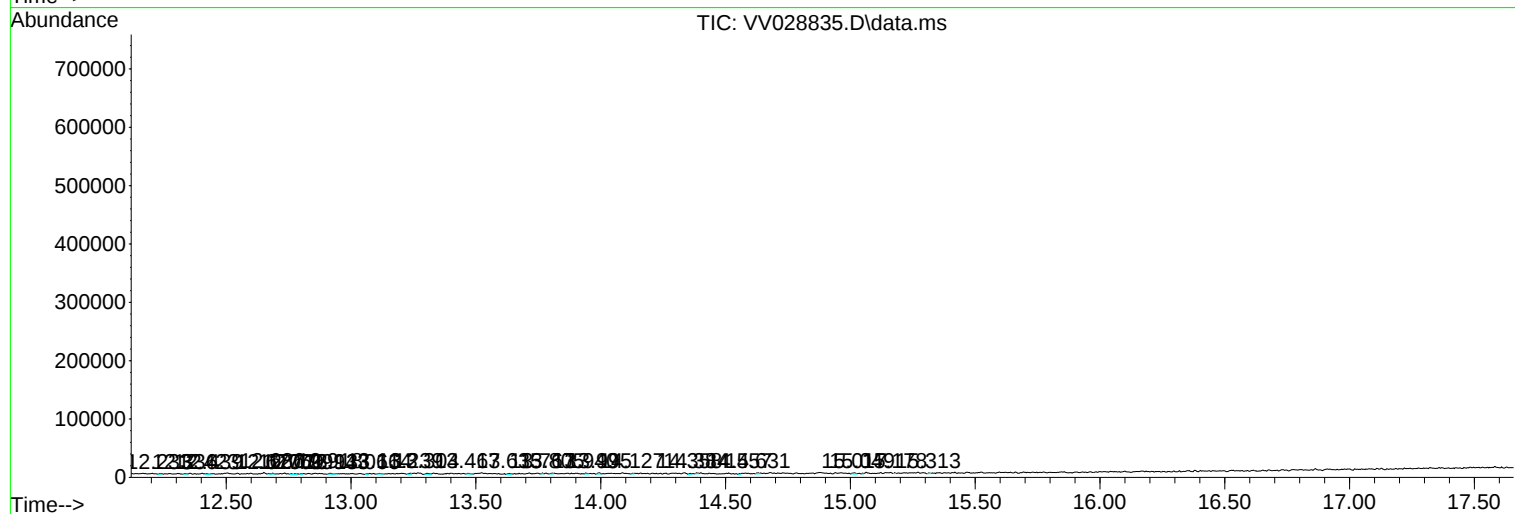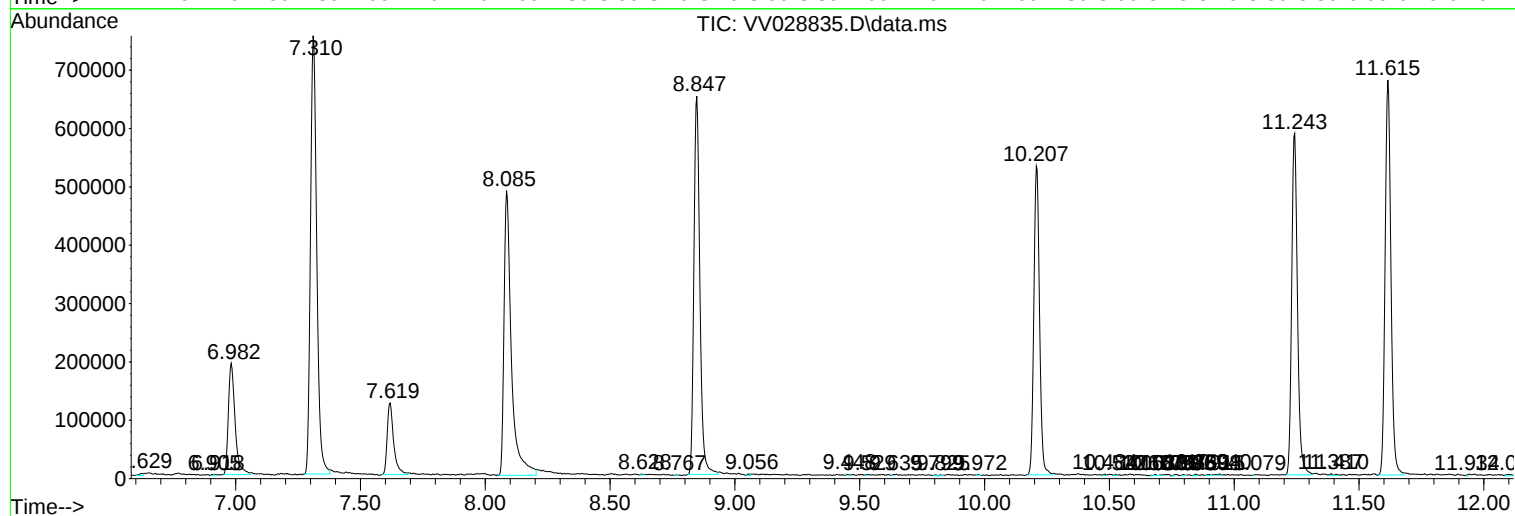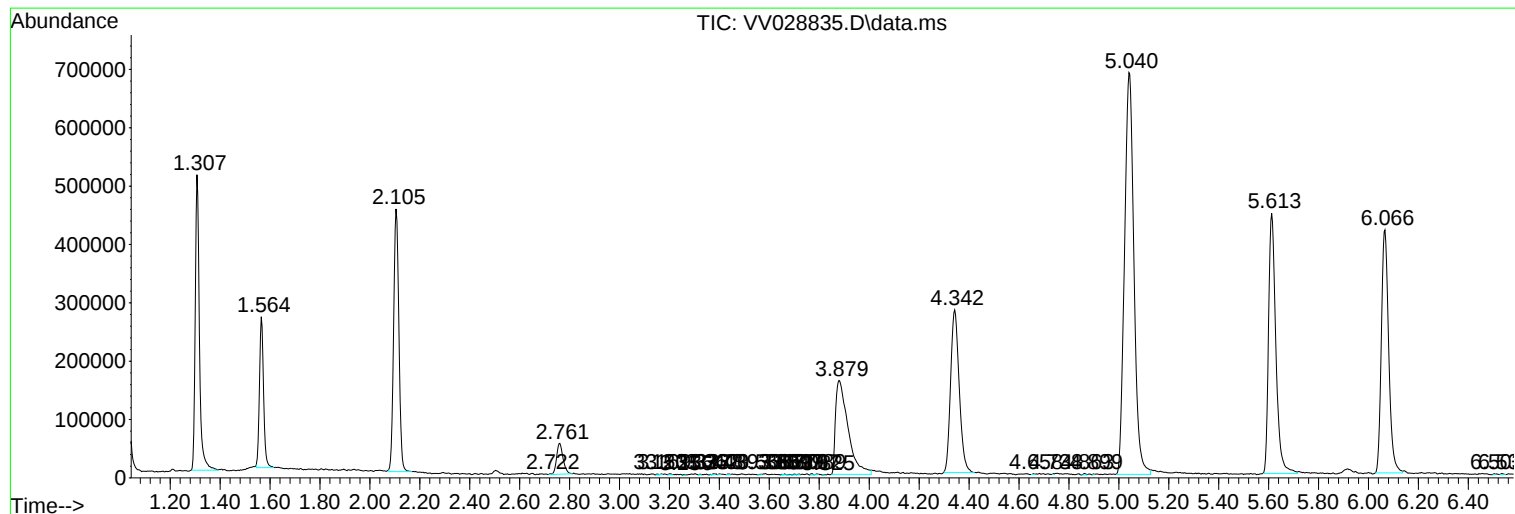

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028835.D
Acq On : 02 Nov 2022 12:44
Operator : SY/MD
Sample : N5353-10DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWU7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028835.D
Acq On : 02 Nov 2022 12:44
Operator : SY/MD
Sample : N5353-10DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWU7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------