

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028836.D
 Acq On : 02 Nov 2022 13:08
 Operator : SY/MD
 Sample : N5321-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rBV2	235581	269460	13.90%	1.742%
2	1.564	157	163	176	rVB	239598	273101	14.08%	1.765%
3	2.105	322	331	344	rBV	413767	592956	30.58%	3.833%
4	2.365	408	412	418	rVB8	2091	1814	0.09%	0.012%
5	2.757	524	534	555	rBV	147869	264763	13.65%	1.711%
6	2.966	596	599	604	rBV7	1481	1514	0.08%	0.010%
7	3.008	609	612	616	rBV5	1186	1152	0.06%	0.007%
8	3.101	638	641	645	rVB5	1509	1047	0.05%	0.007%
9	3.172	659	663	664	rBV4	1059	687	0.04%	0.004%
10	3.214	674	676	679	rVB4	1854	862	0.04%	0.006%
11	3.240	679	684	686	rBV6	2736	2067	0.11%	0.013%
12	3.310	702	706	708	rBV5	1611	955	0.05%	0.006%
13	3.323	708	710	712	rVV3	1616	795	0.04%	0.005%
14	3.465	748	754	756	rBV6	1505	1686	0.09%	0.011%
15	3.510	766	768	774	rVB7	865	881	0.05%	0.006%
16	3.555	778	782	785	rBV6	1138	964	0.05%	0.006%
17	3.574	785	788	792	rBV6	1074	1075	0.06%	0.007%
18	3.641	807	809	814	rVB5	1155	802	0.04%	0.005%
19	3.902	871	890	922	rBV2	682733	1939103	100.00%	12.535%
20	4.342	1012	1027	1053	rBV	254351	639534	32.98%	4.134%
21	4.571	1096	1098	1101	rBV4	1367	912	0.05%	0.006%
22	4.773	1157	1161	1165	rBV6	1313	1469	0.08%	0.009%
23	4.940	1208	1213	1215	rBV5	1837	1710	0.09%	0.011%
24	4.966	1219	1221	1223	rBV3	1284	719	0.04%	0.005%
25	5.040	1229	1244	1271	rBV2	626614	1646101	84.89%	10.641%
26	5.612	1411	1422	1448	rBV	523869	1057823	54.55%	6.838%
27	5.908	1502	1514	1537	rBV	578666	1133685	58.46%	7.328%
28	6.066	1552	1563	1586	rVB	384474	777924	40.12%	5.029%
29	6.436	1676	1678	1681	rVB4	1152	640	0.03%	0.004%
30	6.558	1713	1716	1717	rBV3	1814	1058	0.05%	0.007%
31	6.625	1735	1737	1738	rBV	1959	882	0.05%	0.006%
32	6.776	1782	1784	1789	rBV6	1514	1012	0.05%	0.007%
33	6.982	1839	1848	1864	rBV	174971	318489	16.42%	2.059%
34	7.310	1939	1950	1975	rBV	699210	1214406	62.63%	7.850%
35	7.619	2038	2046	2066	rVB	110757	193117	9.96%	1.248%
36	7.899	2130	2133	2134	rBV3	1641	985	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028836.D
 Acq On : 02 Nov 2022 13:08
 Operator : SY/MD
 Sample : N5321-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	8.085	2179	2191	2221	rBV	438198	888981	45.84%	5.747%
38	8.532	2325	2330	2331	rBV5	1893	1444	0.07%	0.009%
39	8.641	2362	2364	2365	rBV2	1449	636	0.03%	0.004%
40	8.686	2375	2378	2381	rBV4	1327	1026	0.05%	0.007%
41	8.702	2381	2383	2388	rVB6	1617	1084	0.06%	0.007%
42	8.728	2388	2391	2392	rBV3	1872	895	0.05%	0.006%
43	8.847	2417	2428	2451	rBV	768235	1263808	65.17%	8.170%
44	9.120	2512	2513	2518	rVB5	1909	917	0.05%	0.006%
45	9.278	2559	2562	2563	rVB3	1382	592	0.03%	0.004%
46	9.352	2582	2585	2595	rVB3	1844	2042	0.11%	0.013%
47	9.471	2619	2622	2625	rBV5	815	650	0.03%	0.004%
48	9.506	2630	2633	2637	rVB6	1452	1236	0.06%	0.008%
49	9.599	2660	2662	2664	rBV3	1522	758	0.04%	0.005%
50	9.632	2670	2672	2674	rBV3	1675	790	0.04%	0.005%
51	9.673	2681	2685	2686	rBV4	1768	1165	0.06%	0.008%
52	9.728	2700	2702	2705	rBV3	908	667	0.03%	0.004%
53	9.757	2709	2711	2715	rBV4	1103	683	0.04%	0.004%
54	9.821	2728	2731	2735	rBV6	1864	1556	0.08%	0.010%
55	10.027	2792	2795	2798	rBV5	1694	1051	0.05%	0.007%
56	10.207	2834	2851	2868	rBV	485156	777298	40.09%	5.025%
57	10.323	2884	2887	2891	rBV5	1788	1489	0.08%	0.010%
58	10.378	2898	2904	2909	rBV10	3261	4690	0.24%	0.030%
59	10.458	2927	2929	2933	rVB4	1029	635	0.03%	0.004%
60	10.516	2943	2947	2951	rVB6	1676	1566	0.08%	0.010%
61	10.689	2998	3001	3003	rBV5	1181	812	0.04%	0.005%
62	10.789	3030	3032	3034	rBV3	1529	602	0.03%	0.004%
63	10.985	3090	3093	3095	rBV4	1342	715	0.04%	0.005%
64	11.040	3107	3110	3113	rBV5	1157	859	0.04%	0.006%
65	11.242	3162	3173	3196	rBV	689121	1113650	57.43%	7.199%
66	11.487	3247	3249	3254	rVB6	2292	1597	0.08%	0.010%
67	11.615	3278	3289	3312	rVB	631388	1010213	52.10%	6.530%
68	11.840	3355	3359	3361	rBV4	2025	1525	0.08%	0.010%
69	12.017	3410	3414	3416	rBV4	1546	973	0.05%	0.006%
70	12.037	3417	3420	3421	rBV2	1260	757	0.04%	0.005%
71	12.130	3447	3449	3451	rVB3	1818	763	0.04%	0.005%
72	12.149	3451	3455	3458	rVB5	1830	1378	0.07%	0.009%
73	12.165	3458	3460	3464	rBV4	1224	1097	0.06%	0.007%
74	12.226	3477	3479	3482	rBV4	1536	710	0.04%	0.005%
75	12.320	3505	3508	3510	rBV5	1098	594	0.03%	0.004%
76	12.535	3573	3575	3579	rVB5	2158	1350	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028836.D
 Acq On : 02 Nov 2022 13:08
 Operator : SY/MD
 Sample : N5321-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.564	3579	3584	3586	rBV5	1968	1662	0.09%	0.011%
78	12.577	3586	3588	3593	rVB6	2002	1360	0.07%	0.009%
79	12.612	3593	3599	3600	rBV6	2356	2036	0.10%	0.013%
80	12.641	3606	3608	3615	rBV8	1809	1340	0.07%	0.009%
81	12.754	3641	3643	3646	rVV3	1317	707	0.04%	0.005%
82	12.789	3651	3654	3656	rBV3	1804	1072	0.06%	0.007%
83	12.831	3661	3667	3668	rBV6	1701	1227	0.06%	0.008%
84	12.911	3690	3692	3695	rBV4	1514	703	0.04%	0.005%
85	13.091	3746	3748	3751	rBV3	1448	923	0.05%	0.006%
86	13.107	3751	3753	3755	rBV3	1642	788	0.04%	0.005%
87	13.236	3790	3793	3796	rVB4	1452	934	0.05%	0.006%
88	13.262	3796	3801	3806	rBV8	2257	2611	0.13%	0.017%
89	13.316	3814	3818	3821	rBV4	2067	1591	0.08%	0.010%
90	13.557	3889	3893	3894	rBV4	1743	1048	0.05%	0.007%
91	13.667	3925	3927	3930	rBV4	1565	1128	0.06%	0.007%
92	13.818	3970	3974	3978	rVB5	2070	1519	0.08%	0.010%
93	13.844	3978	3982	3983	rBV4	1650	949	0.05%	0.006%
94	13.898	3997	3999	4001	rBV3	1335	697	0.04%	0.005%
95	13.969	4019	4021	4027	rBV7	1086	1093	0.06%	0.007%
96	14.194	4087	4091	4097	rVB8	1867	1885	0.10%	0.012%
97	14.223	4097	4100	4101	rBV3	2334	1268	0.07%	0.008%
98	14.577	4208	4210	4212	rBV3	1369	748	0.04%	0.005%
99	14.979	4333	4335	4342	rBV8	1959	1807	0.09%	0.012%
100	15.310	4434	4438	4440	rBV5	1367	1151	0.06%	0.007%




Sum of corrected areas: 15469651

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028836.D
Acq On : 02 Nov 2022 13:08
Operator : SY/MD
Sample : N5321-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

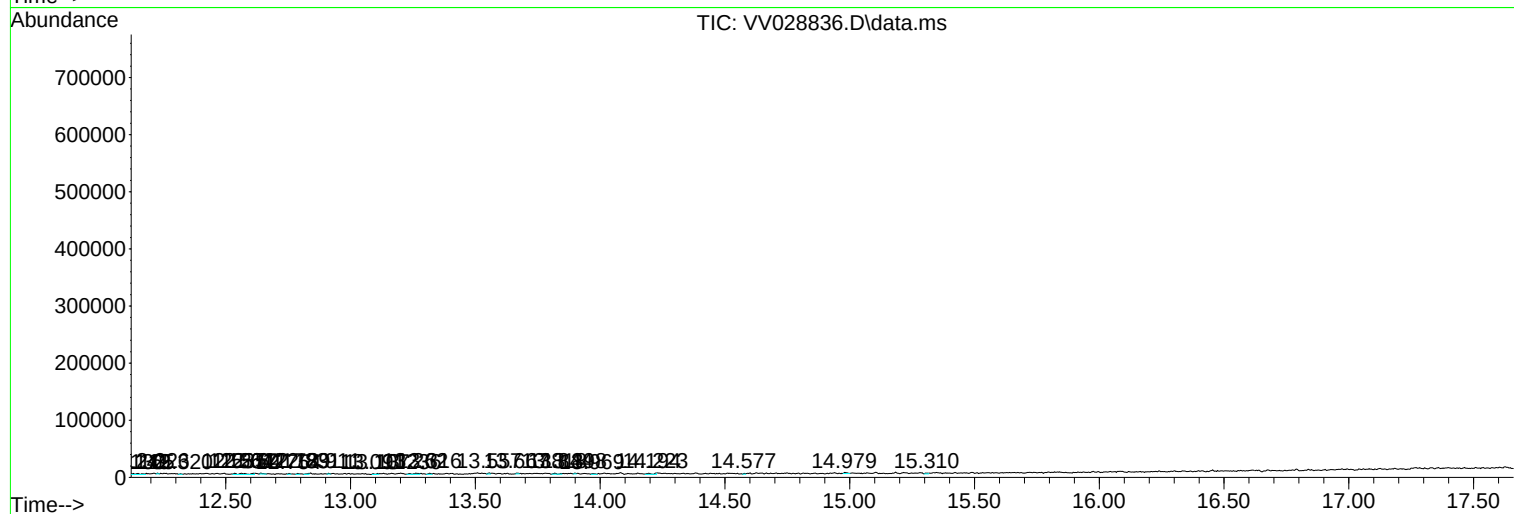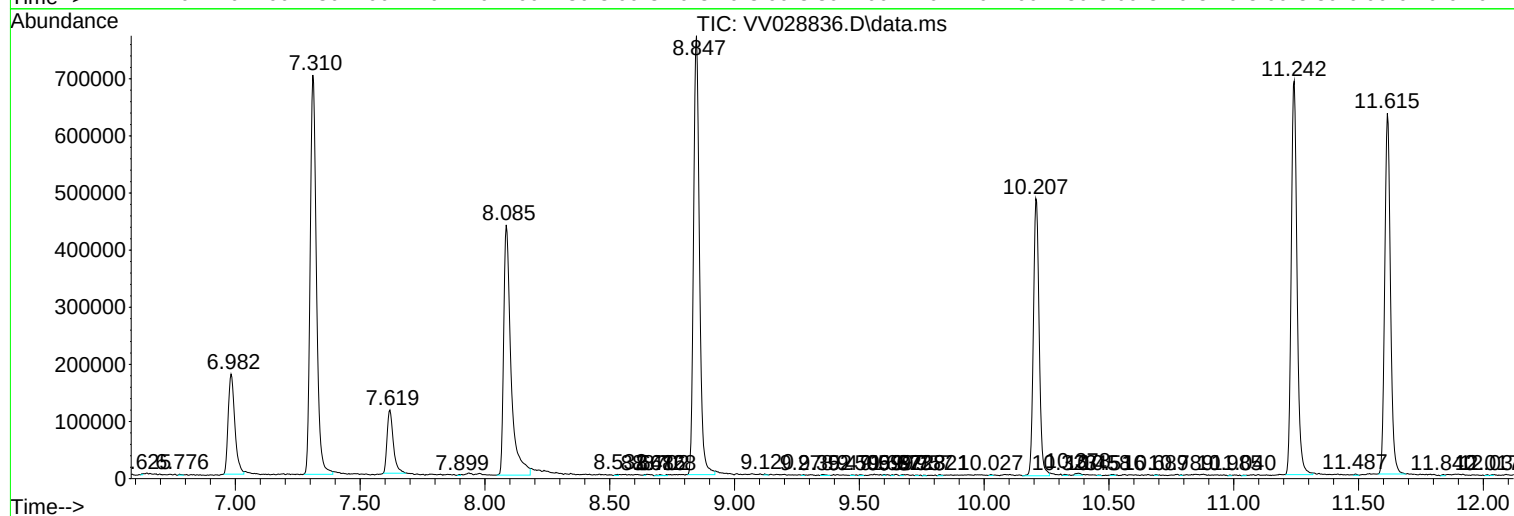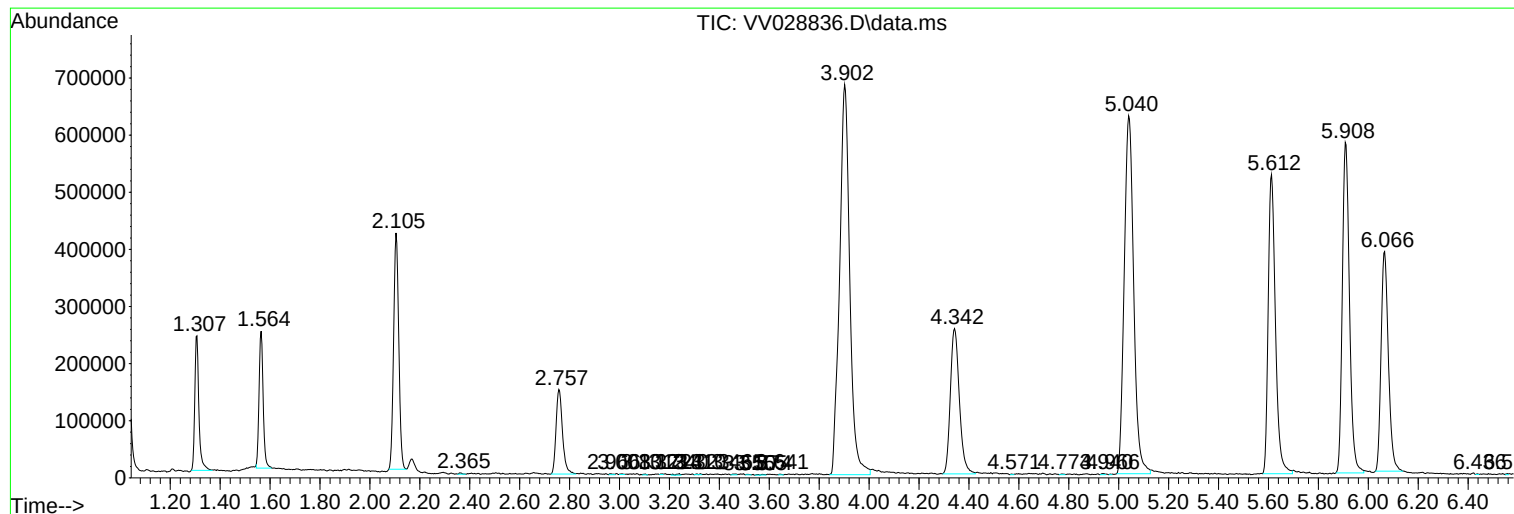

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028836.D
Acq On : 02 Nov 2022 13:08
Operator : SY/MD
Sample : N5321-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028836.D
Acq On : 02 Nov 2022 13:08
Operator : SY/MD
Sample : N5321-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc