

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028837.D
 Acq On : 02 Nov 2022 13:32
 Operator : SY/MD
 Sample : N5321-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rBV2	234206	261805	13.53%	1.706%
2	1.564	156	163	176	rVB	230685	267320	13.82%	1.742%
3	2.105	322	331	344	rVB	415612	596274	30.82%	3.885%
4	2.436	430	434	435	rBV4	1641	1326	0.07%	0.009%
5	2.548	467	469	472	rBV5	1206	897	0.05%	0.006%
6	2.757	525	534	554	rVB	148416	261479	13.51%	1.704%
7	2.966	598	599	603	rBV4	1074	615	0.03%	0.004%
8	3.056	625	627	629	rBV2	1290	607	0.03%	0.004%
9	3.140	649	653	655	rBV4	2798	1819	0.09%	0.012%
10	3.214	674	676	679	rVB4	1346	823	0.04%	0.005%
11	3.230	679	681	683	rBV3	1258	779	0.04%	0.005%
12	3.349	715	718	719	rBV3	912	386	0.02%	0.003%
13	3.359	719	721	724	rVB4	1439	701	0.04%	0.005%
14	3.378	724	727	732	rBV5	1815	1796	0.09%	0.012%
15	3.400	732	734	738	rVB4	1199	661	0.03%	0.004%
16	3.449	746	749	751	rBV4	1641	1190	0.06%	0.008%
17	3.481	756	759	763	rBV6	1711	1705	0.09%	0.011%
18	3.513	767	769	770	rBV2	1050	377	0.02%	0.002%
19	3.555	775	782	784	rBV7	1945	2113	0.11%	0.014%
20	3.600	794	796	798	rVB3	1564	545	0.03%	0.004%
21	3.703	826	828	829	rVB2	817	173	0.01%	0.001%
22	3.735	833	838	843	rBV8	1729	2301	0.12%	0.015%
23	3.834	867	869	871	rBV3	1186	429	0.02%	0.003%
24	3.902	871	890	925	rBV2	672977	1934992	100.00%	12.607%
25	4.281	1003	1008	1010	rBV5	1928	1733	0.09%	0.011%
26	4.342	1015	1027	1052	rVB	253887	625911	32.35%	4.078%
27	4.818	1172	1175	1178	rBV4	2075	1282	0.07%	0.008%
28	5.040	1228	1244	1278	rBV2	631044	1666058	86.10%	10.855%
29	5.465	1374	1376	1379	rBV4	1551	917	0.05%	0.006%
30	5.487	1381	1383	1384	rBV2	1610	602	0.03%	0.004%
31	5.612	1410	1422	1444	rBV	513991	1029130	53.19%	6.705%
32	5.908	1502	1514	1540	rBV	576269	1133248	58.57%	7.383%
33	6.066	1552	1563	1592	rVB2	387491	791655	40.91%	5.158%
34	6.506	1698	1700	1702	rBV2	1154	424	0.02%	0.003%
35	6.921	1824	1829	1831	rBV5	1447	1328	0.07%	0.009%
36	6.934	1831	1833	1834	rBV2	1124	358	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028837.D
 Acq On : 02 Nov 2022 13:32
 Operator : SY/MD
 Sample : N5321-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.982	1837	1848	1871	rBV	175092	335765	17.35%	2.188%
38	7.249	1928	1931	1935	rBV5	1903	1907	0.10%	0.012%
39	7.310	1939	1950	1974	rBV	686804	1214843	62.78%	7.915%
40	7.619	2037	2046	2068	rBV	110055	198604	10.26%	1.294%
41	8.085	2181	2191	2224	rBV	441124	882217	45.59%	5.748%
42	8.561	2335	2339	2342	rBV6	1527	1537	0.08%	0.010%
43	8.712	2384	2386	2387	rBV2	1430	567	0.03%	0.004%
44	8.847	2417	2428	2463	rBV	742088	1227628	63.44%	7.998%
45	9.526	2637	2639	2641	rVB2	1204	376	0.02%	0.002%
46	9.545	2641	2645	2650	rBV8	2491	2747	0.14%	0.018%
47	9.603	2660	2663	2667	rBV4	2419	1806	0.09%	0.012%
48	9.635	2668	2673	2674	rBV5	1555	1080	0.06%	0.007%
49	9.812	2726	2728	2732	rVB6	1151	774	0.04%	0.005%
50	9.850	2737	2740	2741	rBV3	1126	782	0.04%	0.005%
51	9.886	2748	2751	2752	rBV3	1503	695	0.04%	0.005%
52	9.927	2761	2764	2766	rBV4	841	514	0.03%	0.003%
53	9.982	2779	2781	2784	rVB3	1642	580	0.03%	0.004%
54	10.011	2788	2790	2795	rBV5	1668	1218	0.06%	0.008%
55	10.169	2838	2839	2840	rBV	2044	701	0.04%	0.005%
56	10.207	2840	2851	2870	rVV	485678	770763	39.83%	5.022%
57	10.378	2897	2904	2910	rBV9	4850	6319	0.33%	0.041%
58	10.513	2943	2946	2948	rBV4	1265	885	0.05%	0.006%
59	10.635	2982	2984	2989	rBV6	1300	808	0.04%	0.005%
60	10.693	2999	3002	3003	rBV3	1388	553	0.03%	0.004%
61	10.741	3016	3017	3018	rVB	1243	240	0.01%	0.002%
62	10.770	3025	3026	3030	rBV3	1637	1048	0.05%	0.007%
63	10.815	3038	3040	3042	rBV3	954	533	0.03%	0.003%
64	10.882	3059	3061	3064	rBV5	1190	900	0.05%	0.006%
65	10.956	3082	3084	3085	rBV2	1270	360	0.02%	0.002%
66	11.011	3098	3101	3102	rBV2	1694	1066	0.06%	0.007%
67	11.040	3108	3110	3112	rBV3	795	289	0.01%	0.002%
68	11.127	3133	3137	3139	rBV5	1502	1132	0.06%	0.007%
69	11.242	3162	3173	3192	rBV	665599	1061982	54.88%	6.919%
70	11.615	3278	3289	3310	rBV	632915	1006742	52.03%	6.559%
71	11.988	3397	3405	3410	rBV	2297	3544	0.18%	0.023%
72	12.236	3477	3482	3483	rBV4	1303	1284	0.07%	0.008%
73	12.339	3511	3514	3517	rVB5	1887	1218	0.06%	0.008%
74	12.358	3518	3520	3521	rBV	1066	255	0.01%	0.002%
75	12.371	3521	3524	3525	rBV3	1659	1005	0.05%	0.007%
76	12.445	3545	3547	3550	rBV4	1116	749	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028837.D
 Acq On : 02 Nov 2022 13:32
 Operator : SY/MD
 Sample : N5321-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.725	3632	3634	3637	rBV3	1119	837	0.04%	0.005%
78	12.767	3646	3647	3649	rBV2	1051	435	0.02%	0.003%
79	12.812	3658	3661	3662	rBV4	1601	712	0.04%	0.005%
80	12.982	3709	3714	3716	rBV6	1396	1162	0.06%	0.008%
81	13.040	3730	3732	3735	rVB4	2294	1352	0.07%	0.009%
82	13.059	3735	3738	3739	rBV2	826	447	0.02%	0.003%
83	13.069	3739	3741	3744	rVB3	1922	876	0.05%	0.006%
84	13.088	3745	3747	3749	rBV3	1834	821	0.04%	0.005%
85	13.181	3773	3776	3777	rBV3	1616	808	0.04%	0.005%
86	13.217	3782	3787	3790	rBV8	1465	1319	0.07%	0.009%
87	13.310	3814	3816	3817	rBV2	844	270	0.01%	0.002%
88	13.339	3824	3825	3827	rBV2	1197	603	0.03%	0.004%
89	13.619	3911	3912	3914	rBV2	1405	694	0.04%	0.005%
90	13.667	3926	3927	3928	rBV	1008	300	0.02%	0.002%
91	13.693	3932	3935	3937	rBV4	1605	1163	0.06%	0.008%
92	13.741	3947	3950	3951	rBV3	1150	610	0.03%	0.004%
93	13.808	3968	3971	3974	rBV5	1445	1200	0.06%	0.008%
94	13.976	4022	4023	4026	rVB3	1221	515	0.03%	0.003%
95	14.172	4083	4084	4085	rBV	1431	372	0.02%	0.002%
96	14.204	4092	4094	4101	rBV7	1225	1169	0.06%	0.008%
97	14.275	4112	4116	4118	rBV3	2048	1452	0.08%	0.009%
98	14.303	4123	4125	4127	rBV3	1398	821	0.04%	0.005%
99	14.631	4225	4227	4230	rBV4	1235	938	0.05%	0.006%




Sum of corrected areas: 15348651

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028837.D
Acq On : 02 Nov 2022 13:32
Operator : SY/MD
Sample : N5321-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

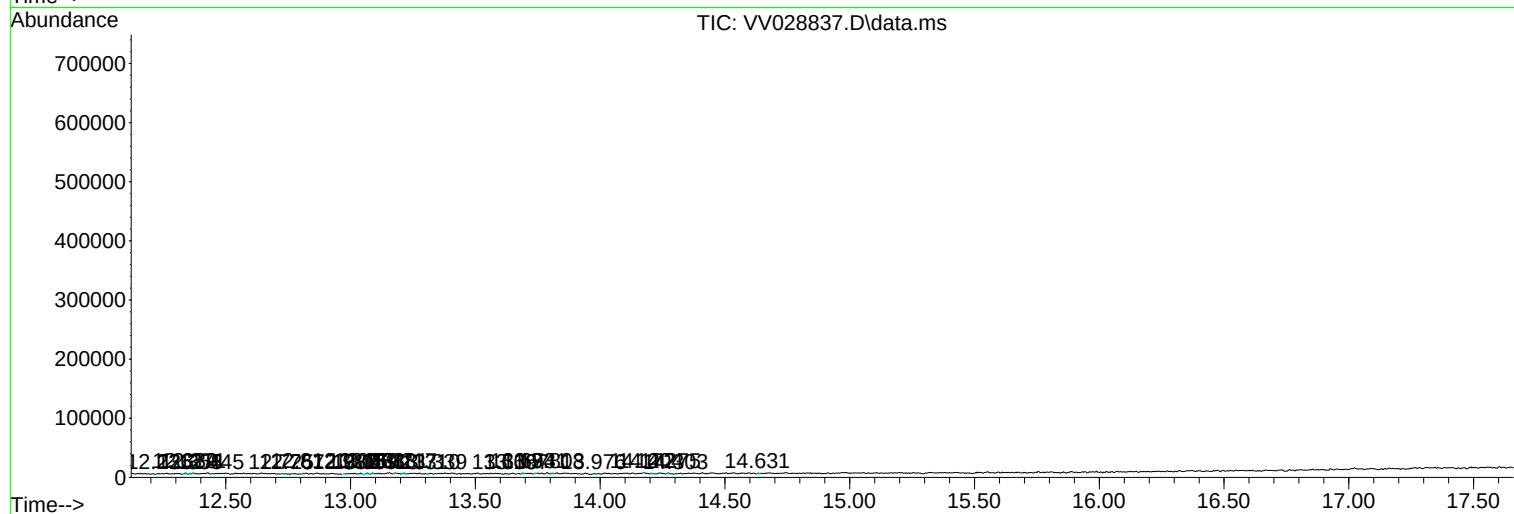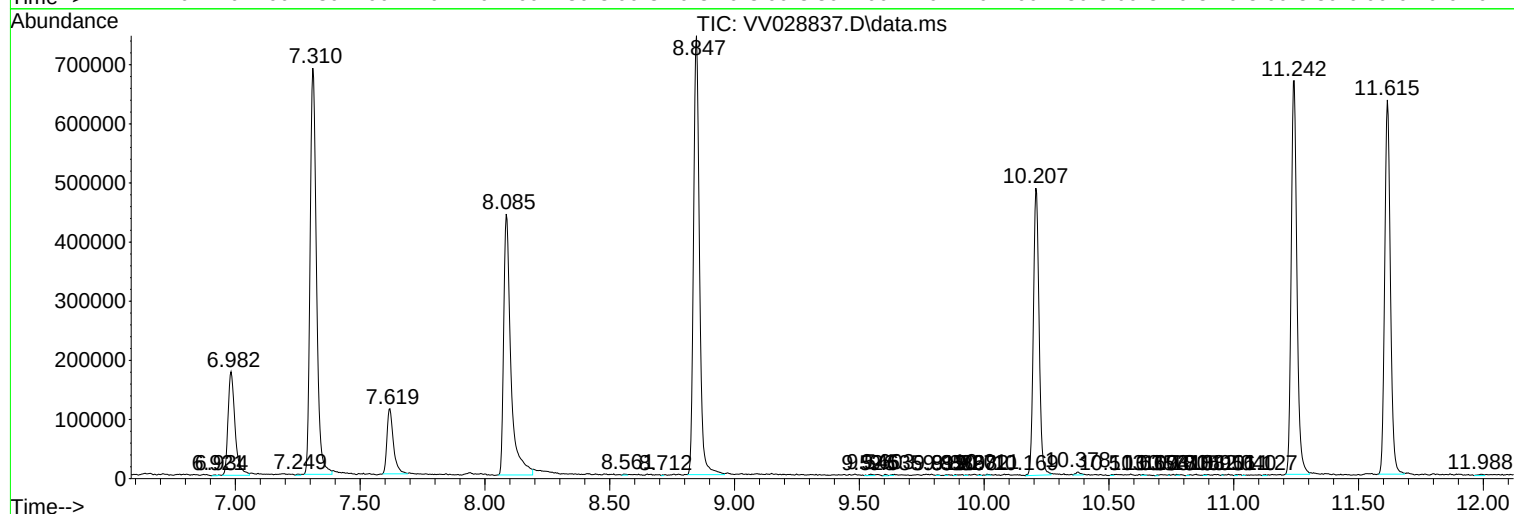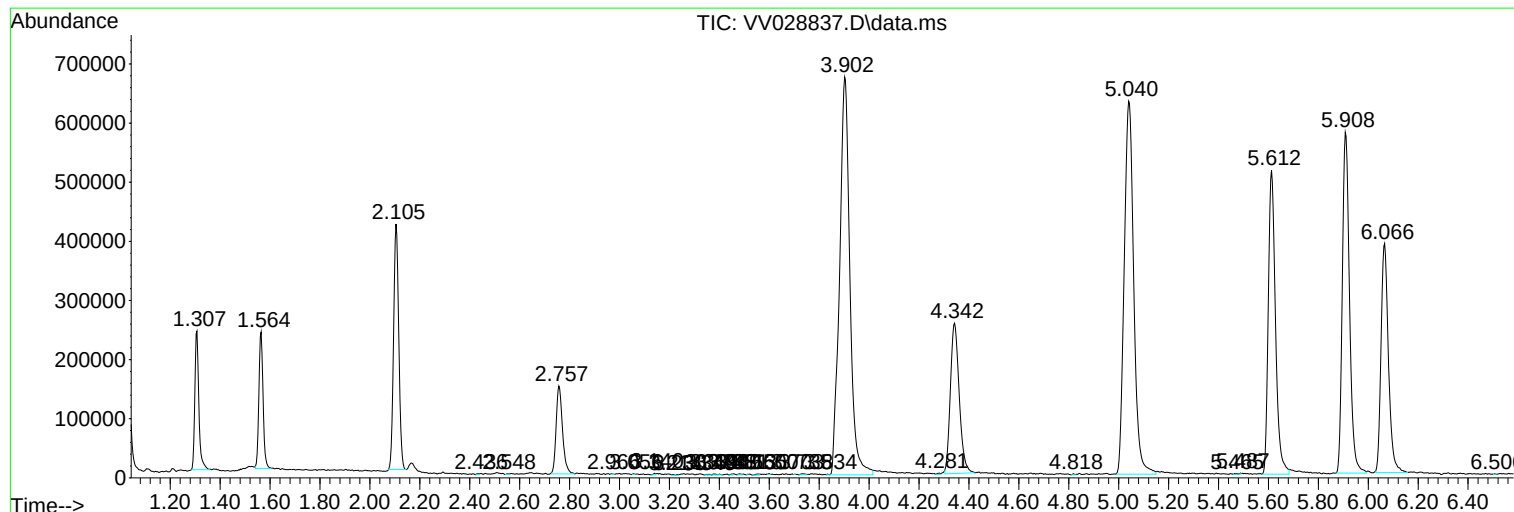

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028837.D
Acq On : 02 Nov 2022 13:32
Operator : SY/MD
Sample : N5321-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028837.D
Acq On : 02 Nov 2022 13:32
Operator : SY/MD
Sample : N5321-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc