

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028838.D
 Acq On : 02 Nov 2022 13:56
 Operator : SY/MD
 Sample : N5353-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028838.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rBV	215502	241810	14.13%	1.899%
2	1.564	156	163	176	rVB	240963	282274	16.49%	2.217%
3	2.105	322	331	348	rVB	426280	611173	35.71%	4.801%
4	2.436	430	434	438	rVB6	2118	1652	0.10%	0.013%
5	2.458	438	441	443	rBV4	2461	1655	0.10%	0.013%
6	2.696	511	515	518	rBV6	2703	2278	0.13%	0.018%
7	2.831	553	557	559	rBV4	1656	1190	0.07%	0.009%
8	2.847	559	562	563	rBV3	1377	681	0.04%	0.005%
9	2.989	604	606	611	rVB6	1895	1252	0.07%	0.010%
10	3.021	611	616	617	rBV4	1390	978	0.06%	0.008%
11	3.134	647	651	654	rVV5	1466	1165	0.07%	0.009%
12	3.150	654	656	659	rVB3	1094	600	0.04%	0.005%
13	3.169	659	662	663	rBV3	1317	689	0.04%	0.005%
14	3.291	697	700	702	rVV4	1181	700	0.04%	0.005%
15	3.391	728	731	733	rBV4	922	758	0.04%	0.006%
16	3.452	748	750	755	rVB5	1399	893	0.05%	0.007%
17	3.474	755	757	761	rVB5	1180	656	0.04%	0.005%
18	3.532	773	775	779	rVB5	1844	913	0.05%	0.007%
19	3.564	781	785	788	rBV5	1205	1059	0.06%	0.008%
20	3.600	791	796	797	rBV5	2038	1904	0.11%	0.015%
21	3.658	812	814	816	rBV3	1086	731	0.04%	0.006%
22	3.831	866	868	872	rVB5	1609	1068	0.06%	0.008%
23	3.873	872	881	912	rBV	150704	435275	25.43%	3.419%
24	4.265	1001	1003	1008	rBV6	1722	850	0.05%	0.007%
25	4.342	1012	1027	1057	rVB	260770	652560	38.13%	5.126%
26	4.651	1121	1123	1125	rBV3	1131	684	0.04%	0.005%
27	4.732	1146	1148	1151	rBV4	1338	648	0.04%	0.005%
28	4.789	1164	1166	1169	rVB3	1487	670	0.04%	0.005%
29	4.812	1169	1173	1176	rBV5	1976	1894	0.11%	0.015%
30	4.957	1216	1218	1221	rVB4	1707	826	0.05%	0.006%
31	4.976	1221	1224	1227	rBV4	1526	1194	0.07%	0.009%
32	5.040	1228	1244	1274	rBV2	659918	1711630	100.00%	13.444%
33	5.285	1317	1320	1321	rBV3	2086	938	0.05%	0.007%
34	5.481	1377	1381	1382	rBV4	1730	1279	0.07%	0.010%
35	5.526	1393	1395	1398	rVB4	1308	703	0.04%	0.006%
36	5.613	1411	1422	1455	rBV	507295	1018323	59.49%	7.999%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028838.D
 Acq On : 02 Nov 2022 13:56
 Operator : SY/MD
 Sample : N5353-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.066	1550	1563	1592	rBV	405120	824200	48.15%	6.474%
38	6.294	1632	1634	1637	rBV4	1977	1177	0.07%	0.009%
39	6.555	1712	1715	1718	rBV4	1811	1414	0.08%	0.011%
40	6.844	1802	1805	1811	rVB8	1668	1579	0.09%	0.012%
41	6.982	1836	1848	1871	rBV	181251	340888	19.92%	2.678%
42	7.310	1939	1950	1970	rBV	726529	1254017	73.26%	9.850%
43	7.551	2022	2025	2026	rBV3	1476	849	0.05%	0.007%
44	7.619	2037	2046	2065	rBV	114253	205647	12.01%	1.615%
45	7.799	2100	2102	2105	rBV4	1519	1094	0.06%	0.009%
46	7.966	2151	2154	2157	rBV4	2094	1894	0.11%	0.015%
47	7.982	2157	2159	2161	rBV3	1391	818	0.05%	0.006%
48	8.085	2179	2191	2224	rBV	486762	955320	55.81%	7.504%
49	8.487	2313	2316	2319	rBV5	1407	1144	0.07%	0.009%
50	8.574	2341	2343	2346	rBV5	1633	1181	0.07%	0.009%
51	8.847	2417	2428	2451	rBV	730249	1221247	71.35%	9.593%
52	9.233	2546	2548	2549	rBV3	1391	713	0.04%	0.006%
53	9.384	2592	2595	2599	rVB5	2829	1470	0.09%	0.012%
54	9.410	2599	2603	2605	rBV4	1567	1096	0.06%	0.009%
55	9.535	2635	2642	2643	rBV7	961	1068	0.06%	0.008%
56	9.593	2656	2660	2661	rBV4	2014	1193	0.07%	0.009%
57	9.725	2695	2701	2703	rBV6	1231	1083	0.06%	0.009%
58	9.998	2783	2786	2788	rBV4	1697	1125	0.07%	0.009%
59	10.062	2804	2806	2811	rBV6	1379	1082	0.06%	0.008%
60	10.098	2814	2817	2818	rBV2	1320	821	0.05%	0.006%
61	10.207	2838	2851	2868	rBV	503011	796008	46.51%	6.252%
62	10.487	2935	2938	2940	rBV4	1777	984	0.06%	0.008%
63	10.805	3034	3037	3039	rBV3	1199	602	0.04%	0.005%
64	10.837	3042	3047	3050	rBV7	2764	2339	0.14%	0.018%
65	10.873	3055	3058	3063	rBV6	1786	1414	0.08%	0.011%
66	10.908	3066	3069	3071	rVV4	1280	750	0.04%	0.006%
67	10.921	3071	3073	3075	rVV3	1581	648	0.04%	0.005%
68	10.937	3075	3078	3082	rVB6	1381	959	0.06%	0.008%
69	10.979	3087	3091	3093	rBV5	2110	1639	0.10%	0.013%
70	11.008	3099	3100	3104	rVB3	1316	732	0.04%	0.006%
71	11.056	3113	3115	3120	rVB6	1033	769	0.04%	0.006%
72	11.091	3123	3126	3130	rBV6	1456	1248	0.07%	0.010%
73	11.111	3130	3132	3134	rBV3	1501	834	0.05%	0.007%
74	11.181	3150	3154	3155	rBV4	1511	825	0.05%	0.006%
75	11.243	3162	3173	3191	rBV	660179	1044394	61.02%	8.203%
76	11.615	3276	3289	3309	rBV	647363	1044580	61.03%	8.205%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028838.D
 Acq On : 02 Nov 2022 13:56
 Operator : SY/MD
 Sample : N5353-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.037	3415	3420	3425	rBV8	2183	2190	0.13%	0.017%
78	12.059	3425	3427	3428	rBV2	1601	643	0.04%	0.005%
79	12.140	3450	3452	3453	rBV2	1649	697	0.04%	0.005%
80	12.207	3470	3473	3478	rVV6	1610	1542	0.09%	0.012%
81	12.513	3563	3568	3571	rBV7	1797	1680	0.10%	0.013%
82	12.648	3606	3610	3611	rBV4	1637	1246	0.07%	0.010%
83	12.673	3615	3618	3619	rBV2	1525	667	0.04%	0.005%
84	12.686	3619	3622	3623	rBV4	1361	594	0.03%	0.005%
85	12.718	3629	3632	3633	rBV3	1106	758	0.04%	0.006%
86	12.972	3706	3711	3712	rBV4	1379	874	0.05%	0.007%
87	13.069	3737	3741	3742	rBV4	1128	737	0.04%	0.006%
88	13.101	3750	3751	3754	rVB2	1231	626	0.04%	0.005%
89	13.130	3757	3760	3761	rBV3	1759	1073	0.06%	0.008%
90	13.204	3778	3783	3784	rBV4	2016	1479	0.09%	0.012%
91	13.493	3870	3873	3876	rBV6	1504	1475	0.09%	0.012%
92	13.606	3907	3908	3913	rBV3	1343	914	0.05%	0.007%
93	13.657	3922	3924	3927	rBV4	1510	996	0.06%	0.008%
94	13.728	3943	3946	3948	rBV4	1838	862	0.05%	0.007%
95	13.873	3985	3991	3998	rBV10	2269	2406	0.14%	0.019%
96	14.094	4059	4060	4062	rBV2	1363	653	0.04%	0.005%
97	14.320	4128	4130	4132	rBV3	1864	699	0.04%	0.005%
98	14.702	4246	4249	4252	rBV5	1579	1079	0.06%	0.008%
99	14.754	4263	4265	4267	rBV3	1402	597	0.03%	0.005%
100	15.117	4375	4378	4382	rBV6	2650	2353	0.14%	0.018%




Sum of corrected areas: 12731238

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028838.D
Acq On : 02 Nov 2022 13:56
Operator : SY/MD
Sample : N5353-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

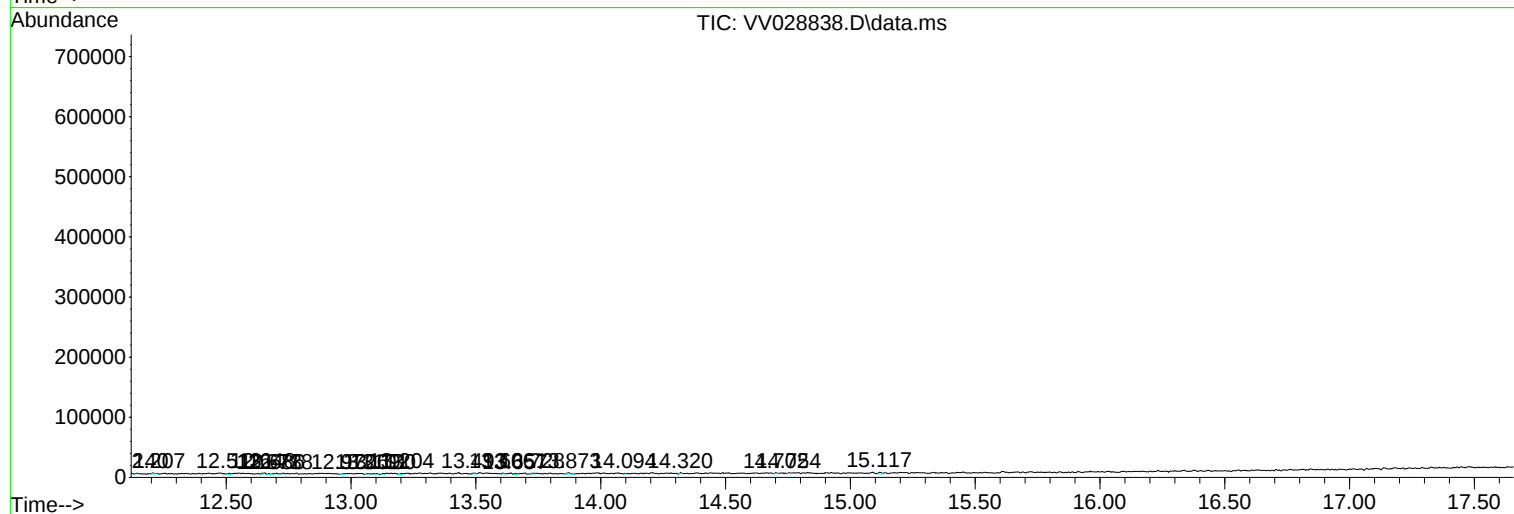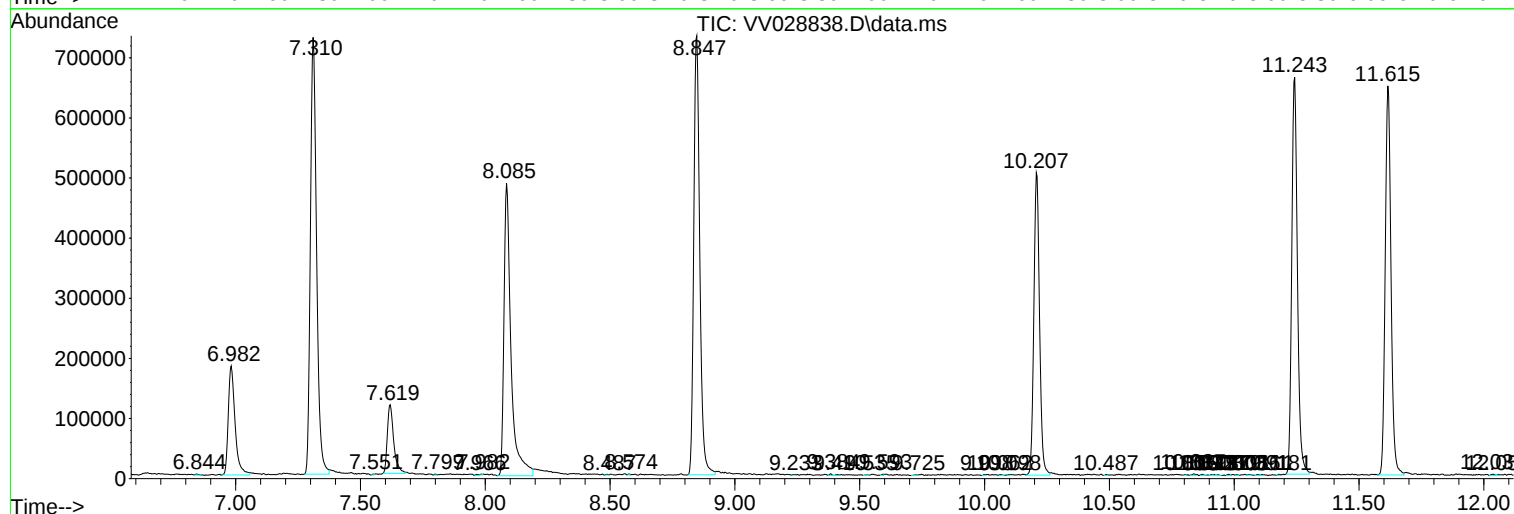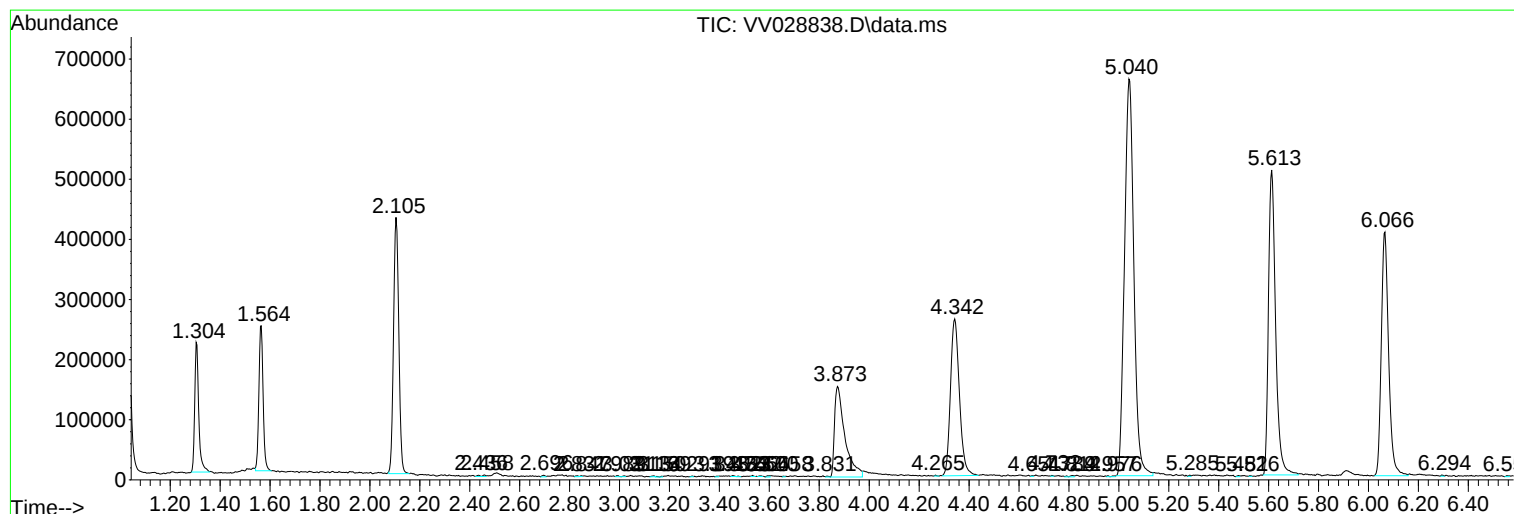

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028838.D
Acq On : 02 Nov 2022 13:56
Operator : SY/MD
Sample : N5353-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028838.D
Acq On : 02 Nov 2022 13:56
Operator : SY/MD
Sample : N5353-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc