

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028841.D
 Acq On : 02 Nov 2022 15:08
 Operator : SY/MD
 Sample : N5421-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1118

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	105	rVB	199252	222941	14.38%	1.918%
2	1.561	156	162	177	rVB	207248	246836	15.92%	2.123%
3	2.105	322	331	344	rVB	377418	534629	34.49%	4.599%
4	2.458	438	441	443	rBV3	1946	1554	0.10%	0.013%
5	2.609	486	488	490	rBV3	977	426	0.03%	0.004%
6	2.722	520	523	527	rBV5	2148	1732	0.11%	0.015%
7	2.825	552	555	556	rBV3	1390	855	0.06%	0.007%
8	2.851	562	563	565	rBV3	1265	448	0.03%	0.004%
9	2.879	570	572	573	rBV2	764	251	0.02%	0.002%
10	2.892	573	576	578	rBV4	1424	815	0.05%	0.007%
11	2.925	584	586	588	rBV3	758	469	0.03%	0.004%
12	2.979	601	603	605	rBV3	1101	413	0.03%	0.004%
13	2.992	605	607	611	rBV5	1690	1085	0.07%	0.009%
14	3.066	626	630	633	rBV5	2596	1941	0.13%	0.017%
15	3.150	654	656	660	rBV5	1533	842	0.05%	0.007%
16	3.214	672	676	678	rBV5	1365	1006	0.06%	0.009%
17	3.323	705	710	712	rBV5	1373	1401	0.09%	0.012%
18	3.474	754	757	758	rBV3	825	475	0.03%	0.004%
19	3.625	802	804	808	rVB5	1488	981	0.06%	0.008%
20	3.651	808	812	815	rBV5	1469	1271	0.08%	0.011%
21	3.738	836	839	840	rBV3	1266	618	0.04%	0.005%
22	3.793	854	856	859	rBV4	2472	1675	0.11%	0.014%
23	3.828	866	867	868	rBV	1274	391	0.03%	0.003%
24	3.873	872	881	912	rBV	136421	390768	25.21%	3.361%
25	4.342	1014	1027	1054	rVB2	239274	586208	37.81%	5.043%
26	4.725	1144	1146	1147	rBV2	687	236	0.02%	0.002%
27	4.789	1165	1166	1170	rBV4	1349	812	0.05%	0.007%
28	4.883	1194	1195	1199	rBV4	1023	585	0.04%	0.005%
29	4.905	1199	1202	1208	rVB8	1419	1452	0.09%	0.012%
30	4.934	1209	1211	1214	rVB4	1867	996	0.06%	0.009%
31	4.953	1215	1217	1220	rVB4	1793	1045	0.07%	0.009%
32	4.973	1221	1223	1224	rBV2	602	212	0.01%	0.002%
33	5.040	1228	1244	1275	rBV2	595494	1550236	100.00%	13.335%
34	5.339	1333	1337	1338	rBV4	1680	1315	0.08%	0.011%
35	5.539	1396	1399	1402	rVB5	1401	1092	0.07%	0.009%
36	5.612	1410	1422	1453	rBV	483311	984999	63.54%	8.473%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028841.D
 Acq On : 02 Nov 2022 15:08
 Operator : SY/MD
 Sample : N5421-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1118

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.066	1551	1563	1582	rBV	360942	725242	46.78%	6.239%
38	6.423	1673	1674	1677	rBV3	1518	1030	0.07%	0.009%
39	6.780	1783	1785	1787	rBV3	1250	516	0.03%	0.004%
40	6.866	1809	1812	1817	rVB7	2507	1860	0.12%	0.016%
41	6.982	1839	1848	1871	rBV	160456	292980	18.90%	2.520%
42	7.310	1939	1950	1977	rBV	646241	1120615	72.29%	9.639%
43	7.619	2037	2046	2065	rBV	103940	186985	12.06%	1.608%
44	7.854	2115	2119	2120	rBV3	1615	1079	0.07%	0.009%
45	7.889	2128	2130	2134	rVB4	2336	1439	0.09%	0.012%
46	7.928	2134	2142	2144	rBV9	5494	6946	0.45%	0.060%
47	7.976	2154	2157	2166	rVB10	2066	2323	0.15%	0.020%
48	8.011	2166	2168	2169	rBV2	1133	538	0.03%	0.005%
49	8.085	2181	2191	2222	rBV	427856	858342	55.37%	7.383%
50	8.583	2344	2346	2347	rVB2	1280	318	0.02%	0.003%
51	8.738	2392	2394	2395	rBV2	1139	342	0.02%	0.003%
52	8.799	2412	2413	2415	rBV2	1372	405	0.03%	0.003%
53	8.847	2415	2428	2452	rBV	697636	1160922	74.89%	9.986%
54	9.053	2489	2492	2493	rBV3	1858	882	0.06%	0.008%
55	9.320	2571	2575	2578	rBV5	1709	1514	0.10%	0.013%
56	9.432	2608	2610	2612	rBV	1240	364	0.02%	0.003%
57	9.509	2631	2634	2637	rBV4	1711	1081	0.07%	0.009%
58	9.526	2637	2639	2640	rBV2	868	306	0.02%	0.003%
59	9.577	2653	2655	2657	rBV2	1016	645	0.04%	0.006%
60	9.989	2780	2783	2785	rBV4	2265	1436	0.09%	0.012%
61	10.159	2834	2836	2838	rBV2	1833	956	0.06%	0.008%
62	10.207	2838	2851	2875	rVV	457922	739783	47.72%	6.364%
63	10.619	2972	2979	2980	rBV9	1892	1883	0.12%	0.016%
64	10.664	2991	2993	2994	rBV	1673	812	0.05%	0.007%
65	10.763	3020	3024	3026	rBV4	1106	815	0.05%	0.007%
66	10.812	3037	3039	3042	rBV4	1244	692	0.04%	0.006%
67	10.853	3049	3052	3060	rVB10	1909	2277	0.15%	0.020%
68	10.886	3060	3062	3063	rBV2	1196	545	0.04%	0.005%
69	10.931	3073	3076	3078	rBV4	1536	895	0.06%	0.008%
70	10.976	3088	3090	3091	rBV2	868	416	0.03%	0.004%
71	11.011	3100	3101	3102	rBV	871	328	0.02%	0.003%
72	11.053	3110	3114	3120	rBV8	1034	1568	0.10%	0.013%
73	11.079	3120	3122	3125	rVV4	1273	771	0.05%	0.007%
74	11.242	3162	3173	3199	rBV	637424	1005282	64.85%	8.647%
75	11.615	3278	3289	3308	rBV	598094	932601	60.16%	8.022%
76	11.918	3381	3383	3385	rBV2	926	547	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028841.D
 Acq On : 02 Nov 2022 15:08
 Operator : SY/MD
 Sample : N5421-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1118

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	11.976	3399	3401	3403	rBV3	1595	703	0.05%	0.006%
78	12.149	3451	3455	3458	rBV5	1748	1867	0.12%	0.016%
79	12.194	3465	3469	3471	rBV4	1741	1224	0.08%	0.011%
80	12.246	3478	3485	3486	rBV6	2064	1976	0.13%	0.017%
81	12.287	3495	3498	3501	rVB4	2614	1758	0.11%	0.015%
82	12.310	3501	3505	3507	rBV4	1928	1078	0.07%	0.009%
83	12.400	3531	3533	3534	rBV2	1552	692	0.04%	0.006%
84	12.435	3543	3544	3546	rBV2	1107	545	0.04%	0.005%
85	12.551	3576	3580	3582	rBV4	1720	1344	0.09%	0.012%
86	12.767	3645	3647	3650	rVB4	2320	1382	0.09%	0.012%
87	12.789	3652	3654	3657	rVB4	1261	625	0.04%	0.005%
88	12.812	3657	3661	3663	rBV4	2319	1893	0.12%	0.016%
89	12.969	3708	3710	3712	rBV2	1067	496	0.03%	0.004%
90	12.985	3713	3715	3717	rBV3	976	430	0.03%	0.004%
91	13.040	3730	3732	3735	rBV4	1237	638	0.04%	0.005%
92	13.185	3775	3777	3778	rBV2	1128	462	0.03%	0.004%
93	13.213	3784	3786	3788	rBV3	1273	828	0.05%	0.007%
94	13.487	3869	3871	3876	rBV5	1504	1269	0.08%	0.011%
95	13.918	4004	4005	4009	rVB4	1108	478	0.03%	0.004%
96	13.934	4009	4010	4012	rBV3	1224	663	0.04%	0.006%
97	14.062	4048	4050	4051	rBV2	864	272	0.02%	0.002%
98	14.239	4103	4105	4109	rVB4	1652	732	0.05%	0.006%
99	14.972	4330	4333	4334	rBV2	1705	1129	0.07%	0.010%
100	15.300	4432	4435	4438	rBV5	1853	1469	0.09%	0.013%




Sum of corrected areas: 11625245

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028841.D
Acq On : 02 Nov 2022 15:08
Operator : SY/MD
Sample : N5421-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

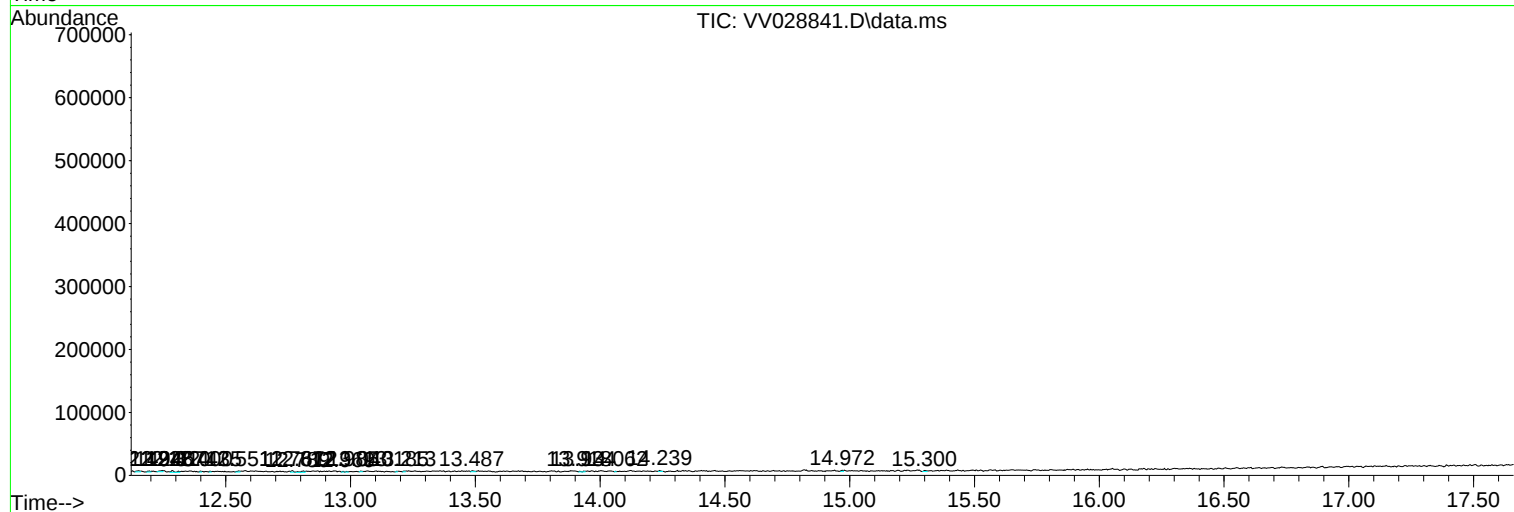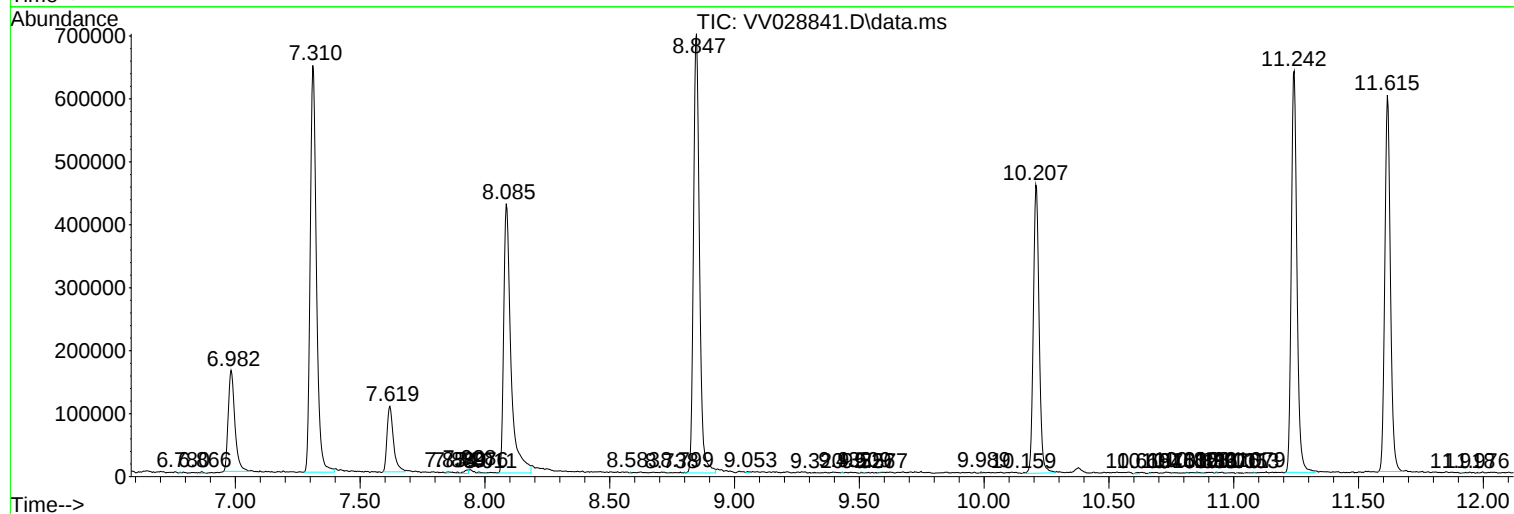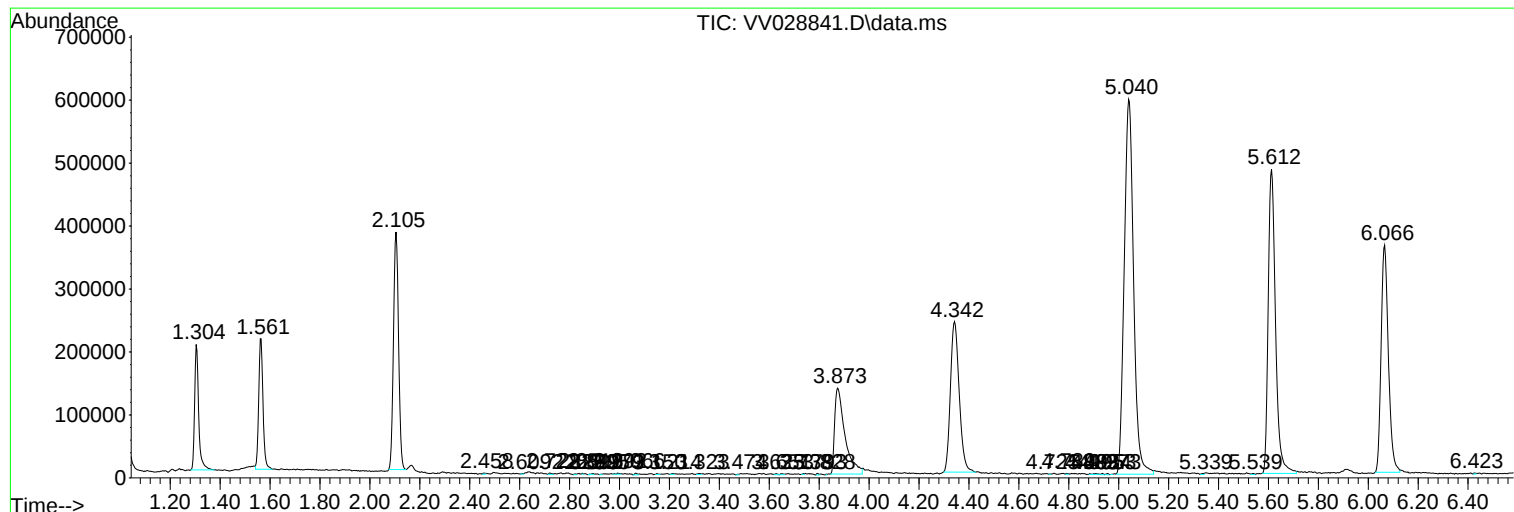

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028841.D
Acq On : 02 Nov 2022 15:08
Operator : SY/MD
Sample : N5421-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028841.D
Acq On : 02 Nov 2022 15:08
Operator : SY/MD
Sample : N5421-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------