

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028843.D
 Acq On : 02 Nov 2022 15:57
 Operator : SY/MD
 Sample : N5421-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M

Title : VOC Analysis

Signal : TIC: VV028843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	189173	208455	13.73%	1.796%
2	1.561	156	162	179	rVB	213168	247393	16.29%	2.132%
3	2.105	322	331	348	rVB	363664	523452	34.48%	4.511%
4	2.503	447	455	463	rBV5	7346	12476	0.82%	0.108%
5	2.574	475	477	478	rBV2	1247	490	0.03%	0.004%
6	2.712	517	520	521	rBV3	823	455	0.03%	0.004%
7	3.002	607	610	614	rBV4	1667	1324	0.09%	0.011%
8	3.323	707	710	716	rBV7	1550	1378	0.09%	0.012%
9	3.381	726	728	732	rBV5	1102	742	0.05%	0.006%
10	3.455	747	751	755	rBV7	1143	947	0.06%	0.008%
11	3.580	787	790	792	rBV4	1106	778	0.05%	0.007%
12	3.603	795	797	802	rVB6	1368	917	0.06%	0.008%
13	3.625	802	804	805	rBV2	1607	657	0.04%	0.006%
14	3.709	828	830	831	rBV2	1229	462	0.03%	0.004%
15	3.873	872	881	908	rBV	148746	411180	27.08%	3.544%
16	4.342	1014	1027	1052	rVB	230152	565340	37.23%	4.872%
17	4.748	1149	1153	1155	rBV4	2301	1836	0.12%	0.016%
18	4.831	1177	1179	1182	rBV4	2529	1989	0.13%	0.017%
19	4.921	1205	1207	1215	rBV9	1437	1342	0.09%	0.012%
20	5.040	1227	1244	1272	rBV2	572662	1518328	100.00%	13.085%
21	5.471	1376	1378	1380	rVB3	2119	953	0.06%	0.008%
22	5.555	1402	1404	1406	rBV3	1623	677	0.04%	0.006%
23	5.613	1411	1422	1444	rBV	477836	962129	63.37%	8.292%
24	6.066	1550	1563	1582	rBV	355252	724919	47.74%	6.247%
25	6.825	1796	1799	1801	rBV3	1958	1339	0.09%	0.012%
26	6.982	1838	1848	1871	rBV	159060	295205	19.44%	2.544%
27	7.310	1939	1950	1979	rBV	620888	1103605	72.69%	9.511%
28	7.619	2037	2046	2065	rBV2	102704	186568	12.29%	1.608%
29	8.085	2182	2191	2235	rBV	464891	937669	61.76%	8.081%
30	8.529	2326	2329	2331	rBV3	1702	1132	0.07%	0.010%
31	8.770	2402	2404	2409	rVB6	1986	1287	0.08%	0.011%
32	8.792	2409	2411	2415	rBV5	1956	1590	0.10%	0.014%
33	8.847	2417	2428	2449	rBV	705325	1160506	76.43%	10.001%
34	9.172	2527	2529	2530	rBV2	977	327	0.02%	0.003%
35	9.310	2570	2572	2575	rBV3	1512	785	0.05%	0.007%
36	9.481	2623	2625	2628	rBV4	1349	929	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028843.D
 Acq On : 02 Nov 2022 15:57
 Operator : SY/MD
 Sample : N5421-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	9.770	2711	2715	2717	rBV5	1725	1191	0.08%	0.010%
38	9.889	2747	2752	2755	rBV6	2206	2104	0.14%	0.018%
39	9.953	2769	2772	2773	rBV3	1251	660	0.04%	0.006%
40	10.111	2819	2821	2822	rBV2	1207	565	0.04%	0.005%
41	10.143	2829	2831	2835	rVB5	2078	1068	0.07%	0.009%
42	10.207	2840	2851	2870	rBV	457548	740107	48.74%	6.378%
43	10.329	2886	2889	2891	rBV4	2256	1523	0.10%	0.013%
44	10.384	2904	2906	2908	rBV3	1434	560	0.04%	0.005%
45	10.400	2908	2911	2914	rBV5	1585	1156	0.08%	0.010%
46	10.484	2935	2937	2939	rBV3	1120	671	0.04%	0.006%
47	10.625	2979	2981	2984	rVB4	2566	1478	0.10%	0.013%
48	10.641	2984	2986	2988	rBV3	789	378	0.02%	0.003%
49	10.670	2992	2995	2997	rBV3	844	579	0.04%	0.005%
50	10.683	2997	2999	3000	rBV	718	342	0.02%	0.003%
51	10.747	3017	3019	3021	rBV3	1387	632	0.04%	0.005%
52	10.786	3029	3031	3034	rBV4	1692	1201	0.08%	0.010%
53	10.831	3041	3045	3046	rBV3	1347	909	0.06%	0.008%
54	10.911	3067	3070	3071	rBV3	1767	868	0.06%	0.007%
55	11.056	3113	3115	3118	rBV4	976	527	0.03%	0.005%
56	11.072	3118	3120	3121	rBV2	608	171	0.01%	0.001%
57	11.082	3121	3123	3124	rBV2	1195	438	0.03%	0.004%
58	11.143	3138	3142	3143	rBV4	1256	956	0.06%	0.008%
59	11.169	3149	3150	3151	rBV	989	357	0.02%	0.003%
60	11.243	3162	3173	3193	rBV	633358	1010482	66.55%	8.708%
61	11.522	3258	3260	3262	rVB3	1898	738	0.05%	0.006%
62	11.615	3278	3289	3310	rBV	577164	933246	61.47%	8.043%
63	11.898	3375	3377	3380	rBV4	2087	1326	0.09%	0.011%
64	12.062	3426	3428	3433	rBV6	1613	864	0.06%	0.007%
65	12.114	3440	3444	3446	rBV4	1828	1362	0.09%	0.012%
66	12.178	3462	3464	3466	rBV3	1319	820	0.05%	0.007%
67	12.304	3496	3503	3505	rBV7	2424	2660	0.18%	0.023%
68	12.413	3534	3537	3543	rBV6	2520	2710	0.18%	0.023%
69	12.628	3601	3604	3605	rBV3	850	351	0.02%	0.003%
70	12.725	3632	3634	3635	rBV3	893	291	0.02%	0.003%
71	12.818	3661	3663	3665	rBV3	1541	683	0.04%	0.006%
72	12.918	3692	3694	3697	rBV4	1138	610	0.04%	0.005%
73	13.210	3784	3785	3789	rBV3	1228	744	0.05%	0.006%
74	13.400	3842	3844	3847	rVB4	1836	792	0.05%	0.007%
75	13.416	3847	3849	3852	rBV4	2043	1274	0.08%	0.011%
76	13.699	3934	3937	3940	rBV5	1567	1173	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028843.D
 Acq On : 02 Nov 2022 15:57
 Operator : SY/MD
 Sample : N5421-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M

Title : VOC Analysis

77	13.834	3976	3979	3981	rBV4	2395	1739	0.11%	0.015%
78	13.882	3992	3994	3995	rBV2	1323	541	0.04%	0.005%
79	14.008	4030	4033	4034	rBV2	1602	902	0.06%	0.008%
80	14.072	4048	4053	4054	rBV3	1983	1733	0.11%	0.015%
81	14.464	4173	4175	4176	rBV2	1161	509	0.03%	0.004%




Sum of corrected areas: 11603552

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028843.D
Acq On : 02 Nov 2022 15:57
Operator : SY/MD
Sample : N5421-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

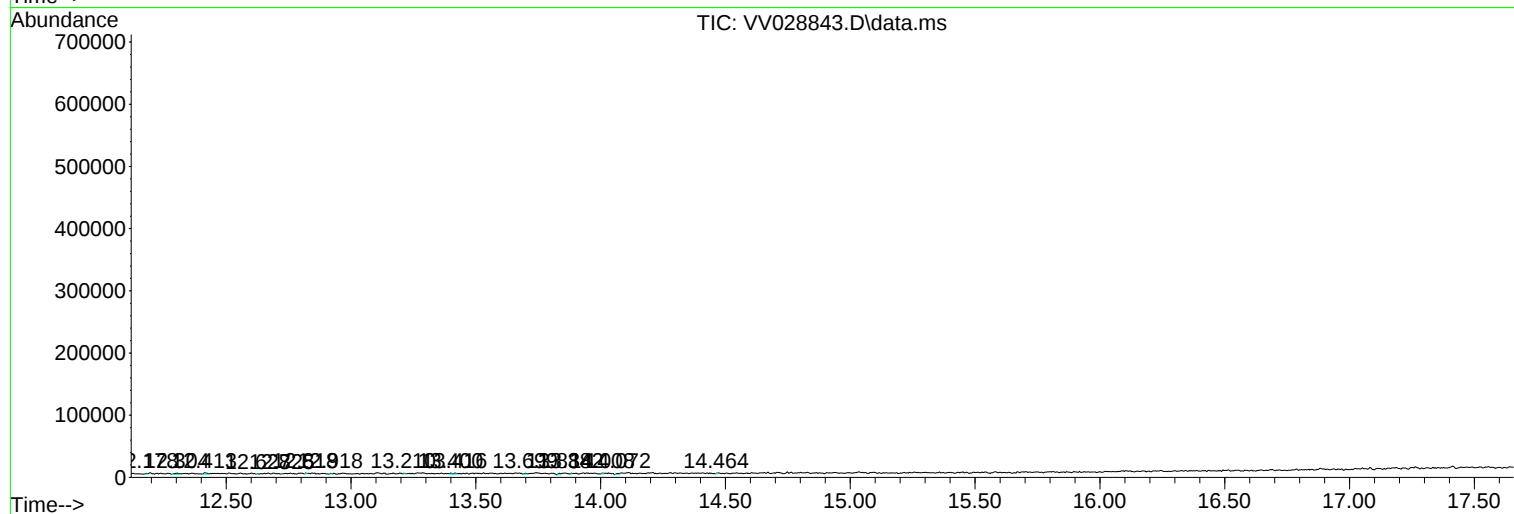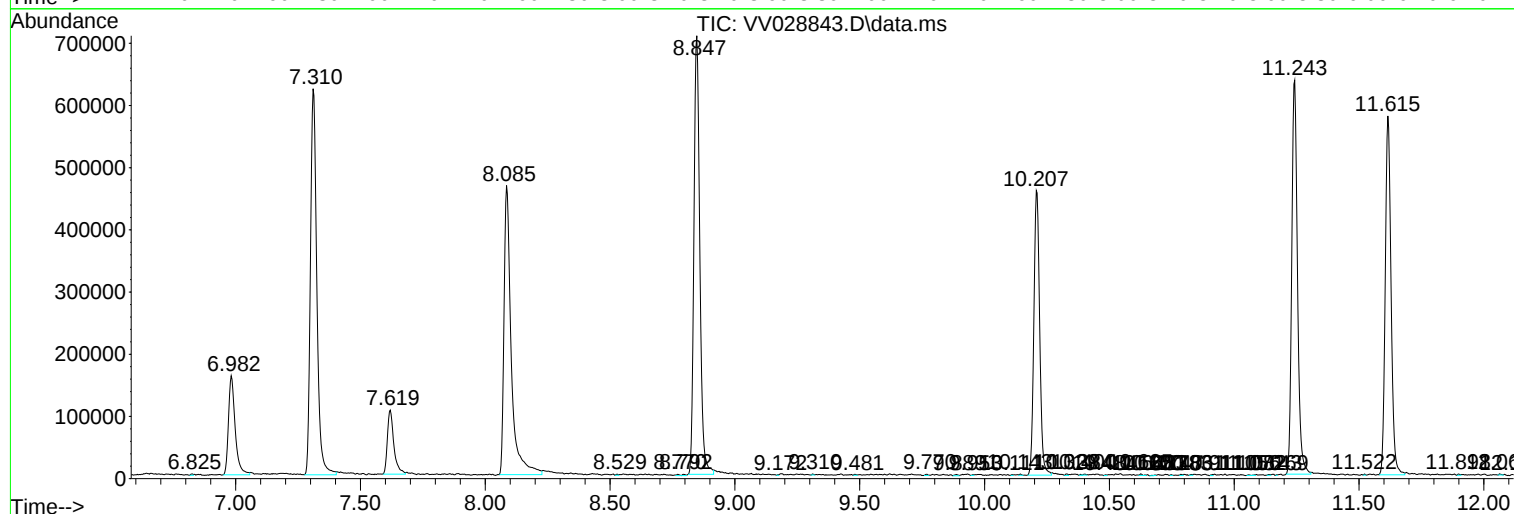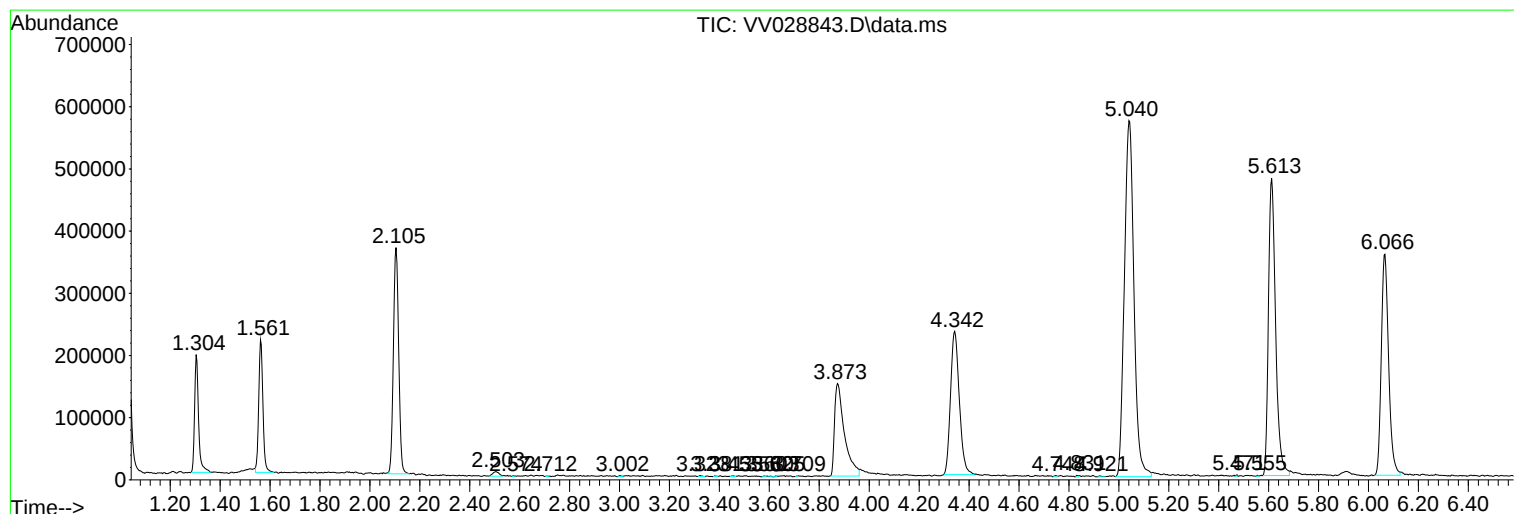

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028843.D
Acq On : 02 Nov 2022 15:57
Operator : SY/MD
Sample : N5421-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028843.D
Acq On : 02 Nov 2022 15:57
Operator : SY/MD
Sample : N5421-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc