
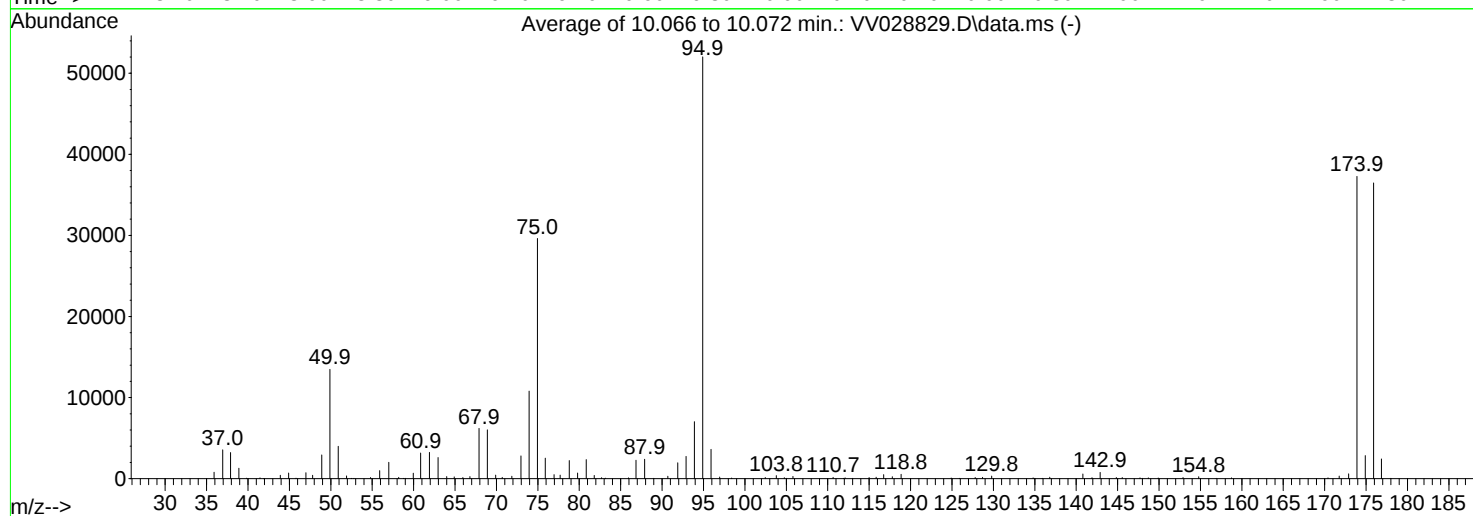


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028829.D
 Acq On : 02 Nov 2022 09:16
 Operator : SY/MD
 Sample : BFB334
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB334

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis
 Last Update : Wed Nov 02 05:10:28 2022

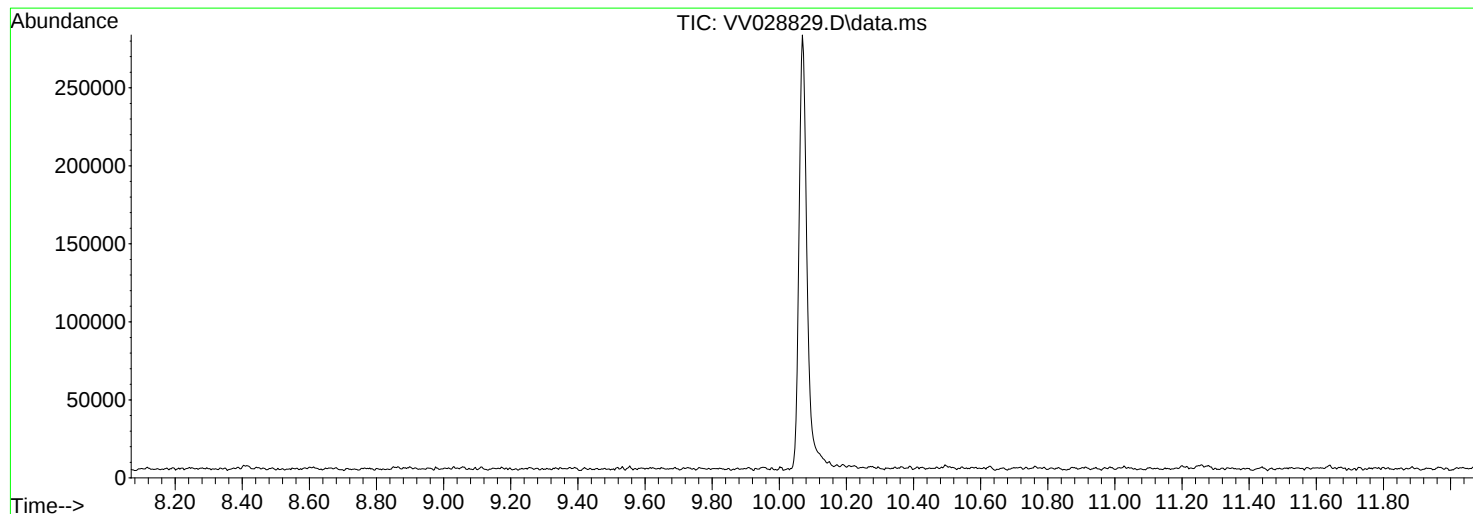

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.9	13489	PASS
75	95	30	80	57.0	29627	PASS
95	95	100	100	100.0	52021	PASS
96	95	5	9	7.0	3619	PASS
173	174	0.00	2	1.6	587	PASS
174	95	50	120	71.7	37285	PASS
175	174	5	9	7.6	2850	PASS
176	174	95	105	97.8	36472	PASS
177	176	5	10	6.6	2421	PASS

m/z	Abundance
35.50	181.0
36.20	150.0
37.80	178.0
38.40	141.0
38.90	200.0
39.90	1120.0
40.80	202.0
41.90	151.0
42.80	110.0
43.90	613.0
45.80	139.0
46.70	113.0
47.20	134.0
48.30	134.0
51.60	186.0
54.40	135.0
54.80	139.0
56.40	114.0
57.90	137.0
60.70	123.0
61.50	157.0
69.90	133.0
87.00	118.0
88.40	129.0
100.00	102.0
263.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

m/z	Abundance
35.90	740.0
37.00	3421.0
38.00	3336.0
38.90	1520.0
39.90	1220.0
40.70	166.0
42.00	163.0
43.90	1050.0
44.90	673.0
45.80	199.0
47.00	849.0
47.80	387.0
48.90	2891.0
49.90	13322.0
50.90	4348.0
51.90	362.0
52.50	141.0
54.80	308.0
55.90	979.0
57.00	1965.0
57.70	120.0
58.20	178.0
60.00	701.0
60.90	3078.0
61.90	3196.0
63.00	2604.0
64.00	247.0
64.90	184.0
66.00	136.0
66.80	266.0
67.90	5903.0
68.90	6183.0
69.90	561.0
70.70	146.0
71.90	249.0
72.90	2931.0
73.90	10424.0
74.90	28576.0
75.90	2565.0
77.00	463.0
77.70	381.0
78.80	2081.0
79.80	629.0
80.90	2312.0
81.80	327.0
82.70	142.0
83.10	104.0
86.90	2359.0
87.90	2277.0
89.00	117.0
90.70	291.0
91.90	1818.0
92.90	2665.0
93.90	7139.0
94.90	51368.0
95.90	3560.0
97.00	189.0
102.50	113.0
103.80	337.0
104.80	104.0
105.90	281.0
110.60	178.0
111.90	119.0
115.00	118.0
115.90	191.0
116.80	494.0
117.90	218.0
118.80	522.0
124.90	126.0
125.90	112.0
127.80	148.0
128.70	132.0
129.80	321.0
134.80	138.0
136.90	189.0
140.80	536.0
141.90	112.0
142.90	804.0
144.90	149.0
145.60	119.0
148.00	137.0
148.70	105.0
152.90	149.0
154.80	238.0
170.40	103.0
171.70	335.0
172.90	569.0
173.90	36184.0
174.90	2651.0
175.90	34136.0
176.80	2247.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

m/z	Abundance
35.90	800.0
36.90	3720.0
38.00	3520.0
38.90	1521.0
39.80	1208.0
40.60	172.0
41.50	116.0
41.90	144.0
43.90	1057.0
44.90	707.0
45.90	213.0
47.00	883.0
47.80	412.0
48.90	3018.0
49.90	14021.0
50.90	4058.0
51.90	339.0
54.80	284.0
55.90	993.0
57.00	2130.0
58.20	169.0
60.00	704.0
60.90	3442.0
61.90	3345.0
63.00	2673.0
64.00	257.0
64.90	238.0
66.00	153.0
66.80	290.0
67.90	6353.0
68.90	6211.0
69.90	563.0
70.70	170.0
71.80	287.0
72.90	2915.0
73.90	11144.0
74.90	30792.0
75.90	2624.0
77.00	513.0
77.70	489.0
78.80	2287.0
79.80	715.0
80.90	2458.0
81.80	379.0
82.70	135.0
83.20	102.0
86.00	149.0
86.80	2418.0
87.90	2501.0
90.70	306.0
91.90	2045.0
92.90	2880.0
93.90	7291.0
94.90	53848.0
95.90	3704.0
97.00	201.0
98.40	120.0
102.50	154.0
103.80	400.0
104.80	122.0
105.80	279.0
110.60	175.0
112.10	139.0
115.00	156.0
115.80	182.0
116.70	523.0
117.80	247.0
118.80	574.0
124.90	120.0
127.80	137.0
128.70	164.0
129.80	331.0
134.80	135.0
136.80	181.0
140.80	590.0
141.90	118.0
142.90	808.0
144.80	149.0
145.60	131.0
147.70	153.0
148.70	107.0
149.90	122.0
152.90	142.0
154.80	278.0
158.70	129.0
170.40	115.0
171.70	333.0
172.90	598.0
173.90	38488.0
174.90	2953.0
175.90	37952.0
176.90	2498.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

m/z	Abundance
35.90	842.0
36.90	3531.0
37.90	3312.0
38.90	1425.0
39.80	1103.0
41.40	154.0
41.80	161.0
43.90	1008.0
44.90	674.0
45.90	195.0
47.00	873.0
47.80	429.0
48.90	2861.0
49.90	13125.0
50.90	3529.0
51.90	289.0
52.80	101.0
54.80	240.0
55.90	1004.0
57.00	1946.0
58.20	150.0
58.80	108.0
59.00	105.0
59.90	613.0
60.90	3347.0
61.90	3180.0
62.90	2532.0
64.00	272.0
64.90	222.0
65.90	145.0
66.80	231.0
67.90	6312.0
68.90	5641.0
69.90	558.0
70.70	159.0
71.80	336.0
73.00	2552.0
74.00	10845.0
75.00	29512.0
75.90	2395.0
76.90	518.0
77.70	451.0
78.80	2350.0
79.80	721.0
80.80	2266.0
81.80	458.0
82.70	100.0
85.90	127.0
86.80	2379.0
87.90	2395.0
90.70	313.0
91.90	2011.0
92.90	2714.0
93.90	6636.0
94.90	50848.0
95.90	3594.0
96.90	201.0
98.40	131.0
102.40	143.0
103.80	381.0
104.60	112.0
105.00	113.0
105.70	254.0
110.70	149.0
112.10	146.0
113.00	116.0
115.00	150.0
115.80	190.0
116.80	449.0
117.70	267.0
118.90	506.0
127.80	137.0
128.70	178.0
129.80	274.0
135.00	130.0
135.90	103.0
136.70	158.0
140.80	620.0
141.90	131.0
142.90	701.0
144.80	105.0
145.50	141.0
147.70	167.0
148.70	108.0
149.90	133.0
152.90	130.0
154.80	224.0
156.90	133.0
158.80	161.0
170.40	104.0
171.80	281.0
172.90	593.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

173.90	37184.0
174.90	2947.0
175.90	37328.0
176.90	2517.0
178.00	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334