

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110223\
 Data File : VV032828.D
 Acq On : 01 Nov 2023 16:58
 Operator : SY/MD
 Sample : VIBLK327
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK327

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	18	23	33	rVB	8906	12812	2.65%	0.293%
2	1.278	67	74	83	rBV	61002	64149	13.25%	1.465%
3	1.532	146	153	166	rVV	66193	77965	16.10%	1.781%
4	2.060	308	317	329	rBV	109798	161412	33.33%	3.687%
5	2.179	347	354	367	rVB3	13602	25412	5.25%	0.580%
6	2.445	433	437	450	rVB7	7064	11482	2.37%	0.262%
7	3.802	848	859	887	rBV2	66156	220869	45.61%	5.045%
8	4.252	977	999	1022	rBV4	89296	282202	58.27%	6.446%
9	4.368	1026	1035	1040	rBV3	7896	15913	3.29%	0.363%
10	4.957	1202	1218	1237	rBV3	184606	477942	98.69%	10.917%
11	5.535	1387	1398	1415	rBV	142527	298556	61.65%	6.820%
12	5.989	1528	1539	1553	rBV2	109360	224031	46.26%	5.117%
13	6.436	1669	1678	1697	rBV3	18186	41925	8.66%	0.958%
14	6.918	1816	1828	1841	rBV	45881	91786	18.95%	2.097%
15	7.246	1918	1930	1952	rBV	204513	402502	83.12%	9.194%
16	7.558	2018	2027	2047	rBV	30869	61890	12.78%	1.414%
17	7.876	2117	2126	2132	rBV4	7040	14188	2.93%	0.324%
18	8.030	2164	2174	2204	rBV	215530	484267	100.00%	11.061%
19	8.365	2267	2278	2291	rBV3	13998	30555	6.31%	0.698%
20	8.786	2398	2409	2428	rBV	235882	420103	86.75%	9.596%
21	9.088	2497	2503	2511	rVB	4470	6843	1.41%	0.156%
22	10.156	2822	2835	2850	rBV	93465	158710	32.77%	3.625%
23	10.329	2880	2889	2898	rVB4	10736	17237	3.56%	0.394%
24	11.188	3145	3156	3174	rBV	232400	372103	76.84%	8.499%
25	11.564	3257	3273	3290	rBV	218675	370701	76.55%	8.467%
26	12.197	3462	3470	3482	rVB2	8206	13862	2.86%	0.317%
27	13.204	3774	3783	3793	rBV2	10061	18547	3.83%	0.424%




Sum of corrected areas: 4377964

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110223\
Data File : VV032828.D
Acq On : 01 Nov 2023 16:58
Operator : SY/MD
Sample : VIBLK327
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

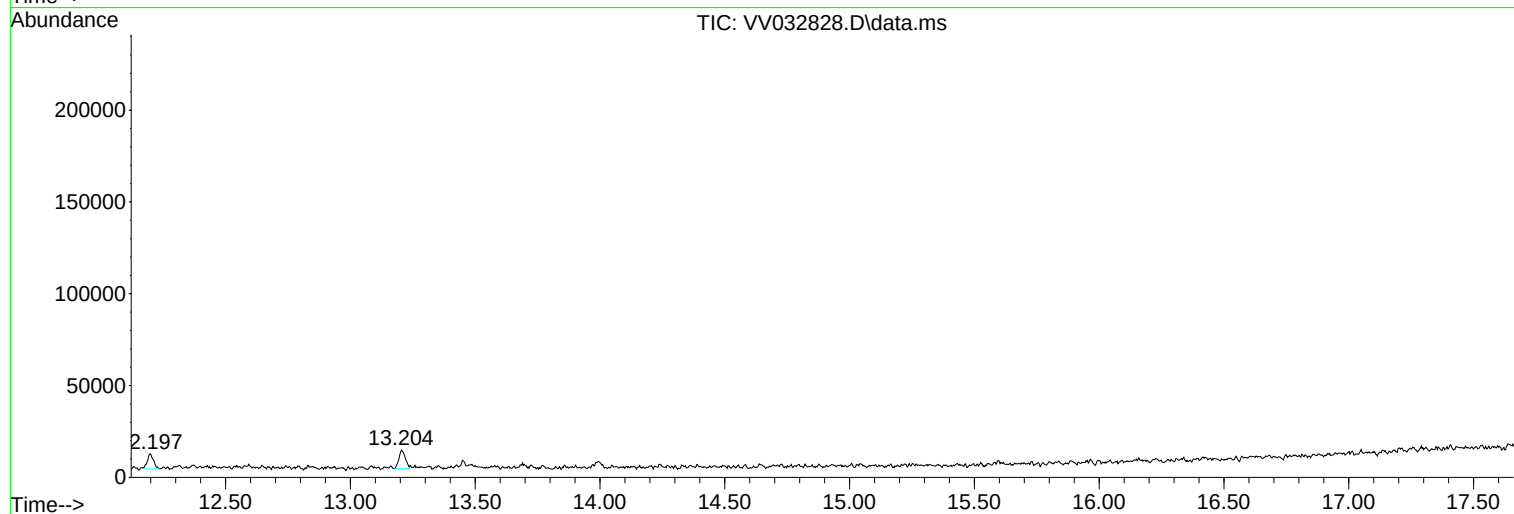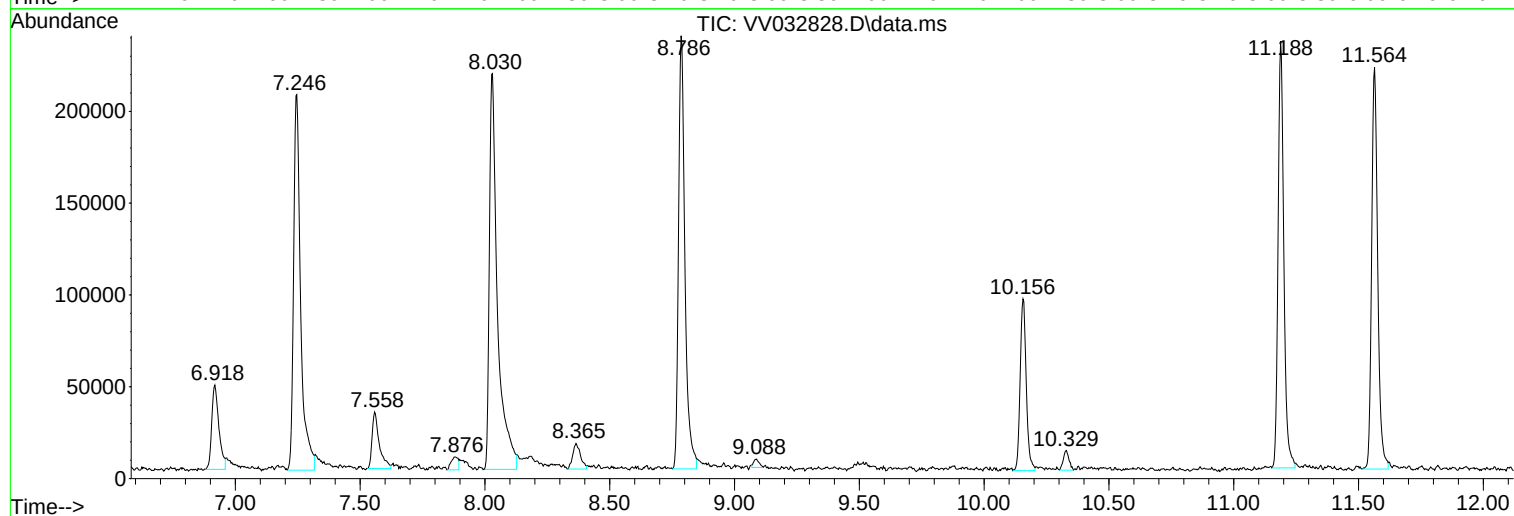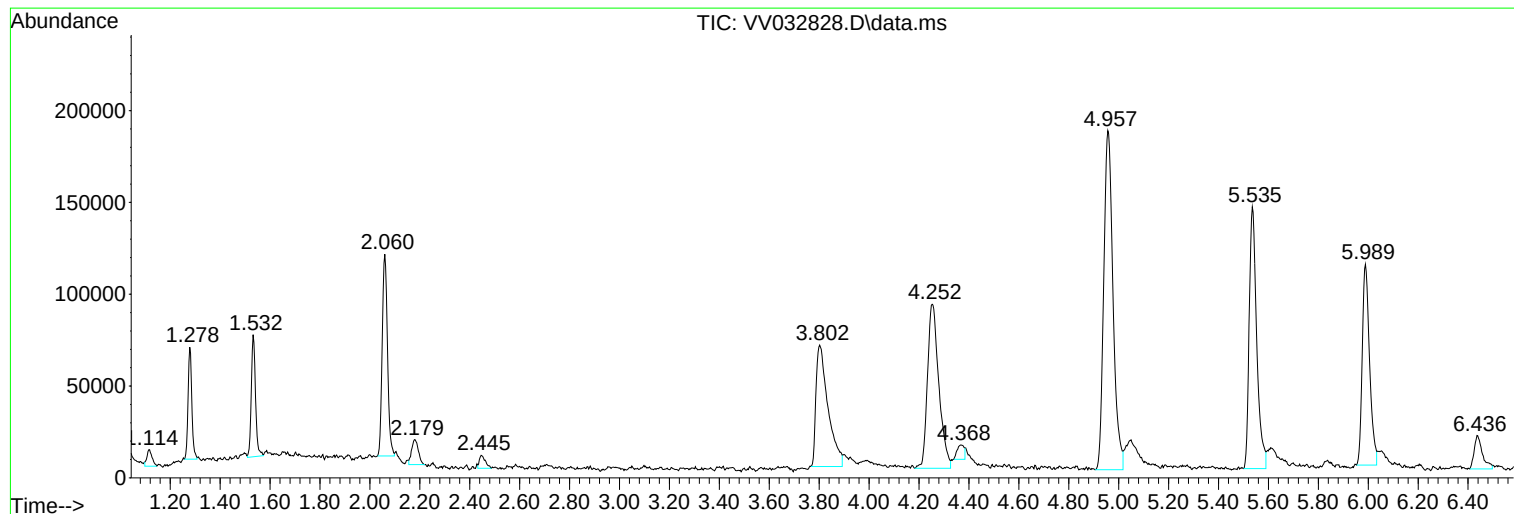

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110223\
Data File : VV032828.D
Acq On : 01 Nov 2023 16:58
Operator : SY/MD
Sample : VIBLK327
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110223\
Data File : VV032828.D
Acq On : 01 Nov 2023 16:58
Operator : SY/MD
Sample : VIBLK327
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------