


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110223\
Data File : VV032824.D
Acq On : 01 Nov 2023 14:04
Operator : SY/MD
Sample : BFB231
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB231

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 02 01:31:24 2023

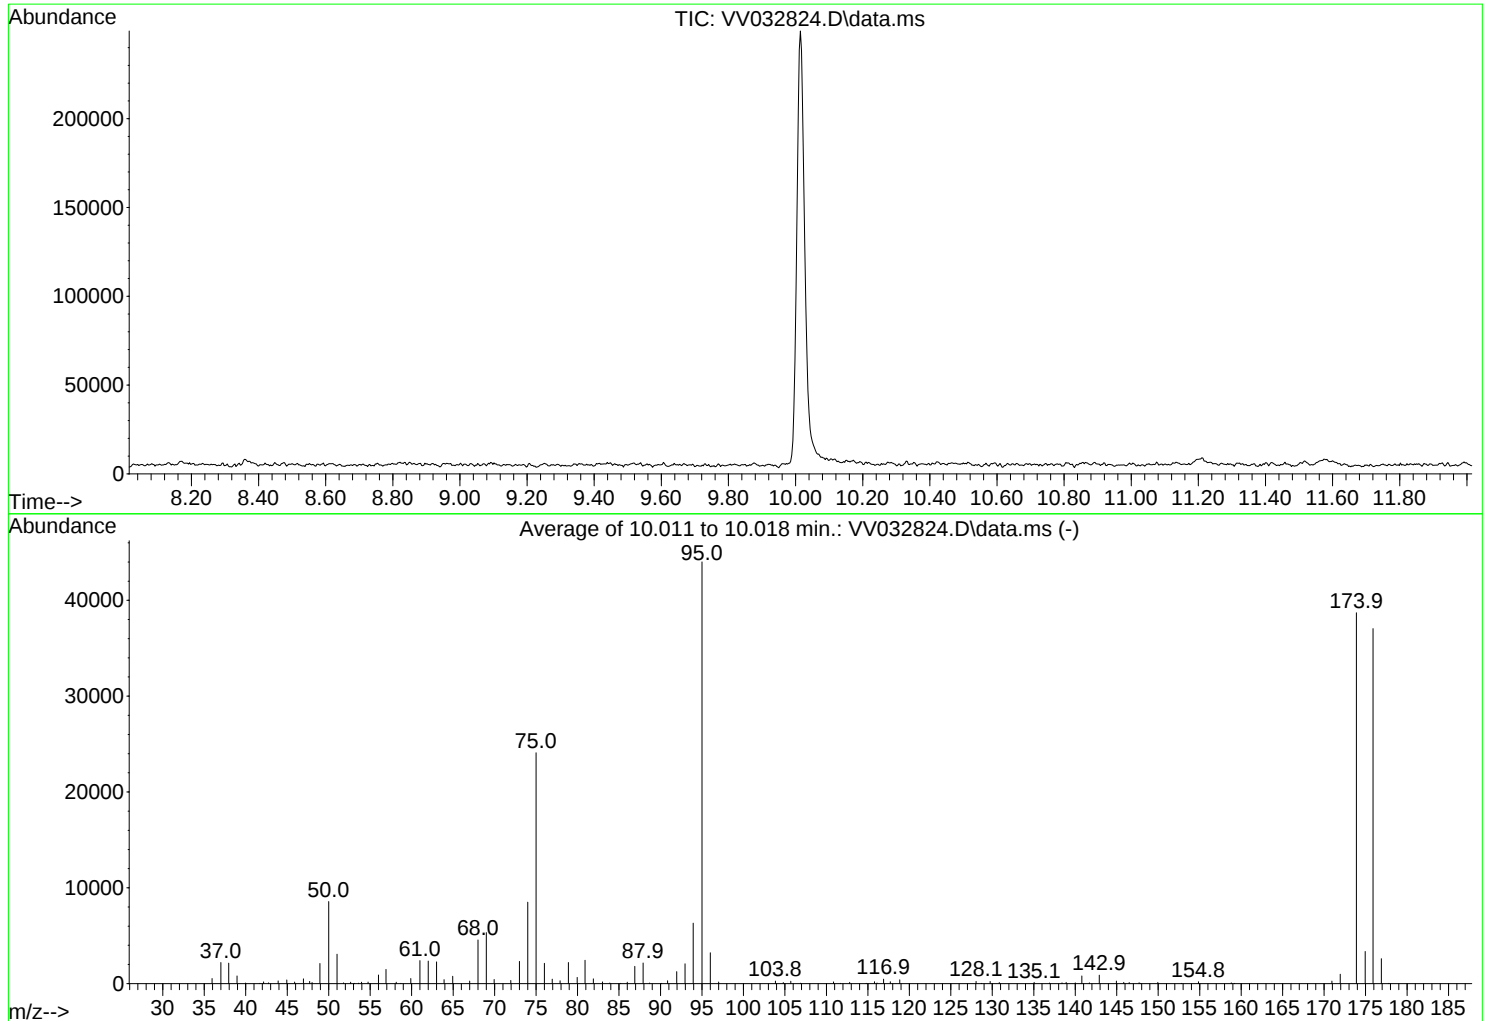

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	8574	PASS
75	95	30	80	54.8	24100	PASS
95	95	100	100	100.0	44016	PASS
96	95	5	9	7.3	3216	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.9	38704	PASS
175	174	5	9	8.7	3362	PASS
176	174	95	105	95.7	37056	PASS
177	176	5	10	7.0	2611	PASS

m/z	Abundance
35.40	108.0
36.30	120.0
37.00	178.0
37.50	147.0
38.00	170.0
38.50	143.0
39.10	245.0
40.00	337.0
41.10	202.0
41.80	143.0
43.00	130.0
43.90	453.0
44.90	115.0
45.50	120.0
47.20	145.0
47.80	153.0
51.00	151.0
52.10	148.0
55.00	103.0
56.20	154.0
57.40	120.0
59.20	117.0
60.50	102.0
61.50	114.0
66.20	116.0
68.70	144.0
70.70	106.0
75.20	113.0
77.50	114.0
80.20	105.0
81.50	107.0
91.20	123.0
91.90	116.0
93.70	121.0
103.30	117.0
106.30	120.0
110.50	116.0
137.10	108.0
188.90	110.0
217.40	111.0
221.30	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
35.90	529.0
37.00	2403.0
38.00	2219.0
39.00	928.0
40.00	396.0
41.00	102.0
41.60	188.0
42.20	227.0
44.00	765.0
45.00	516.0
45.90	131.0
47.00	470.0
47.70	373.0
48.00	375.0
49.00	2130.0
50.00	8625.0
51.00	3171.0
51.80	228.0
52.70	128.0
53.10	129.0
53.60	152.0
53.90	152.0
54.70	163.0
56.00	1045.0
56.90	1396.0
58.10	140.0
58.70	103.0
59.90	517.0
61.00	2476.0
62.00	2384.0
63.00	2320.0
63.90	475.0
65.00	777.0
66.10	201.0
67.00	266.0
68.00	4651.0
69.00	5292.0
69.90	441.0
71.90	305.0
73.00	2248.0
74.00	8476.0
75.00	24064.0
76.00	2175.0
76.90	477.0
77.90	297.0
78.90	2154.0
79.90	622.0
80.90	2146.0
81.90	551.0
83.00	159.0
85.20	104.0
86.00	140.0
86.90	1856.0
87.90	2115.0
90.10	107.0
90.90	318.0
92.00	1336.0
93.00	1989.0
93.90	6388.0
95.00	43928.0
96.00	3132.0
97.00	141.0
103.90	288.0
104.70	120.0
105.70	239.0
106.90	139.0
110.80	192.0
111.70	113.0
112.80	159.0
115.80	239.0
116.90	506.0
117.70	236.0
118.90	413.0
128.00	267.0
128.70	117.0
129.80	199.0
130.90	122.0
135.00	131.0
136.80	179.0
138.90	145.0
140.80	728.0
141.70	134.0
142.90	877.0
144.90	253.0
145.90	168.0
146.50	104.0
147.70	183.0
150.00	141.0
154.90	179.0
159.20	122.0
170.90	246.0
172.00	883.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

173.90	36896.0
174.90	3360.0
175.90	35992.0
176.90	2444.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
35.90	547.0
37.00	2520.0
38.00	2360.0
38.90	1103.0
40.00	440.0
41.60	168.0
42.20	197.0
42.80	123.0
44.00	723.0
45.00	526.0
45.90	179.0
47.00	519.0
47.70	413.0
49.00	2185.0
50.00	8868.0
51.00	3394.0
52.00	199.0
52.60	152.0
54.00	166.0
54.70	164.0
56.00	1133.0
56.90	1524.0
58.10	147.0
59.90	572.0
61.00	2495.0
62.00	2399.0
63.00	2418.0
63.90	429.0
64.90	823.0
66.10	146.0
67.00	286.0
68.00	4706.0
69.00	5481.0
70.00	438.0
72.00	349.0
73.00	2369.0
74.00	8870.0
75.00	25184.0
76.00	2105.0
76.90	495.0
77.90	304.0
78.90	2231.0
79.90	688.0
80.90	2509.0
81.90	495.0
83.00	194.0
83.90	111.0
86.00	150.0
86.90	1814.0
87.90	2260.0
88.70	107.0
90.90	295.0
92.00	1399.0
93.00	2105.0
94.00	6510.0
95.00	45016.0
96.00	3363.0
97.00	161.0
103.90	269.0
104.80	118.0
105.70	261.0
110.80	196.0
112.80	149.0
115.90	191.0
116.90	480.0
117.70	187.0
118.90	415.0
128.00	252.0
129.70	240.0
130.90	123.0
135.10	138.0
136.80	193.0
138.40	125.0
138.90	123.0
140.00	109.0
140.80	852.0
141.70	121.0
142.90	913.0
145.00	269.0
145.90	128.0
146.50	131.0
147.70	143.0
150.00	128.0
154.80	224.0
158.80	117.0
170.90	278.0
171.90	1038.0
173.90	39944.0
175.00	3472.0
175.90	38296.0
176.90	2697.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
36.00	540.0
37.00	2240.0
37.90	2349.0
38.90	1126.0
40.00	363.0
41.10	122.0
41.70	159.0
42.10	152.0
42.70	138.0
43.90	730.0
45.00	476.0
45.90	194.0
46.90	530.0
47.70	397.0
48.90	1990.0
50.00	8228.0
51.00	3095.0
52.10	197.0
52.60	161.0
54.00	140.0
54.80	173.0
56.00	982.0
56.90	1529.0
58.20	164.0
59.90	533.0
61.00	2247.0
62.00	2286.0
63.00	2094.0
63.90	373.0
64.90	708.0
67.00	235.0
68.00	4314.0
69.00	5213.0
70.00	410.0
72.00	362.0
73.00	2360.0
74.00	8174.0
75.00	23392.0
76.00	2064.0
77.00	424.0
77.90	299.0
78.90	2221.0
80.00	621.0
80.90	2638.0
81.90	456.0
83.00	204.0
83.90	100.0
86.00	172.0
86.90	1719.0
87.90	2095.0
88.70	102.0
90.80	269.0
92.00	1378.0
92.90	2118.0
94.00	6038.0
95.00	43104.0
96.00	3153.0
97.00	201.0
103.80	239.0
104.90	134.0
105.70	240.0
110.90	163.0
112.80	102.0
114.80	106.0
115.70	168.0
116.10	205.0
116.90	418.0
117.70	159.0
118.80	356.0
128.10	211.0
129.70	273.0
130.80	119.0
135.10	127.0
136.90	171.0
138.40	111.0
138.90	112.0
140.00	169.0
140.80	808.0
142.90	861.0
145.00	306.0
145.70	113.0
146.50	105.0
147.90	117.0
149.90	109.0
152.80	109.0
154.80	189.0
158.80	119.0
171.00	272.0
171.90	1038.0
173.90	39272.0
175.00	3253.0
175.90	36880.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

176.902692.0

177.80118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231