
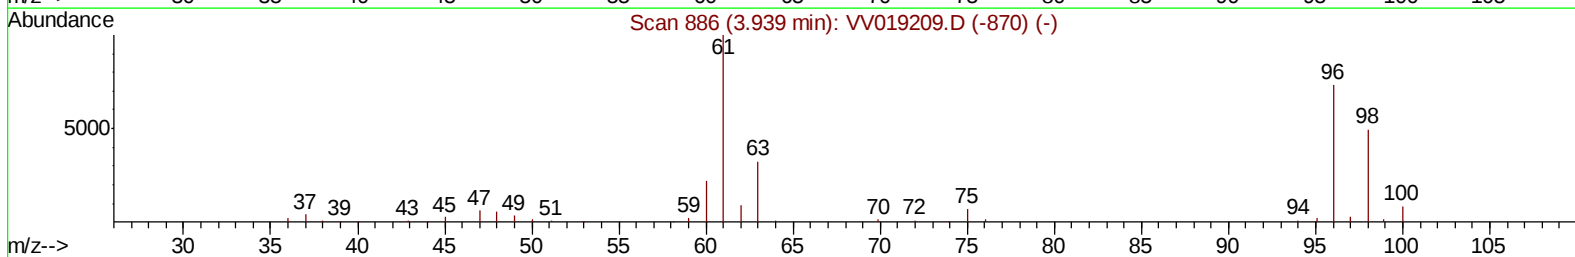
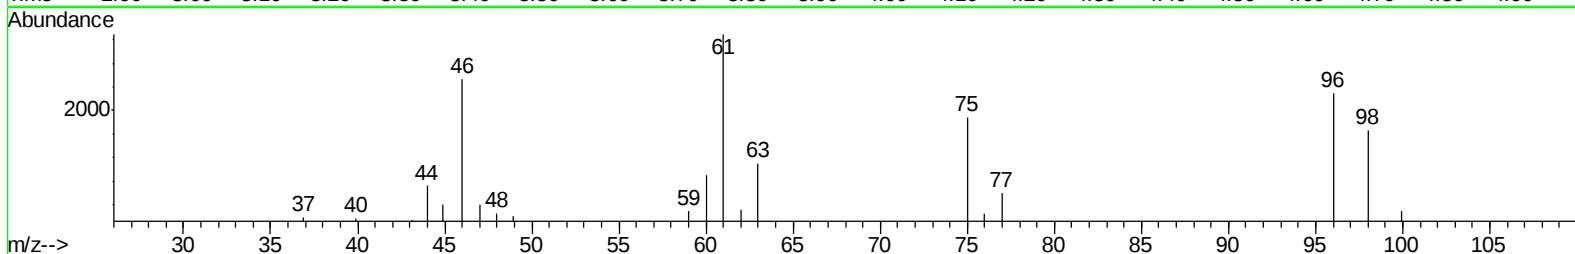


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110320\
Data File : VV019206.D
Acq On : 02 Nov 2020 17:47
Operator : SY/MD
Sample : VSTD00566
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 03 04:31:19 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 03 04:30:18 2020
Response via : Initial Calibration

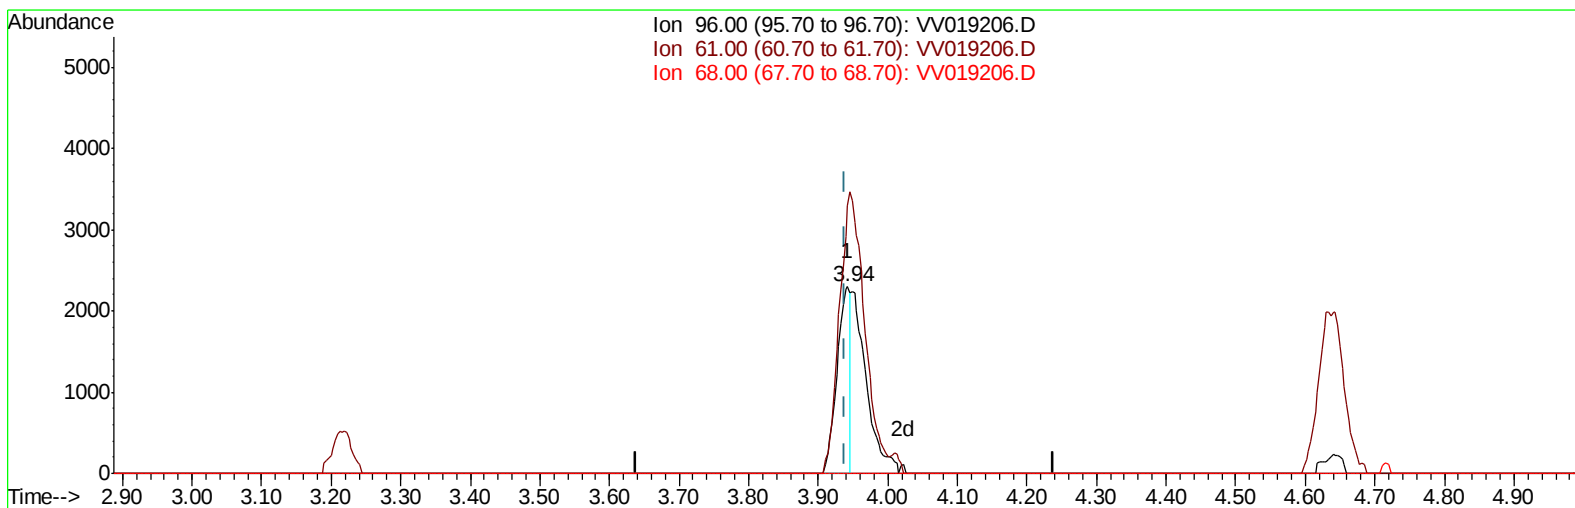

TIC: VV019206.D

(20) cis-1,2-Dichloroethene (T)

3.942min (+0.003) 1.94ug/L

response 3042

Ion	Exp%	Act%
96.00	100	100
61.00	136.60	143.29
68.00	0.00	0.00
0.00	0.00	0.00