

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110320\
 Data File : VV019218.D
 Acq On : 02 Nov 2020 23:42
 Operator : SY/MD
 Sample : VV1103MBL02
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK308

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	81	rBV	141469	143648	14.14%	1.891%
2	1.579	145	152	163	rBV	130619	146853	14.45%	1.933%
3	2.126	311	322	343	rBV	252892	383373	37.73%	5.047%
4	2.389	402	404	410	rVB2	372	237	0.02%	0.003%
5	2.460	424	426	429	rVB	257	104	0.01%	0.001%
6	2.582	459	464	468	rBV2	444	567	0.06%	0.007%
7	2.634	475	480	482	rBV	323	279	0.03%	0.004%
8	2.666	486	490	493	rBV	407	265	0.03%	0.003%
9	2.791	524	529	532	rBV	208	203	0.02%	0.003%
10	2.810	532	535	538	rVV	298	233	0.02%	0.003%
11	2.830	538	541	545	rVB	308	216	0.02%	0.003%
12	2.917	565	568	571	rVB2	222	149	0.01%	0.002%
13	3.042	605	607	608	rBV2	195	95	0.01%	0.001%
14	3.212	657	660	663	rBV	238	141	0.01%	0.002%
15	3.290	681	684	686	rBV	184	106	0.01%	0.001%
16	3.380	710	712	716	rBV2	178	133	0.01%	0.002%
17	3.482	741	744	745	rBV2	242	129	0.01%	0.002%
18	3.527	756	758	764	rVB2	285	249	0.02%	0.003%
19	3.576	770	773	776	rBV	180	143	0.01%	0.002%
20	3.630	788	790	796	rBV	225	209	0.02%	0.003%
21	3.826	849	851	856	rVB	228	123	0.01%	0.002%
22	3.849	856	858	861	rVB2	215	120	0.01%	0.002%
23	3.910	861	877	912	rBV2	68974	208398	20.51%	2.743%
24	4.376	1006	1022	1057	rBV	167923	413310	40.67%	5.441%
25	4.572	1079	1083	1084	rBV	333	207	0.02%	0.003%
26	4.630	1098	1101	1103	rBV2	302	164	0.02%	0.002%
27	4.646	1103	1106	1108	rVV2	376	194	0.02%	0.003%
28	4.740	1131	1135	1139	rBV2	446	377	0.04%	0.005%
29	4.897	1182	1184	1189	rBV	192	143	0.01%	0.002%
30	4.942	1196	1198	1203	rVB2	266	186	0.02%	0.002%
31	4.965	1203	1205	1209	rVB	269	162	0.02%	0.002%
32	4.997	1209	1215	1220	rBV	383	451	0.04%	0.006%
33	5.071	1221	1238	1268	rBV2	392056	1016164	100.00%	13.377%
34	5.341	1318	1322	1324	rBV2	514	359	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110320\
 Data File : VV019218.D
 Acq On : 02 Nov 2020 23:42
 Operator : SY/MD
 Sample : VV1103MBL02
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK308

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
 Title : VOC Analysis

35	5.453	1355	1357	1362	rVB	348	160	0.02%	0.002%
36	5.492	1363	1369	1370	rBV2	284	262	0.03%	0.003%
37	5.527	1377	1380	1384	rBV	176	145	0.01%	0.002%
38	5.550	1384	1387	1390	rVV2	234	178	0.02%	0.002%
39	5.640	1403	1415	1449	rBV	292106	580889	57.16%	7.647%
40	5.933	1496	1506	1523	rVB3	8321	16992	1.67%	0.224%
41	6.093	1541	1556	1588	rBV	223954	454464	44.72%	5.983%
42	6.235	1597	1600	1602	rBV3	550	412	0.04%	0.005%
43	6.302	1617	1621	1624	rBV2	316	270	0.03%	0.004%
44	6.347	1631	1635	1637	rBV	194	153	0.02%	0.002%
45	6.379	1643	1645	1648	rVB	220	100	0.01%	0.001%
46	6.399	1648	1651	1654	rVB2	159	134	0.01%	0.002%
47	6.441	1660	1664	1666	rBV2	317	241	0.02%	0.003%
48	6.489	1677	1679	1684	rVB2	242	149	0.01%	0.002%
49	6.511	1684	1686	1689	rBV	281	141	0.01%	0.002%
50	6.556	1697	1700	1702	rBV	255	154	0.02%	0.002%
51	6.711	1742	1748	1753	rBV2	355	444	0.04%	0.006%
52	6.759	1760	1763	1765	rBV	233	159	0.02%	0.002%
53	6.775	1765	1768	1771	rVV2	233	156	0.02%	0.002%
54	6.887	1799	1803	1805	rBV2	310	250	0.02%	0.003%
55	7.006	1830	1840	1865	rBV	135317	239163	23.54%	3.148%
56	7.338	1931	1943	1963	rBV	463160	799204	78.65%	10.521%
57	7.585	2017	2020	2023	rBV2	430	286	0.03%	0.004%
58	7.640	2027	2037	2067	rBV2	96328	169249	16.66%	2.228%
59	7.878	2109	2111	2115	rVB2	347	202	0.02%	0.003%
60	7.955	2133	2135	2137	rBV	227	139	0.01%	0.002%
61	8.106	2172	2182	2208	rBV	226066	403233	39.68%	5.308%
62	8.492	2300	2302	2306	rBV	271	171	0.02%	0.002%
63	8.592	2331	2333	2336	rBV	158	111	0.01%	0.001%
64	8.611	2336	2339	2341	rBV2	203	130	0.01%	0.002%
65	8.736	2375	2378	2384	rBV2	279	332	0.03%	0.004%
66	8.810	2396	2401	2403	rBV2	301	278	0.03%	0.004%
67	8.871	2408	2420	2444	rBV	437139	713436	70.21%	9.392%
68	9.106	2487	2493	2495	rBV2	278	251	0.02%	0.003%
69	9.116	2495	2496	2498	rBV	212	114	0.01%	0.002%
70	9.164	2504	2511	2517	rBV3	456	656	0.06%	0.009%
71	9.248	2534	2537	2540	rBV2	297	219	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110320\
 Data File : VV019218.D
 Acq On : 02 Nov 2020 23:42
 Operator : SY/MD
 Sample : VV1103MBL02
 Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK308

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
 Title : VOC Analysis

72	9.363	2569	2573	2579	rVB	311	333	0.03%	0.004%
73	9.534	2622	2626	2630	rBV2	366	371	0.04%	0.005%
74	9.572	2635	2638	2643	rVV2	320	320	0.03%	0.004%
75	9.736	2686	2689	2691	rBV2	209	175	0.02%	0.002%
76	9.807	2708	2711	2717	rBV2	318	311	0.03%	0.004%
77	9.858	2724	2727	2729	rBV	234	178	0.02%	0.002%
78	10.141	2810	2815	2817	rBV2	620	557	0.05%	0.007%
79	10.235	2832	2844	2865	rBV	287637	438555	43.16%	5.773%
80	10.489	2921	2923	2926	rBV2	255	150	0.01%	0.002%
81	10.588	2951	2954	2956	rBV	278	200	0.02%	0.003%
82	10.624	2963	2965	2967	rBV	196	115	0.01%	0.002%
83	10.778	3009	3013	3019	rVB2	347	372	0.04%	0.005%
84	10.826	3025	3028	3031	rBV	262	211	0.02%	0.003%
85	10.913	3053	3055	3058	rBV	268	197	0.02%	0.003%
86	10.971	3071	3073	3076	rBV	229	133	0.01%	0.002%
87	10.990	3076	3079	3083	rBV	356	330	0.03%	0.004%
88	11.270	3154	3166	3186	rBV	451042	689333	67.84%	9.075%
89	11.550	3250	3253	3256	rBV	214	137	0.01%	0.002%
90	11.646	3271	3283	3303	rBV	484536	760581	74.85%	10.013%
91	11.807	3330	3333	3334	rBV	268	123	0.01%	0.002%
92	11.829	3338	3340	3343	rBV2	230	143	0.01%	0.002%
93	12.116	3425	3429	3433	rVB2	469	383	0.04%	0.005%
94	12.183	3445	3450	3453	rBV	257	278	0.03%	0.004%
95	12.312	3487	3490	3493	rBV	287	170	0.02%	0.002%
96	12.347	3498	3501	3506	rBV	304	246	0.02%	0.003%
97	12.476	3538	3541	3543	rVB	356	195	0.02%	0.003%
98	12.826	3648	3650	3652	rVB	252	106	0.01%	0.001%
99	13.299	3794	3797	3806	rBV3	733	776	0.08%	0.010%
100	14.607	4199	4204	4207	rBV3	416	452	0.04%	0.006%


Sum of corrected areas: 7596148

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110320\
Data File : VV019218.D
Acq On : 02 Nov 2020 23:42
Operator : SY/MD
Sample : VV1103MBL02
Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK308

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

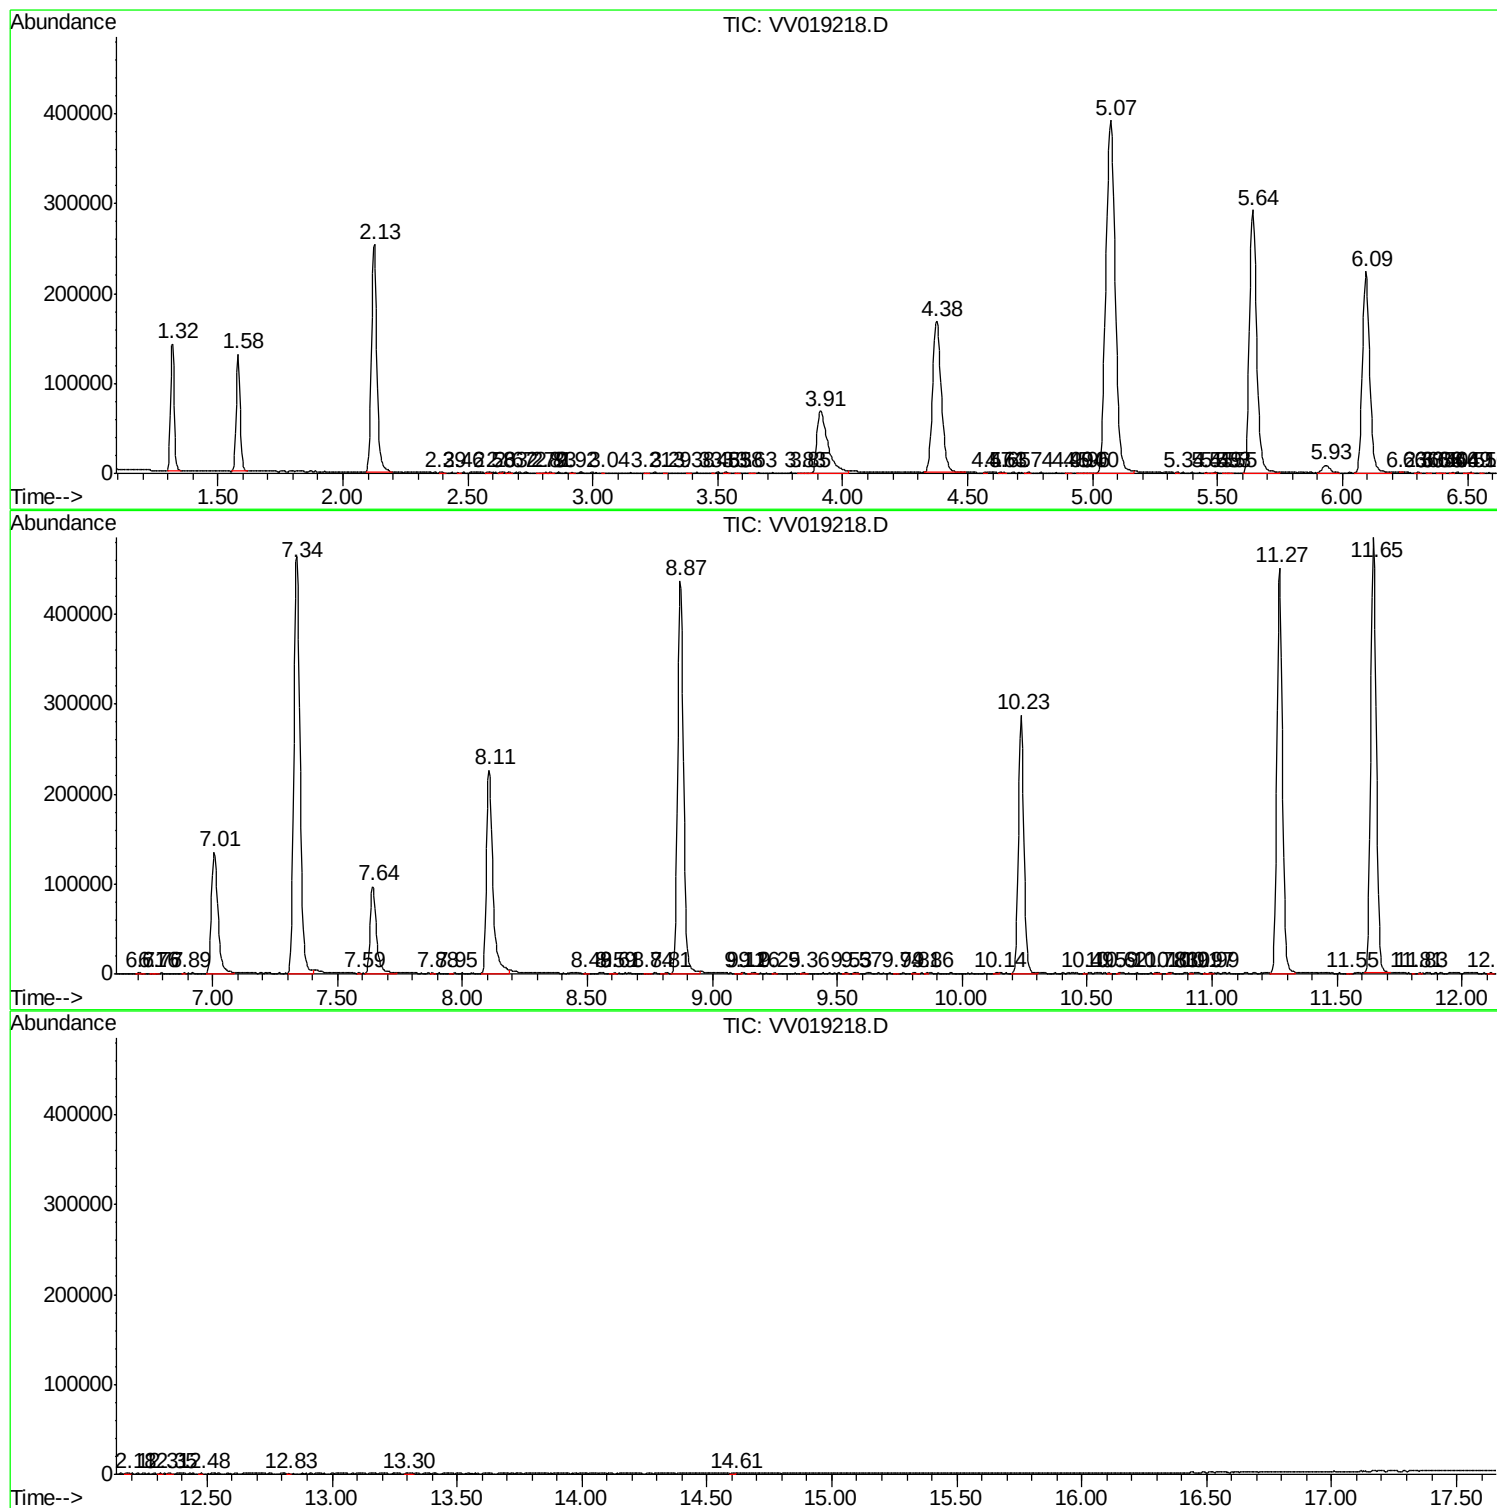

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110320\
Data File : VV019218.D
Acq On : 02 Nov 2020 23:42
Operator : SY/MD
Sample : VV1103MBL02
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK308

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110320\
Data File : VV019218.D
Acq On : 02 Nov 2020 23:42
Operator : SY/MD
Sample : VV1103MBL02
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK308

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc