

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
 Data File : VV023187.D
 Acq On : 03 Nov 2021 15:22
 Operator : SY/MD
 Sample : VV1103MBL07
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK275

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

Signal : TIC: VV023187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	108356	108876	11.29%	1.472%
2	1.568	157	164	177	rVB	97614	108569	11.26%	1.468%
3	2.047	311	313	315	rVB2	448	166	0.02%	0.002%
4	2.111	321	333	350	rBV	198716	299118	31.03%	4.044%
5	2.352	406	408	411	rBV	321	181	0.02%	0.002%
6	2.388	416	419	422	rBV2	418	291	0.03%	0.004%
7	2.568	474	475	479	rVB3	370	140	0.01%	0.002%
8	2.587	479	481	484	rBV	288	142	0.01%	0.002%
9	2.677	507	509	513	rBV2	241	135	0.01%	0.002%
10	3.224	676	679	682	rBV3	419	316	0.03%	0.004%
11	3.265	690	692	695	rBV2	298	169	0.02%	0.002%
12	3.378	723	727	728	rBV	281	137	0.01%	0.002%
13	3.423	738	741	743	rBV2	329	225	0.02%	0.003%
14	3.510	765	768	772	rBV3	213	160	0.02%	0.002%
15	3.825	862	866	869	rBV	261	202	0.02%	0.003%
16	3.844	869	872	873	rBV2	308	217	0.02%	0.003%
17	3.879	874	883	915	rBV	77756	208617	21.64%	2.820%
18	4.256	998	1000	1007	rVB2	748	552	0.06%	0.007%
19	4.352	1014	1030	1056	rBV2	160117	397053	41.18%	5.368%
20	4.754	1153	1155	1158	rBV2	268	145	0.02%	0.002%
21	4.789	1164	1166	1169	rVB	394	169	0.02%	0.002%
22	4.854	1183	1186	1191	rBV2	239	181	0.02%	0.002%
23	4.924	1206	1208	1213	rVB2	280	184	0.02%	0.002%
24	5.047	1229	1246	1274	rBV2	373606	964111	100.00%	13.035%
25	5.265	1312	1314	1319	rBV2	512	247	0.03%	0.003%
26	5.349	1336	1340	1344	rVB2	386	323	0.03%	0.004%
27	5.577	1406	1411	1412	rBV	323	273	0.03%	0.004%
28	5.619	1412	1424	1455	rVV	282357	572233	59.35%	7.736%
29	5.915	1505	1516	1532	rVB6	5781	12500	1.30%	0.169%
30	5.998	1539	1542	1545	rBV2	367	280	0.03%	0.004%
31	6.069	1551	1564	1597	rBV	217851	445105	46.17%	6.018%
32	6.375	1655	1659	1666	rBV3	366	530	0.05%	0.007%
33	6.448	1681	1682	1687	rBV	269	158	0.02%	0.002%
34	6.545	1709	1712	1715	rBV	368	245	0.03%	0.003%
35	6.571	1716	1720	1722	rBV2	231	201	0.02%	0.003%
36	6.584	1722	1724	1729	rVB	425	174	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
 Data File : VV023187.D
 Acq On : 03 Nov 2021 15:22
 Operator : SY/MD
 Sample : VV1103MBL07
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK275

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

37	6.625	1735	1737	1738	rBV	350	154	0.02%	0.002%
38	6.776	1780	1784	1785	rBV	266	157	0.02%	0.002%
39	6.815	1793	1796	1800	rBV	466	369	0.04%	0.005%
40	6.879	1814	1816	1821	rVB	453	290	0.03%	0.004%
41	6.989	1838	1850	1876	rBV	118217	216675	22.47%	2.929%
42	7.159	1901	1903	1907	rBV4	347	260	0.03%	0.004%
43	7.317	1941	1952	1972	rBV	434945	756817	78.50%	10.232%
44	7.622	2038	2047	2070	rBV	86094	150175	15.58%	2.030%
45	8.011	2163	2168	2169	rBV	271	245	0.03%	0.003%
46	8.088	2182	2192	2212	rBV	270502	462026	47.92%	6.246%
47	8.362	2274	2277	2280	rVB3	564	348	0.04%	0.005%
48	8.394	2284	2287	2289	rBV2	412	266	0.03%	0.004%
49	8.510	2322	2323	2326	rBV	328	159	0.02%	0.002%
50	8.538	2330	2332	2335	rBV2	418	237	0.02%	0.003%
51	8.561	2337	2339	2342	rVB2	327	152	0.02%	0.002%
52	8.799	2408	2413	2415	rBV2	312	324	0.03%	0.004%
53	8.854	2418	2430	2463	rVV	439741	718354	74.51%	9.712%
54	9.249	2550	2553	2557	rVB2	251	171	0.02%	0.002%
55	9.413	2600	2604	2606	rBV2	337	284	0.03%	0.004%
56	9.564	2647	2651	2655	rVB2	532	363	0.04%	0.005%
57	9.770	2713	2715	2719	rBV2	263	171	0.02%	0.002%
58	9.834	2732	2735	2736	rBV	234	128	0.01%	0.002%
59	9.937	2765	2767	2772	rVB	345	233	0.02%	0.003%
60	10.008	2786	2789	2792	rBV2	153	144	0.01%	0.002%
61	10.059	2802	2805	2807	rBV	280	132	0.01%	0.002%
62	10.127	2819	2826	2834	rBV6	2162	2940	0.30%	0.040%
63	10.217	2842	2854	2875	rBV	316437	496009	51.45%	6.706%
64	10.381	2901	2905	2906	rBV	652	396	0.04%	0.005%
65	10.545	2953	2956	2958	rBV	330	223	0.02%	0.003%
66	10.571	2961	2964	2968	rVB3	482	374	0.04%	0.005%
67	10.625	2977	2981	2984	rBV2	276	249	0.03%	0.003%
68	10.853	3049	3052	3055	rBV2	153	122	0.01%	0.002%
69	10.921	3065	3073	3081	rVV5	1715	2553	0.26%	0.035%
70	11.030	3102	3107	3110	rBV	420	256	0.03%	0.003%
71	11.143	3136	3142	3143	rBV2	840	808	0.08%	0.011%
72	11.181	3149	3154	3155	rBV	327	212	0.02%	0.003%
73	11.249	3164	3175	3199	rBV	464045	709159	73.56%	9.588%
74	11.490	3249	3250	3253	rVB	385	145	0.02%	0.002%
75	11.625	3280	3292	3317	rBV	483744	745951	77.37%	10.085%
76	11.751	3328	3331	3334	rBV3	428	311	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
 Data File : VV023187.D
 Acq On : 03 Nov 2021 15:22
 Operator : SY/MD
 Sample : VV1103MBL07
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK275

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

77	11.770	3334	3337	3339	rBV3	425	264	0.03%	0.004%
78	11.892	3370	3375	3377	rBV3	248	243	0.03%	0.003%
79	12.059	3424	3427	3430	rBV	273	177	0.02%	0.002%
80	12.091	3434	3437	3439	rBV2	440	291	0.03%	0.004%
81	12.152	3454	3456	3460	rVB	333	196	0.02%	0.003%
82	12.284	3494	3497	3501	rBV	431	384	0.04%	0.005%
83	12.455	3548	3550	3552	rBV2	272	126	0.01%	0.002%
84	12.570	3583	3586	3591	rBV2	395	334	0.03%	0.005%
85	12.628	3600	3604	3606	rBV	232	197	0.02%	0.003%
86	12.689	3621	3623	3625	rBV	311	152	0.02%	0.002%
87	12.754	3641	3643	3648	rBV2	298	251	0.03%	0.003%
88	12.796	3652	3656	3658	rBV2	432	323	0.03%	0.004%
89	13.458	3860	3862	3863	rBV	298	129	0.01%	0.002%
90	13.590	3898	3903	3909	rBV	223	349	0.04%	0.005%
91	13.693	3931	3935	3936	rBV	370	214	0.02%	0.003%
92	13.702	3936	3938	3941	rVB	326	142	0.01%	0.002%
93	13.722	3942	3944	3947	rVB2	414	210	0.02%	0.003%
94	13.744	3947	3951	3953	rBV3	799	639	0.07%	0.009%
95	13.837	3978	3980	3983	rBV2	269	149	0.02%	0.002%
96	13.895	3995	3998	3999	rBV2	244	131	0.01%	0.002%
97	13.982	4022	4025	4026	rBV2	293	141	0.01%	0.002%
98	14.185	4086	4088	4090	rBV	412	182	0.02%	0.002%
99	14.397	4150	4154	4158	rBV4	427	382	0.04%	0.005%
100	14.570	4205	4208	4211	rBV3	439	334	0.03%	0.005%




Sum of corrected areas: 7396607

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
Data File : VV023187.D
Acq On : 03 Nov 2021 15:22
Operator : SY/MD
Sample : VV1103MBL07
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK275

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

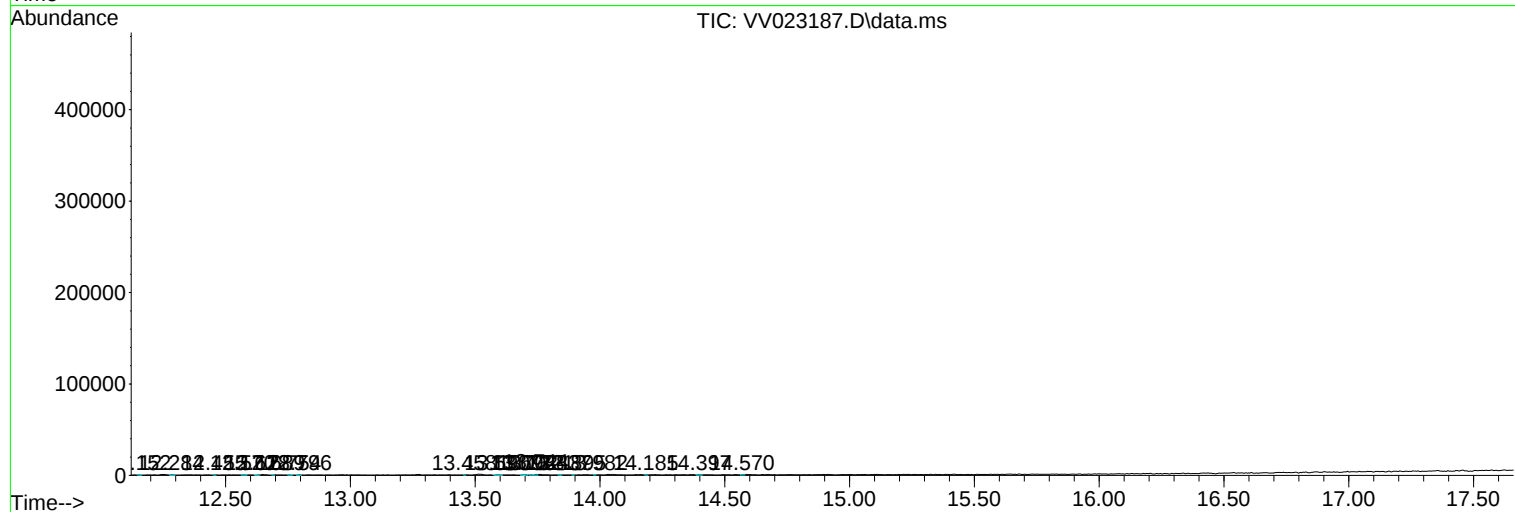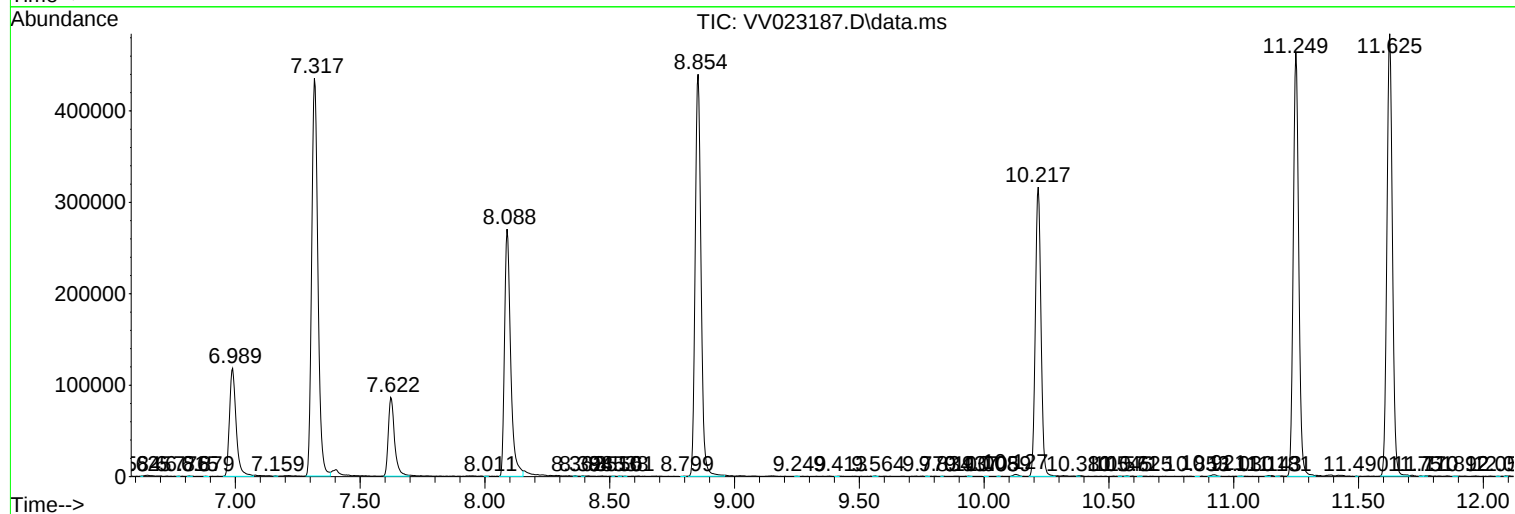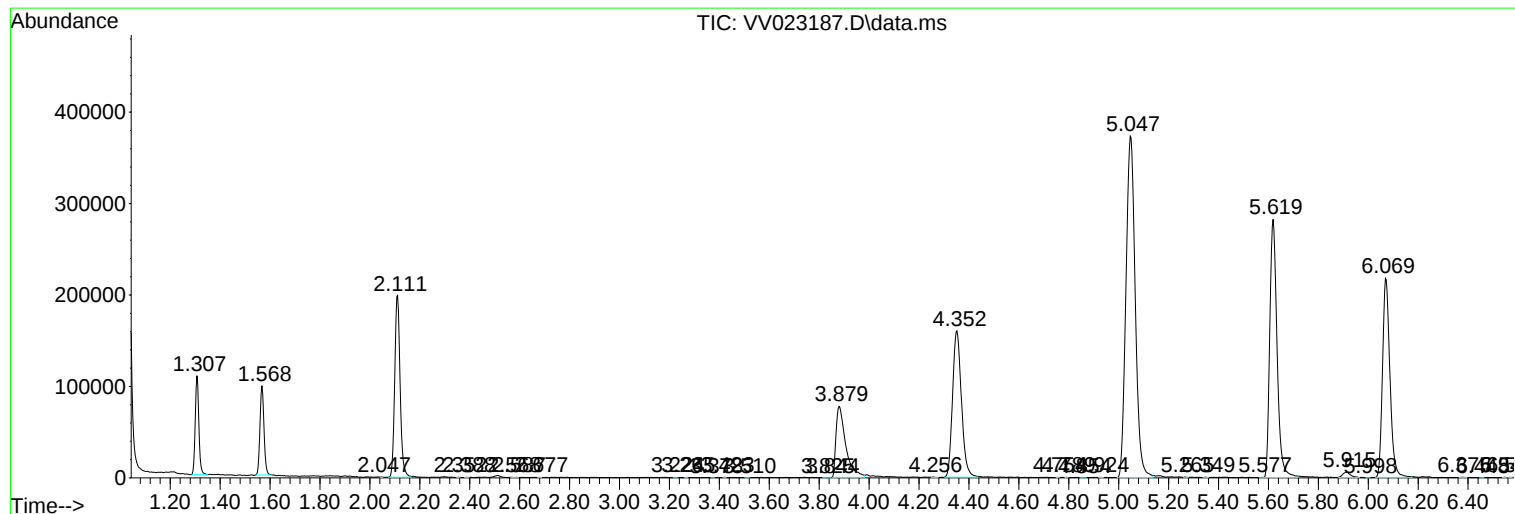

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
Data File : VV023187.D
Acq On : 03 Nov 2021 15:22
Operator : SY/MD
Sample : VV1103MBL07
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK275

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
Data File : VV023187.D
Acq On : 03 Nov 2021 15:22
Operator : SY/MD
Sample : VV1103MBL07
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK275

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc