

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
 Data File : VV023189.D
 Acq On : 03 Nov 2021 16:10
 Operator : SY/MD
 Sample : VV1103WBL07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M

Title : VOC Analysis

Signal : TIC: VV023189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	116726	114541	11.59%	1.519%
2	1.568	157	164	179	rVB	100349	111785	11.31%	1.483%
3	2.108	321	332	351	rBV	210236	310588	31.42%	4.119%
4	2.320	396	398	402	rVB3	485	218	0.02%	0.003%
5	2.346	404	406	412	rVB2	387	239	0.02%	0.003%
6	2.439	432	435	436	rBV	419	258	0.03%	0.003%
7	2.507	449	456	458	rBV3	1603	1656	0.17%	0.022%
8	2.552	467	470	473	rVB	396	210	0.02%	0.003%
9	2.571	473	476	478	rBV2	341	141	0.01%	0.002%
10	2.632	491	495	499	rBV	387	373	0.04%	0.005%
11	2.809	546	550	554	rBV	311	324	0.03%	0.004%
12	3.105	637	642	643	rBV	310	227	0.02%	0.003%
13	3.150	652	656	659	rBV	279	243	0.02%	0.003%
14	3.230	679	681	685	rBV2	263	151	0.02%	0.002%
15	3.413	735	738	742	rVV2	221	159	0.02%	0.002%
16	3.462	749	753	757	rBV	234	276	0.03%	0.004%
17	3.487	757	761	763	rBV2	227	186	0.02%	0.002%
18	3.645	809	810	815	rVB2	337	200	0.02%	0.003%
19	3.683	820	822	825	rVB2	237	129	0.01%	0.002%
20	3.838	867	870	873	rVB2	245	150	0.02%	0.002%
21	3.880	873	883	919	rBV	81719	225668	22.83%	2.993%
22	4.349	1014	1029	1055	rBV	164889	404693	40.94%	5.367%
23	4.558	1090	1094	1098	rBV2	460	423	0.04%	0.006%
24	4.600	1103	1107	1110	rBV	405	362	0.04%	0.005%
25	4.683	1131	1133	1135	rBV2	543	240	0.02%	0.003%
26	4.732	1146	1148	1153	rVB	496	244	0.02%	0.003%
27	4.905	1197	1202	1205	rBV2	328	330	0.03%	0.004%
28	5.047	1230	1246	1278	rBV2	380677	988472	100.00%	13.110%
29	5.256	1307	1311	1312	rBV2	440	266	0.03%	0.004%
30	5.400	1354	1356	1358	rBV2	387	189	0.02%	0.003%
31	5.445	1366	1370	1373	rBV	352	258	0.03%	0.003%
32	5.516	1390	1392	1395	rBV	330	144	0.01%	0.002%
33	5.539	1397	1399	1403	rVB4	453	238	0.02%	0.003%
34	5.619	1412	1424	1449	rBV	279988	565000	57.16%	7.494%
35	5.912	1505	1515	1533	rBV7	5661	12717	1.29%	0.169%
36	6.008	1541	1545	1550	rVB2	398	325	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
 Data File : VV023189.D
 Acq On : 03 Nov 2021 16:10
 Operator : SY/MD
 Sample : VV1103WBL07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

37	6.069	1550	1564	1587	rBV	219133	452991	45.83%	6.008%
38	6.281	1627	1630	1632	rBV3	425	249	0.03%	0.003%
39	6.375	1658	1659	1662	rVB	436	151	0.02%	0.002%
40	6.410	1665	1670	1675	rVB2	239	217	0.02%	0.003%
41	6.506	1698	1700	1704	rBV2	421	272	0.03%	0.004%
42	6.535	1707	1709	1711	rVV	511	211	0.02%	0.003%
43	6.551	1711	1714	1720	rVV2	278	345	0.03%	0.005%
44	6.616	1731	1734	1736	rBV	363	157	0.02%	0.002%
45	6.632	1736	1739	1741	rBV2	959	705	0.07%	0.009%
46	6.738	1767	1772	1774	rBV2	499	399	0.04%	0.005%
47	6.751	1774	1776	1781	rVV2	291	228	0.02%	0.003%
48	6.799	1788	1791	1795	rBV2	200	174	0.02%	0.002%
49	6.828	1795	1800	1802	rBV2	268	209	0.02%	0.003%
50	6.860	1807	1810	1811	rBV	282	128	0.01%	0.002%
51	6.986	1836	1849	1869	rBV	122046	220571	22.31%	2.925%
52	7.185	1903	1911	1915	rBV5	962	1269	0.13%	0.017%
53	7.256	1931	1933	1936	rBV3	277	153	0.02%	0.002%
54	7.317	1940	1952	1971	rBV	443817	772090	78.11%	10.240%
55	7.622	2037	2047	2077	rVV2	88273	155203	15.70%	2.058%
56	7.860	2119	2121	2125	rBV3	387	316	0.03%	0.004%
57	8.021	2168	2171	2174	rBV2	171	142	0.01%	0.002%
58	8.047	2178	2179	2182	rBV3	281	153	0.02%	0.002%
59	8.088	2182	2192	2237	rBV	284060	499322	50.51%	6.622%
60	8.397	2286	2288	2290	rVB3	417	186	0.02%	0.002%
61	8.484	2314	2315	2318	rBV3	237	141	0.01%	0.002%
62	8.657	2365	2369	2372	rBV2	275	185	0.02%	0.002%
63	8.854	2418	2430	2462	rBV	442419	711460	71.98%	9.436%
64	9.149	2517	2522	2525	rBV3	681	553	0.06%	0.007%
65	9.313	2569	2573	2575	rBV	288	198	0.02%	0.003%
66	9.339	2580	2581	2584	rBV2	273	148	0.01%	0.002%
67	9.394	2597	2598	2604	rVB3	377	257	0.03%	0.003%
68	9.471	2619	2622	2623	rBV3	261	138	0.01%	0.002%
69	9.661	2678	2681	2685	rBV3	193	152	0.02%	0.002%
70	9.680	2685	2687	2692	rBV2	193	125	0.01%	0.002%
71	9.747	2701	2708	2712	rBV2	447	558	0.06%	0.007%
72	9.767	2712	2714	2717	rVB2	296	142	0.01%	0.002%
73	9.841	2733	2737	2740	rBV2	238	171	0.02%	0.002%
74	9.905	2755	2757	2759	rBV2	262	152	0.02%	0.002%
75	10.124	2821	2825	2835	rVB4	2116	2858	0.29%	0.038%
76	10.217	2841	2854	2873	rBV	328300	513352	51.93%	6.809%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
 Data File : VV023189.D
 Acq On : 03 Nov 2021 16:10
 Operator : SY/MD
 Sample : VV1103WBL07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

77	10.317	2883	2885	2887	rBV2	499	338	0.03%	0.004%
78	10.416	2913	2916	2918	rBV	205	121	0.01%	0.002%
79	10.612	2975	2977	2981	rVB2	450	281	0.03%	0.004%
80	10.699	3000	3004	3009	rBV2	255	221	0.02%	0.003%
81	10.789	3028	3032	3039	rVB2	373	307	0.03%	0.004%
82	10.886	3058	3062	3064	rBV3	215	167	0.02%	0.002%
83	10.911	3064	3070	3071	rBV	1073	776	0.08%	0.010%
84	11.066	3114	3118	3120	rBV3	394	303	0.03%	0.004%
85	11.249	3164	3175	3196	rBV	456848	695975	70.41%	9.231%
86	11.522	3256	3260	3262	rBV3	345	259	0.03%	0.003%
87	11.625	3280	3292	3316	rBV	479592	759655	76.85%	10.075%
88	12.079	3430	3433	3435	rBV2	217	158	0.02%	0.002%
89	12.098	3437	3439	3445	rVB3	436	318	0.03%	0.004%
90	12.548	3577	3579	3584	rBV3	253	196	0.02%	0.003%
91	12.603	3592	3596	3601	rVB3	518	495	0.05%	0.007%
92	12.731	3632	3636	3638	rBV2	476	404	0.04%	0.005%
93	12.931	3696	3698	3701	rBV2	256	147	0.01%	0.002%
94	13.027	3726	3728	3732	rBV2	316	167	0.02%	0.002%
95	13.271	3800	3804	3805	rBV	414	272	0.03%	0.004%
96	13.554	3890	3892	3893	rBV	304	133	0.01%	0.002%
97	13.776	3959	3961	3962	rBV	478	169	0.02%	0.002%
98	14.021	4033	4037	4038	rBV	538	397	0.04%	0.005%
99	14.149	4075	4077	4079	rBV	307	150	0.02%	0.002%
100	14.300	4120	4124	4128	rBV4	421	339	0.03%	0.004%




Sum of corrected areas: 7539802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
Data File : VV023189.D
Acq On : 03 Nov 2021 16:10
Operator : SY/MD
Sample : VV1103WBL07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

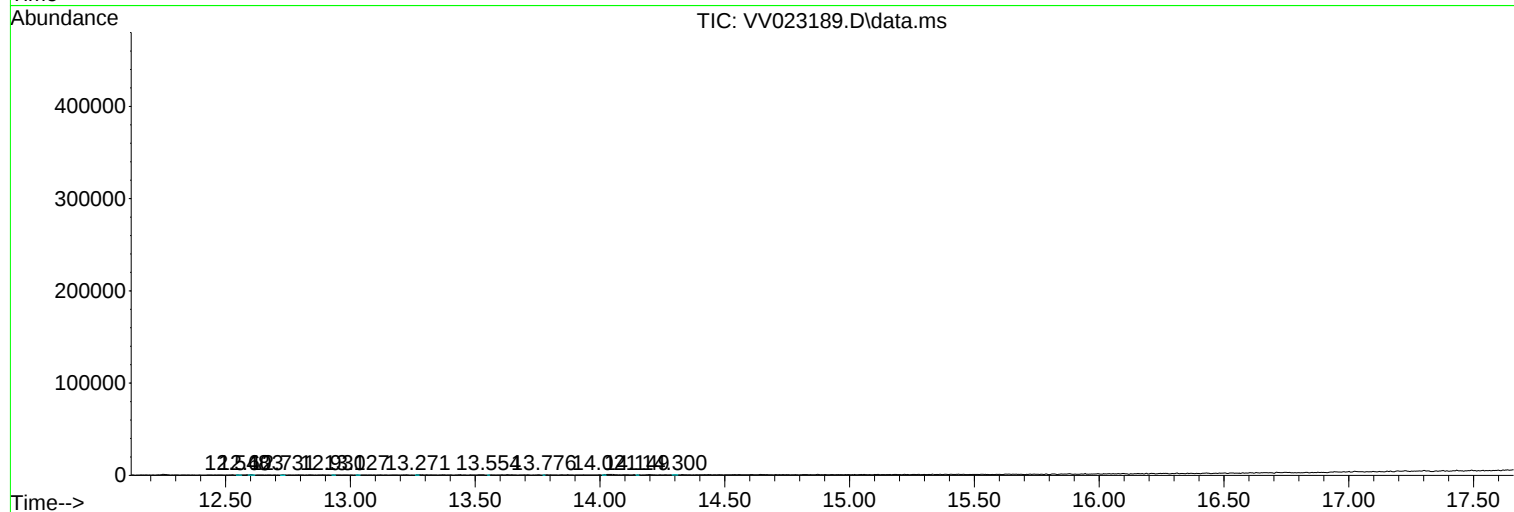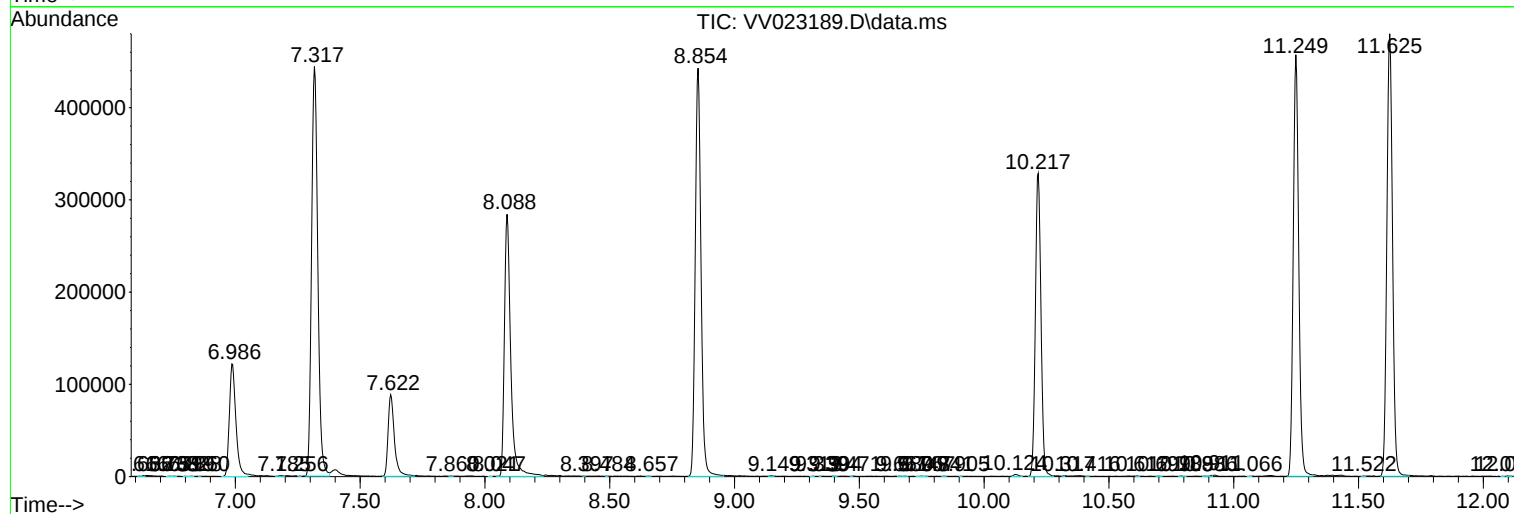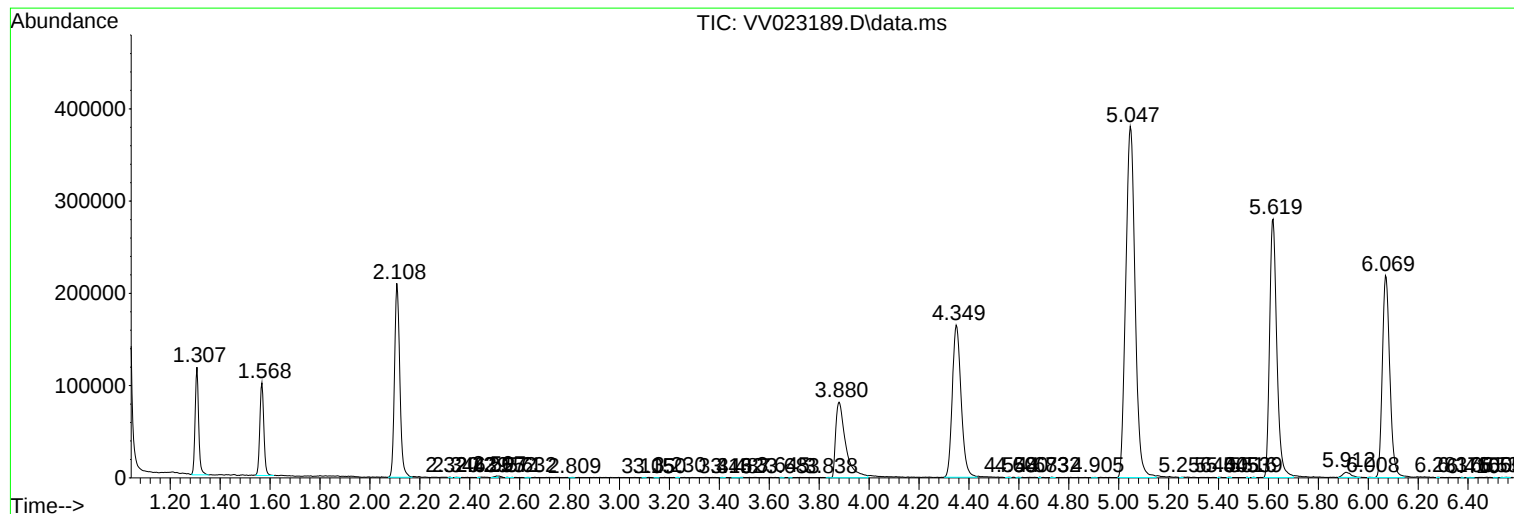

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
Data File : VV023189.D
Acq On : 03 Nov 2021 16:10
Operator : SY/MD
Sample : VV1103WBL07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
Data File : VV023189.D
Acq On : 03 Nov 2021 16:10
Operator : SY/MD
Sample : VV1103WBL07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
