
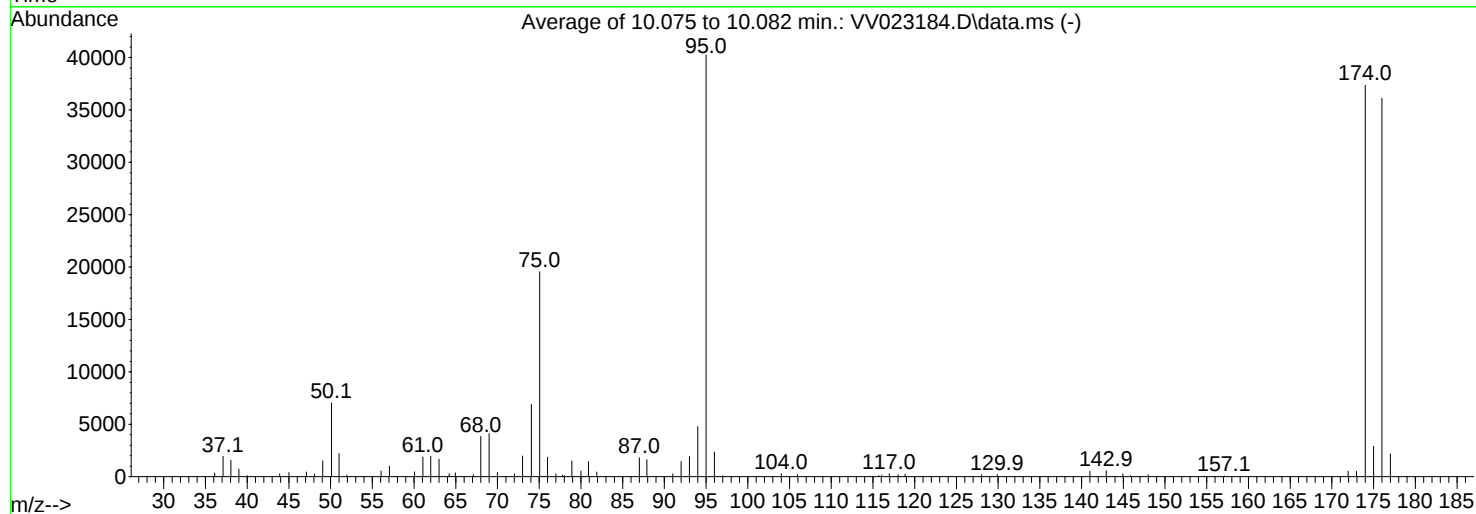


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110321\
Data File : VV023184.D
Acq On : 03 Nov 2021 14:00
Operator : SY/MD
Sample : BFB245
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB245

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Title : VOC Analysis
Last Update : Sat Oct 30 00:25:16 2021

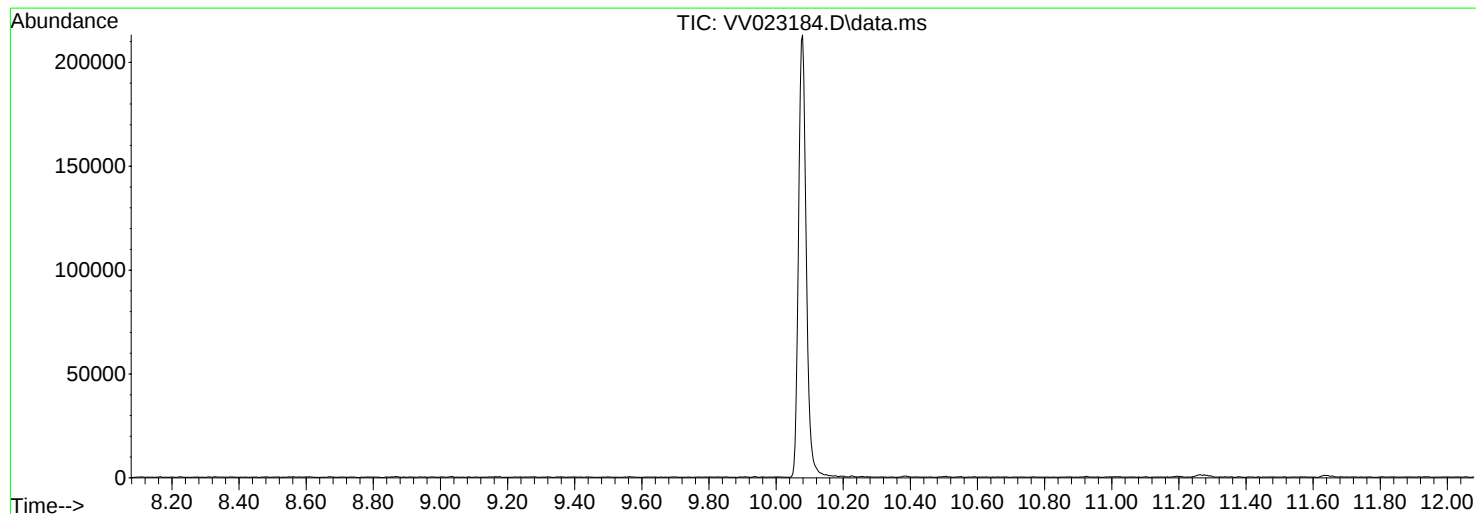

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	7042	PASS
75	95	30	80	48.5	19539	PASS
95	95	100	100	100.0	40251	PASS
96	95	5	9	5.8	2352	PASS
173	174	0.00	2	1.3	502	PASS
174	95	50	120	92.8	37355	PASS
175	174	5	9	7.8	2908	PASS
176	174	95	105	96.7	36117	PASS
177	176	5	10	6.0	2171	PASS

m/z	Abundance
40.10	161.0
43.80	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.10	436.0
37.10	1902.0
38.10	1606.0
39.00	720.0
40.10	199.0
40.90	116.0
44.00	441.0
45.00	402.0
47.10	458.0
48.00	227.0
49.10	1554.0
50.10	7240.0
51.00	2257.0
52.00	138.0
53.00	116.0
55.10	116.0
56.00	616.0
57.00	1089.0
60.00	466.0
61.10	1953.0
62.00	2046.0
63.00	1722.0
64.20	294.0
65.00	417.0
67.10	161.0
68.00	3884.0
69.00	4357.0
70.00	393.0
72.00	242.0
73.00	1837.0
74.10	7011.0
75.10	20208.0
76.00	1998.0
77.00	298.0
77.80	232.0
78.90	1502.0
80.00	547.0
80.90	1440.0
81.90	457.0
87.00	1911.0
87.90	1642.0
91.00	290.0
92.00	1509.0
93.00	1802.0
94.00	5125.0
95.00	41152.0
96.00	2395.0
97.00	145.0
104.00	257.0
105.90	242.0
115.70	171.0
116.10	166.0
117.00	281.0
118.00	205.0
118.80	205.0
128.00	198.0
129.90	163.0
130.70	114.0
141.00	561.0
142.90	568.0
144.90	242.0
145.90	109.0
148.00	130.0
154.70	108.0
171.90	477.0
173.00	460.0
174.00	37048.0
175.00	3095.0
176.00	36432.0
177.00	2290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.10	349.0
37.10	2016.0
38.10	1630.0
39.00	722.0
39.90	179.0
40.10	172.0
43.90	443.0
45.00	426.0
47.10	454.0
48.10	242.0
49.10	1544.0
50.10	7249.0
51.00	2242.0
52.00	144.0
56.10	548.0
57.10	1033.0
60.00	499.0
61.00	1921.0
62.00	1991.0
63.00	1703.0
64.20	307.0
65.00	348.0
67.10	195.0
68.00	3944.0
69.00	4237.0
70.00	417.0
72.00	267.0
73.00	2054.0
74.10	7104.0
75.10	20128.0
76.00	1880.0
77.00	252.0
77.80	225.0
78.90	1561.0
80.00	551.0
80.90	1456.0
81.90	459.0
87.00	1846.0
87.90	1655.0
91.00	271.0
92.00	1526.0
93.00	2017.0
94.00	4867.0
95.00	41512.0
96.00	2390.0
97.00	118.0
104.00	281.0
105.90	203.0
115.70	152.0
116.10	138.0
117.00	281.0
118.00	185.0
118.80	238.0
128.00	191.0
129.90	205.0
141.00	546.0
143.00	577.0
144.90	267.0
145.80	111.0
148.00	187.0
157.10	103.0
171.90	535.0
173.00	497.0
174.00	38744.0
175.00	3050.0
176.00	37360.0
177.00	2223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.10	287.0
37.10	1888.0
38.00	1506.0
39.00	721.0
39.90	191.0
43.90	415.0
45.00	378.0
47.10	431.0
48.00	251.0
49.00	1430.0
50.10	6637.0
51.00	2128.0
51.90	137.0
56.00	466.0
57.10	872.0
60.10	399.0
61.00	1784.0
62.00	1773.0
63.00	1552.0
64.20	295.0
64.90	317.0
67.10	193.0
68.00	3688.0
69.00	3739.0
70.00	378.0
72.10	252.0
73.00	2003.0
74.00	6574.0
75.00	18280.0
76.00	1712.0
77.00	238.0
78.00	235.0
78.90	1409.0
80.00	497.0
80.90	1377.0
81.90	421.0
87.00	1634.0
87.90	1558.0
91.00	234.0
92.00	1328.0
93.00	1906.0
94.00	4358.0
95.00	38088.0
96.00	2272.0
104.00	265.0
105.00	104.0
106.00	175.0
116.00	136.0
116.80	289.0
118.00	173.0
118.90	255.0
128.00	162.0
129.90	225.0
141.00	446.0
143.00	541.0
145.00	252.0
145.80	110.0
148.00	192.0
157.10	101.0
172.00	544.0
172.90	549.0
174.00	36272.0
175.00	2580.0
176.00	34560.0
177.00	1999.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245