

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
 Data File : VV028847.D
 Acq On : 03 Nov 2022 12:20
 Operator : SY/MD
 Sample : VV1103MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK286

Quant Time: Nov 04 04:43:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 04 04:43:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	398316	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	360571	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	158449	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	154803	40.997	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	82.000%		
7) Chloroethane-d5	1.561	69	141904	43.962	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.920%		
11) 1,1-Dichloroethene-d2	2.104	63	223368	31.098	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.200%		
21) 2-Butanone-d5	3.873	46	296701	107.944	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	107.940%		
24) Chloroform-d	4.342	84	253471	44.508	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.020%		
26) 1,2-Dichloroethane-d4	5.027	65	181360	48.152	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.300%		
32) Benzene-d6	5.043	84	509531	45.267	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.540%		
36) 1,2-Dichloropropane-d6	6.066	67	184835	47.830	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.660%		
41) Toluene-d8	7.310	98	423780	42.826	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.660%		
43) trans-1,3-Dichloroprop...	7.619	79	66021	44.482	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.960%		
47) 2-Hexanone-d5	8.085	63	171665	98.298	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.300%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	243940	47.871	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.740%		
66) 1,2-Dichlorobenzene-d4	11.615	152	142689	45.622	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.240%		
Target Compounds						Qvalue
35) Methylcyclohexane	6.066	83	39411	7.485	ug/L	# 16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
Data File : VV028847.D
Acq On : 03 Nov 2022 12:20
Operator : SY/MD
Sample : VV1103MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK286

Quant Time: Nov 04 04:43:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 04 04:43:26 2022
Response via : Initial Calibration

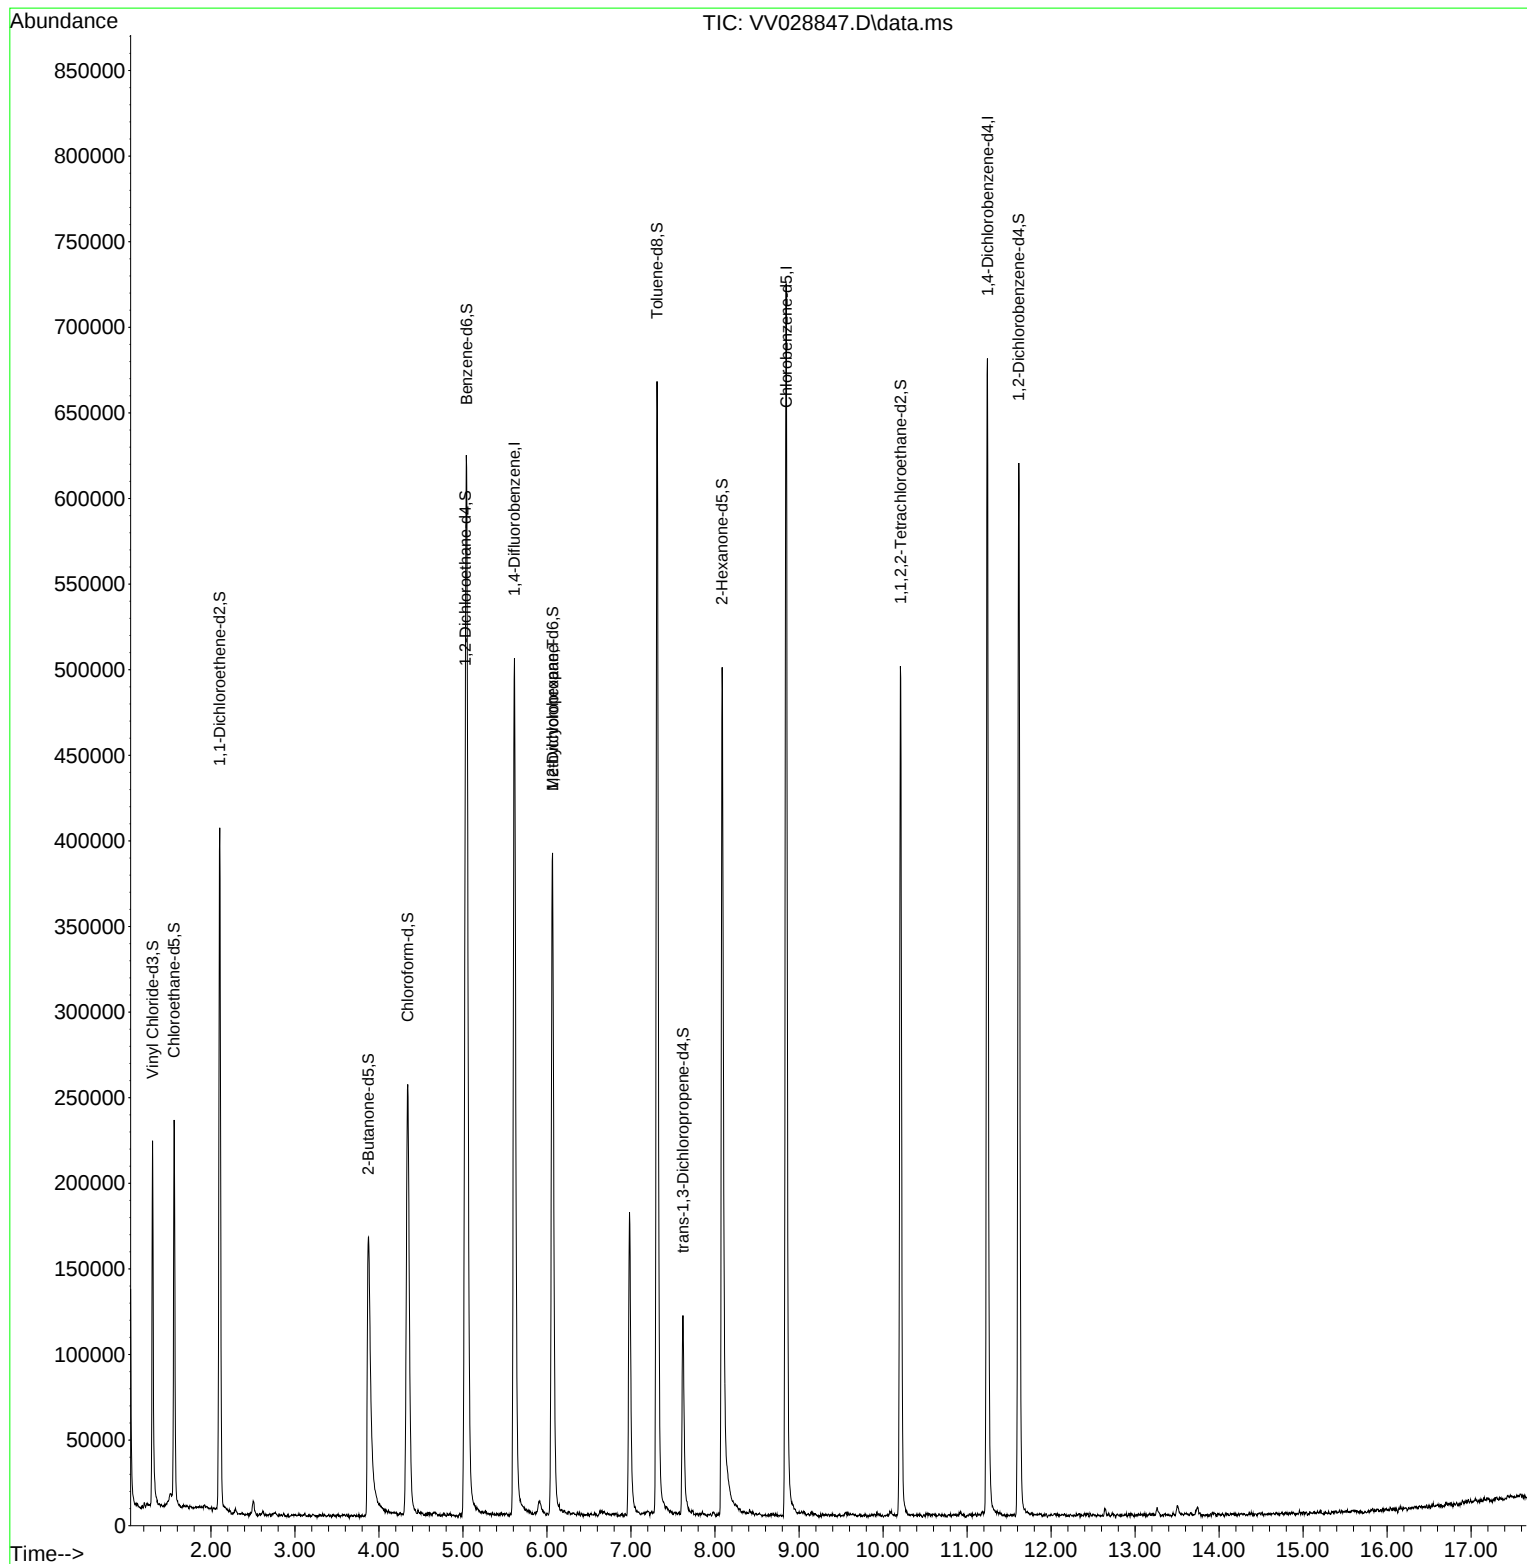

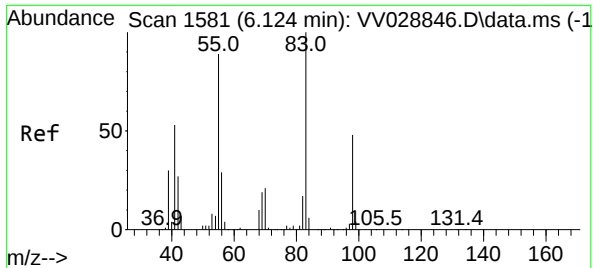

#35
 Methylcyclohexane
 Concen: 7.485 ug/L
 RT: 6.066 min Scan# 11
 Delta R.T. -0.058 min
 Lab File: VV028847.D
 Acq: 03 Nov 2022 12:20

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK286

Tgt Ion:	83	Resp:	39411
Ion	Ratio	Lower	Upper
83	100		
55	1.3	69.4	104.2#
98	1.0	37.0	55.4#

