




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
 Data File : VV028848.D
 Acq On : 03 Nov 2022 12:45
 Operator : SY/MD
 Sample : VV1103WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK287

Manual IntegrationsAPPROVED

Quant Time: Nov 04 04:44:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 04 04:43:26 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/04/2022
 Supervised By :Mahesh Dadoda 11/04/2022

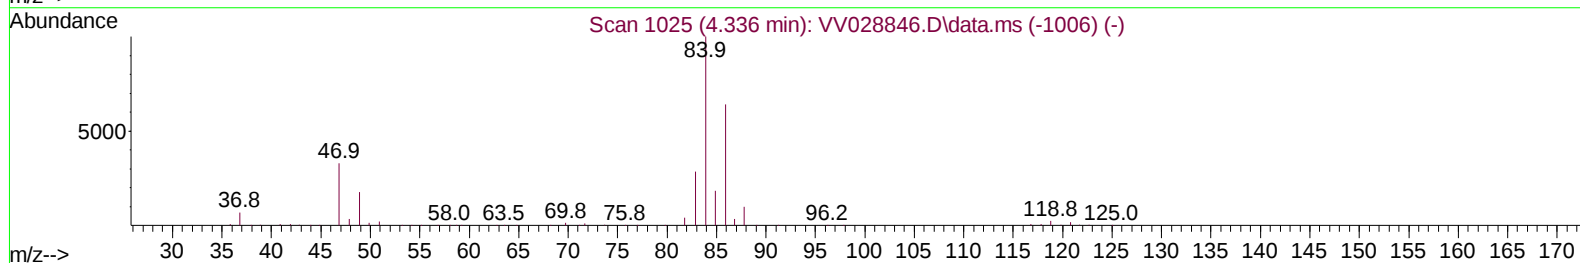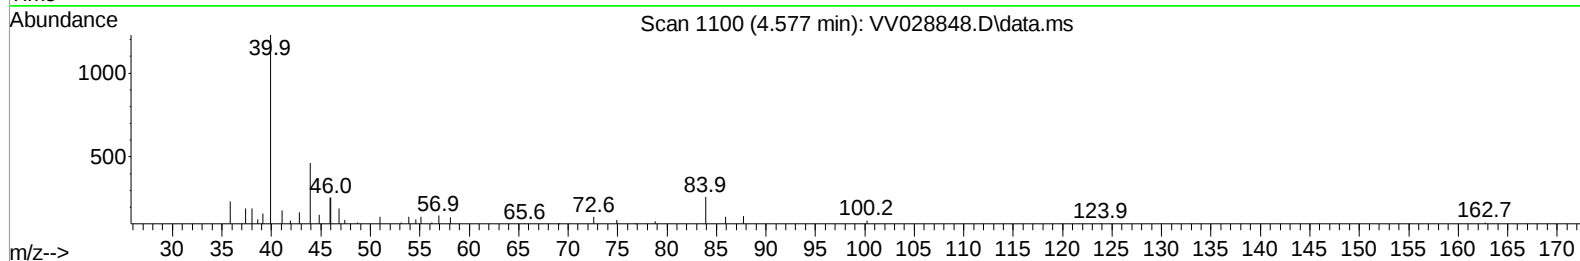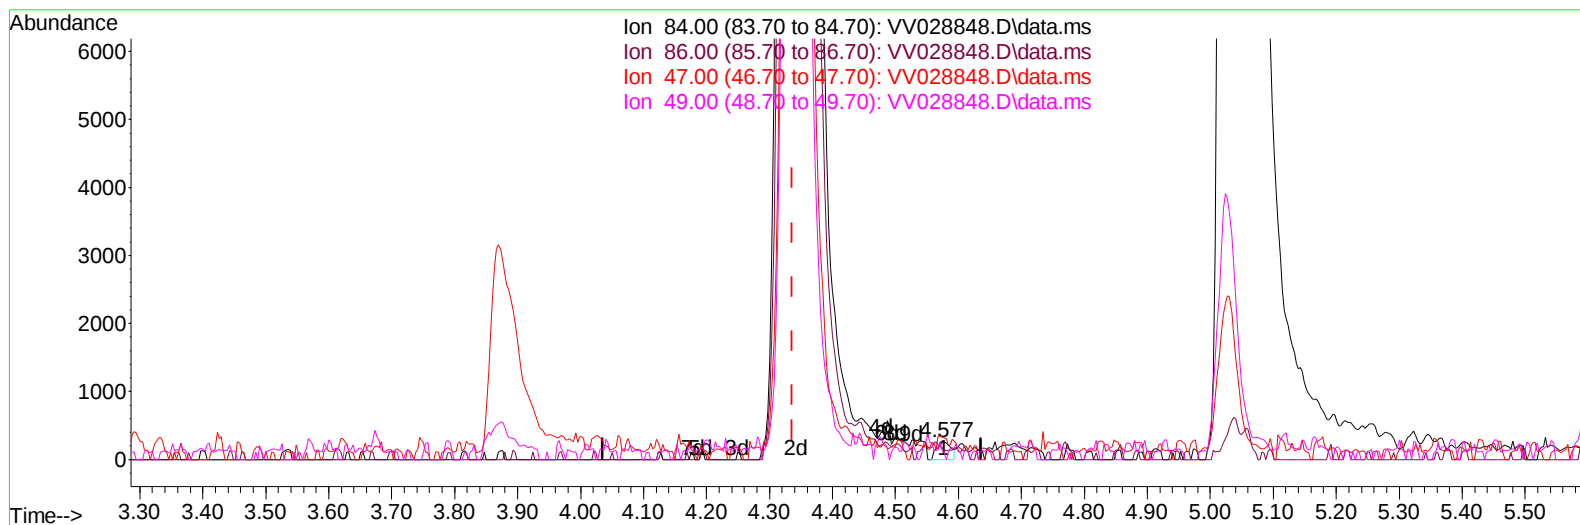

TIC: VV028848.D\data.ms

(24) Chloroform-d (S)

4.577min (+ 0.241) 0.08 ug/L

response 411

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	45.26
47.00	52.10	46.23
49.00	30.40	30.41

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
 Data File : VV028848.D
 Acq On : 03 Nov 2022 12:45
 Operator : SY/MD
 Sample : VV1103WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK287

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/04/2022
 Supervised By :Mahesh Dadoda 11/04/2022

Quant Time: Nov 04 04:44:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 04 04:43:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	377204	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	343226	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	147218	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	139563	39.030	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	78.060%	
7) Chloroethane-d5	1.561	69	126522	41.390	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	82.780%	
11) 1,1-Dichloroethene-d2	2.105	63	207394	30.490	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	60.980%	
21) 2-Butanone-d5	3.870	46	276322	106.157	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	106.160%	
24) Chloroform-d	4.342	84	241583m	44.795	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	89.580%	
26) 1,2-Dichloroethane-d4	5.024	65	174213	48.843	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.680%	
32) Benzene-d6	5.043	84	488667	45.607	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.220%	
36) 1,2-Dichloropropane-d6	6.063	67	176826	48.070	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	96.140%	
41) Toluene-d8	7.310	98	399757	42.439	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	84.880%	
43) trans-1,3-Dichloroprop...	7.619	79	59635	42.210	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	84.420%	
47) 2-Hexanone-d5	8.082	63	163004	98.056	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	98.060%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	235664	48.584	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	97.160%	
66) 1,2-Dichlorobenzene-d4	11.615	152	138122	47.531	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	95.060%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
Data File : VV028848.D
Acq On : 03 Nov 2022 12:45
Operator : SY/MD
Sample : VV1103WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK287

Manual IntegrationsAPPROVED

Quant Time: Nov 04 04:44:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 04 04:43:26 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/04/2022
Supervised By :Mahesh Dadoda 11/04/2022

