

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
 Data File : VV028848.D
 Acq On : 03 Nov 2022 12:45
 Operator : SY/MD
 Sample : VV1103WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK287

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rBV	196432	213802	13.85%	1.816%
2	1.561	155	162	177	rVB	194951	227355	14.73%	1.931%
3	2.105	321	331	346	rVB	369976	527073	34.15%	4.477%
4	2.333	400	402	404	rBV3	1575	905	0.06%	0.008%
5	2.584	475	480	483	rBV6	2082	2226	0.14%	0.019%
6	2.699	514	516	519	rBV4	1667	1113	0.07%	0.009%
7	2.744	528	530	531	rBV2	1405	541	0.04%	0.005%
8	2.912	578	582	586	rBV7	1480	1442	0.09%	0.012%
9	2.960	595	597	599	rBV2	647	316	0.02%	0.003%
10	3.011	611	613	614	rBV2	1748	582	0.04%	0.005%
11	3.040	620	622	625	rVB4	985	544	0.04%	0.005%
12	3.101	639	641	643	rBV4	931	357	0.02%	0.003%
13	3.134	646	651	654	rBV7	1673	1469	0.10%	0.012%
14	3.166	659	661	663	rBV3	935	444	0.03%	0.004%
15	3.230	678	681	682	rBV3	1354	844	0.05%	0.007%
16	3.288	697	699	701	rVB3	1125	390	0.03%	0.003%
17	3.310	701	706	708	rBV5	902	912	0.06%	0.008%
18	3.323	708	710	712	rBV2	1375	644	0.04%	0.005%
19	3.404	732	735	738	rBV5	1917	1579	0.10%	0.013%
20	3.561	783	784	787	rBV3	841	543	0.04%	0.005%
21	3.670	815	818	819	rBV2	862	471	0.03%	0.004%
22	3.693	823	825	828	rBV3	805	408	0.03%	0.003%
23	3.728	832	836	839	rBV6	1558	1389	0.09%	0.012%
24	3.764	846	847	850	rBV3	1021	536	0.03%	0.005%
25	3.815	858	863	866	rBV6	1327	1367	0.09%	0.012%
26	3.870	871	880	909	rBV	159611	460078	29.81%	3.908%
27	4.342	1013	1027	1048	rBV	238000	591171	38.30%	5.021%
28	4.712	1138	1142	1147	rBV8	2124	1863	0.12%	0.016%
29	4.744	1150	1152	1153	rBV2	1050	410	0.03%	0.003%
30	4.770	1159	1160	1163	rBV4	912	425	0.03%	0.004%
31	4.831	1177	1179	1182	rVB4	1875	1054	0.07%	0.009%
32	4.857	1182	1187	1189	rBV6	1706	1739	0.11%	0.015%
33	5.040	1228	1244	1271	rBV2	590267	1543518	100.00%	13.110%
34	5.339	1335	1337	1341	rBV4	1743	1184	0.08%	0.010%
35	5.381	1348	1350	1352	rBV3	1214	670	0.04%	0.006%
36	5.449	1369	1371	1373	rBV3	1648	854	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
 Data File : VV028848.D
 Acq On : 03 Nov 2022 12:45
 Operator : SY/MD
 Sample : VV1103WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK287

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	5.613	1410	1422	1444	rBV	474592	959352	62.15%	8.148%
38	6.066	1551	1563	1586	rBV	372384	747841	48.45%	6.352%
39	6.439	1677	1679	1683	rBV5	1367	984	0.06%	0.008%
40	6.500	1695	1698	1702	rBV6	2481	2542	0.16%	0.022%
41	6.619	1733	1735	1737	rBV3	2060	1257	0.08%	0.011%
42	6.812	1793	1795	1799	rBV5	1545	1019	0.07%	0.009%
43	6.895	1819	1821	1825	rVB4	1090	672	0.04%	0.006%
44	6.982	1838	1848	1875	rBV	168248	313042	20.28%	2.659%
45	7.310	1939	1950	1979	rBV	626350	1108106	71.79%	9.412%
46	7.619	2036	2046	2064	rBV	107926	199374	12.92%	1.693%
47	7.953	2146	2150	2153	rBV5	2549	1788	0.12%	0.015%
48	8.085	2181	2191	2233	rBV	478311	945224	61.24%	8.028%
49	8.545	2332	2334	2337	rVB4	1834	944	0.06%	0.008%
50	8.648	2364	2366	2367	rBV2	1478	623	0.04%	0.005%
51	8.847	2417	2428	2451	rBV	690367	1134049	73.47%	9.632%
52	9.034	2484	2486	2487	rBV2	2036	908	0.06%	0.008%
53	9.526	2637	2639	2642	rBV4	803	598	0.04%	0.005%
54	9.551	2644	2647	2649	rBV4	2025	1307	0.08%	0.011%
55	9.677	2684	2686	2688	rBV3	1191	568	0.04%	0.005%
56	9.747	2706	2708	2709	rBV2	1021	460	0.03%	0.004%
57	9.882	2747	2750	2752	rBV3	1414	786	0.05%	0.007%
58	9.924	2756	2763	2764	rBV7	2203	2093	0.14%	0.018%
59	9.963	2772	2775	2780	rVB6	1356	852	0.06%	0.007%
60	10.021	2792	2793	2794	rBV	494	160	0.01%	0.001%
61	10.034	2795	2797	2799	rVV3	901	335	0.02%	0.003%
62	10.207	2840	2851	2877	rVB	483984	763456	49.46%	6.485%
63	10.480	2932	2936	2938	rBV5	994	733	0.05%	0.006%
64	10.497	2938	2941	2943	rBV4	1428	653	0.04%	0.006%
65	10.532	2946	2952	2956	rBV9	1913	2314	0.15%	0.020%
66	10.632	2981	2983	2984	rBV2	950	270	0.02%	0.002%
67	10.863	3053	3055	3057	rBV3	1275	455	0.03%	0.004%
68	10.918	3066	3072	3073	rBV5	1966	1838	0.12%	0.016%
69	11.005	3097	3099	3103	rBV5	837	677	0.04%	0.006%
70	11.062	3113	3117	3121	rBV7	1546	1812	0.12%	0.015%
71	11.140	3139	3141	3142	rBV2	673	379	0.02%	0.003%
72	11.162	3145	3148	3150	rBV4	2209	1725	0.11%	0.015%
73	11.243	3162	3173	3192	rBV	617477	999261	64.74%	8.487%
74	11.554	3267	3270	3271	rBV3	1500	857	0.06%	0.007%
75	11.615	3278	3289	3313	rBV	591434	957503	62.03%	8.133%
76	11.902	3373	3378	3382	rBV8	1986	2270	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
 Data File : VV028848.D
 Acq On : 03 Nov 2022 12:45
 Operator : SY/MD
 Sample : VV1103WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK287

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	11.956	3393	3395	3399	rBV4	1061	734	0.05%	0.006%
78	11.976	3399	3401	3405	rVB5	1346	692	0.04%	0.006%
79	12.188	3464	3467	3470	rBV4	1457	1187	0.08%	0.010%
80	12.217	3474	3476	3480	rVV4	1345	815	0.05%	0.007%
81	12.284	3495	3497	3501	rBV4	1475	1251	0.08%	0.011%
82	12.381	3524	3527	3529	rVB3	1450	763	0.05%	0.006%
83	12.423	3539	3540	3542	rBV3	1657	709	0.05%	0.006%
84	12.744	3635	3640	3644	rVB8	2125	2121	0.14%	0.018%
85	12.773	3647	3649	3653	rVB4	2532	1655	0.11%	0.014%
86	12.792	3653	3655	3656	rBV2	973	481	0.03%	0.004%
87	12.802	3656	3658	3660	rVB3	1611	771	0.05%	0.007%
88	12.853	3670	3674	3677	rBV6	1577	1442	0.09%	0.012%
89	12.972	3704	3711	3716	rBV6	2011	2829	0.18%	0.024%
90	13.050	3732	3735	3737	rBV4	962	585	0.04%	0.005%
91	13.062	3737	3739	3743	rVB4	1597	1006	0.07%	0.009%
92	13.210	3783	3785	3787	rBV3	942	505	0.03%	0.004%
93	13.297	3809	3812	3814	rBV3	1085	794	0.05%	0.007%
94	13.336	3822	3824	3827	rVB4	977	686	0.04%	0.006%
95	13.352	3827	3829	3830	rBV2	1387	587	0.04%	0.005%
96	13.410	3845	3847	3851	rBV4	1298	848	0.05%	0.007%
97	13.670	3926	3928	3933	rVB6	1691	903	0.06%	0.008%
98	14.021	4034	4037	4042	rBV7	2254	1893	0.12%	0.016%
99	14.345	4136	4138	4140	rBV3	1628	817	0.05%	0.007%




Sum of corrected areas: 11773379

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
Data File : VV028848.D
Acq On : 03 Nov 2022 12:45
Operator : SY/MD
Sample : VV1103WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK287

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

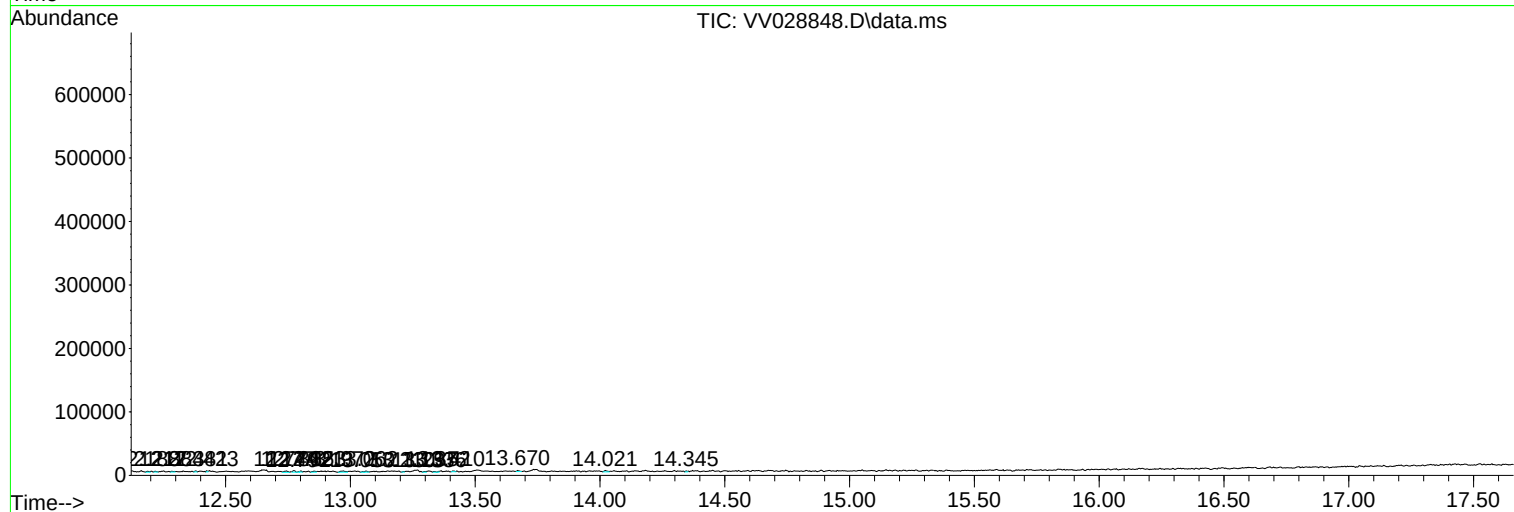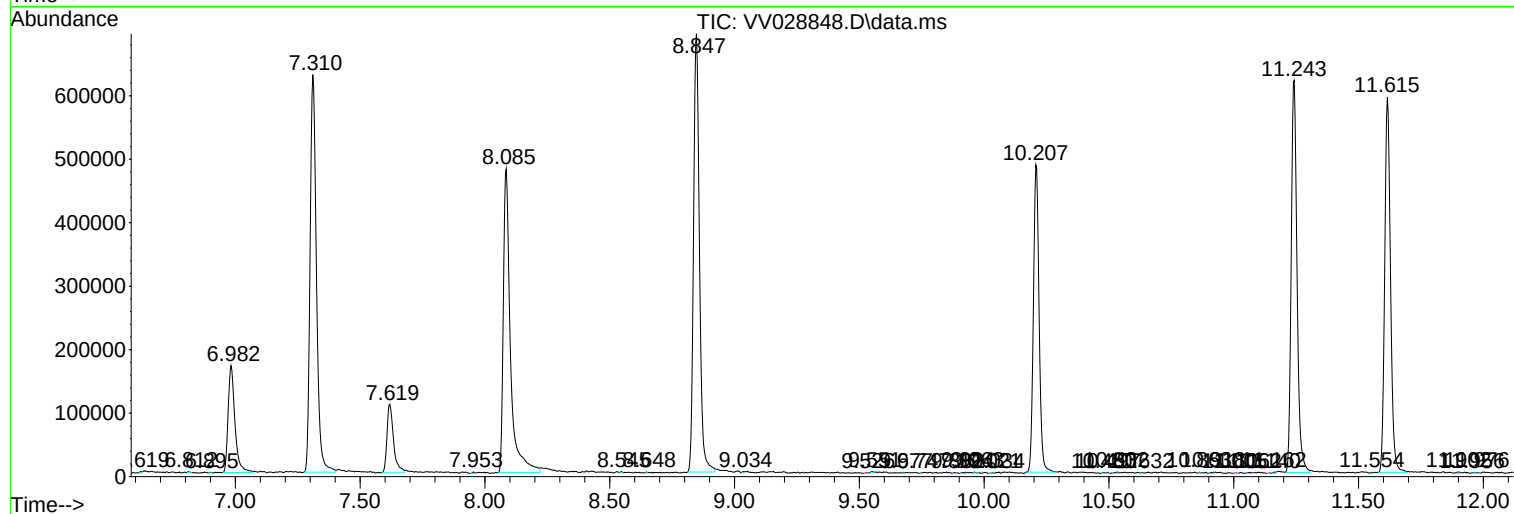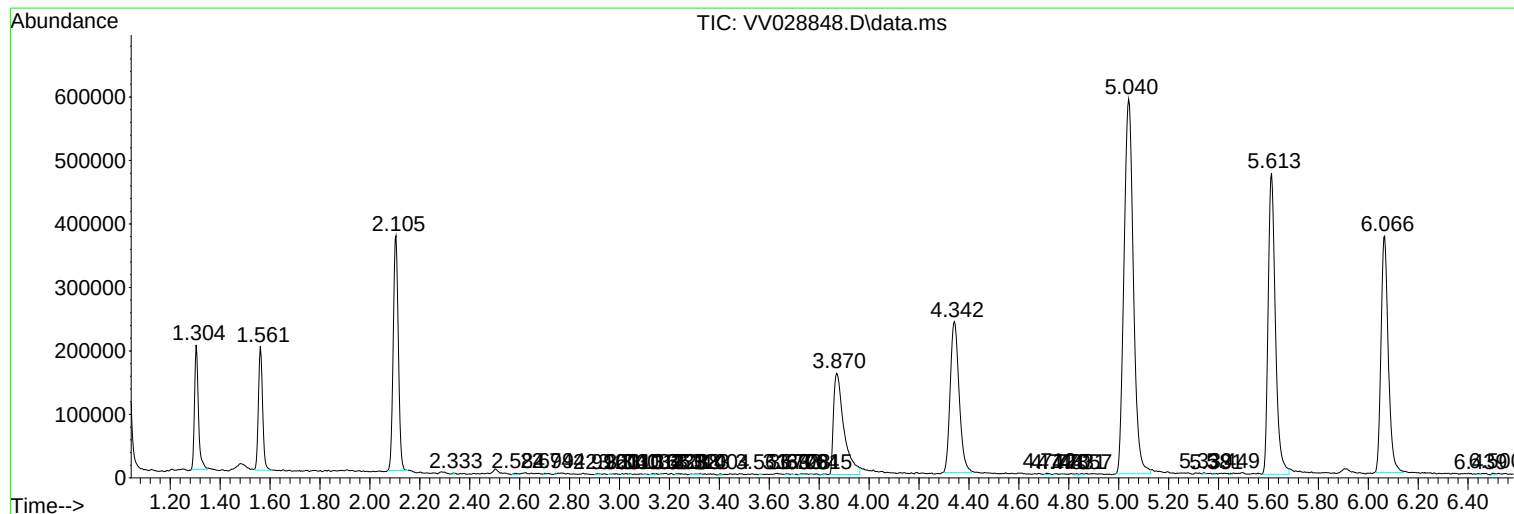

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
Data File : VV028848.D
Acq On : 03 Nov 2022 12:45
Operator : SY/MD
Sample : VV1103WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK287

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
Data File : VV028848.D
Acq On : 03 Nov 2022 12:45
Operator : SY/MD
Sample : VV1103WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK287

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
