

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
 Data File : VV028850.D
 Acq On : 03 Nov 2022 16:11
 Operator : SY/MD
 Sample : N5421-02ME
 Misc : 4.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1114ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M

Title : VOC Analysis

Signal : TIC: VV028850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	109	rVB	131306	195049	11.31%	1.447%
2	1.558	156	161	181	rBV	121592	200100	11.61%	1.484%
3	2.082	315	324	341	rVB	389215	552598	32.05%	4.099%
4	2.606	478	487	505	rVB	28061	59508	3.45%	0.441%
5	2.815	549	552	553	rBV3	1812	1076	0.06%	0.008%
6	3.069	629	631	633	rBV2	1226	756	0.04%	0.006%
7	3.117	643	646	648	rBV4	1285	909	0.05%	0.007%
8	3.153	654	657	660	rBV5	1395	1386	0.08%	0.010%
9	3.214	672	676	678	rBV6	1576	1218	0.07%	0.009%
10	3.262	690	691	694	rBV3	902	457	0.03%	0.003%
11	3.355	718	720	723	rBV4	680	344	0.02%	0.003%
12	3.442	745	747	748	rBV2	858	294	0.02%	0.002%
13	3.468	748	755	758	rVV8	1833	2619	0.15%	0.019%
14	3.503	762	766	767	rBV4	1834	1205	0.07%	0.009%
15	3.596	793	795	798	rBV4	780	551	0.03%	0.004%
16	3.677	818	820	824	rBV5	1583	891	0.05%	0.007%
17	3.696	824	826	827	rBV2	826	295	0.02%	0.002%
18	3.728	833	836	839	rBV5	1482	940	0.05%	0.007%
19	3.744	839	841	842	rBV2	538	180	0.01%	0.001%
20	3.754	842	844	847	rBV3	983	527	0.03%	0.004%
21	3.793	852	856	858	rBV5	1358	1081	0.06%	0.008%
22	3.831	867	868	870	rBV2	716	225	0.01%	0.002%
23	3.847	870	873	875	rBV5	771	475	0.03%	0.004%
24	3.883	875	884	928	rBV2	109646	468638	27.18%	3.476%
25	4.333	1009	1024	1047	rBV	245416	646444	37.49%	4.795%
26	4.793	1161	1167	1169	rBV6	2507	2431	0.14%	0.018%
27	5.031	1225	1241	1275	rBV2	674835	1724125	100.00%	12.788%
28	5.513	1389	1391	1392	rBV2	1666	662	0.04%	0.005%
29	5.603	1406	1419	1448	rBV	583637	1202236	69.73%	8.917%
30	5.902	1500	1512	1531	rBV	343865	693397	40.22%	5.143%
31	6.059	1549	1561	1590	rVB	391710	822681	47.72%	6.102%
32	6.645	1733	1743	1747	rBV	5673	10749	0.62%	0.080%
33	6.934	1830	1833	1835	rBV4	1310	1085	0.06%	0.008%
34	6.979	1837	1847	1870	rVV	167917	326900	18.96%	2.425%
35	7.307	1938	1949	1970	rBV	707067	1257050	72.91%	9.323%
36	7.616	2036	2045	2072	rBV	107535	216163	12.54%	1.603%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
 Data File : VV028850.D
 Acq On : 03 Nov 2022 16:11
 Operator : SY/MD
 Sample : N5421-02ME
 Misc : 4.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1114ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	7.905	2133	2135	2137	rBV3	1445	892	0.05%	0.007%
38	8.091	2182	2193	2196	rBV	218579	319845	18.55%	2.372%
39	8.844	2416	2427	2458	rBV	793230	1464765	84.96%	10.864%
40	9.509	2632	2634	2635	rBV2	1288	467	0.03%	0.003%
41	9.886	2747	2751	2758	rBV9	3304	5083	0.29%	0.038%
42	10.214	2841	2853	2873	rBV	435871	820019	47.56%	6.082%
43	10.657	2990	2991	2993	rBV2	1668	718	0.04%	0.005%
44	11.242	3163	3173	3191	rBV	835102	1336758	77.53%	9.914%
45	11.490	3248	3250	3251	rBV2	1036	486	0.03%	0.004%
46	11.619	3279	3290	3310	rBV	693166	1126354	65.33%	8.354%
47	12.123	3446	3447	3454	rVB6	2601	2140	0.12%	0.016%
48	12.558	3580	3582	3584	rBV3	1458	803	0.05%	0.006%
49	12.789	3649	3654	3656	rBV5	3016	2521	0.15%	0.019%
50	12.850	3671	3673	3676	rBV4	1412	912	0.05%	0.007%
51	12.873	3676	3680	3685	rBV7	2805	3363	0.20%	0.025%
52	13.368	3833	3834	3836	rBV2	1337	683	0.04%	0.005%
53	13.776	3957	3961	3965	rBV7	2021	1816	0.11%	0.013%




Sum of corrected areas: 13482870

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
Data File : VV028850.D
Acq On : 03 Nov 2022 16:11
Operator : SY/MD
Sample : N5421-02ME
Misc : 4.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1114ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

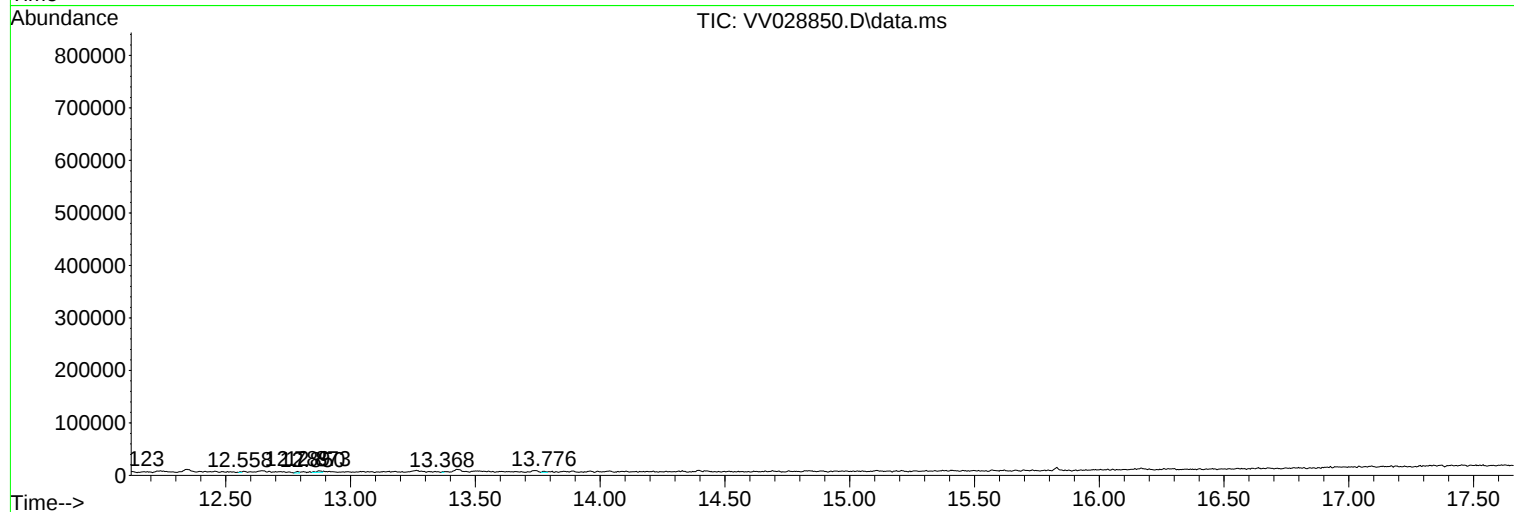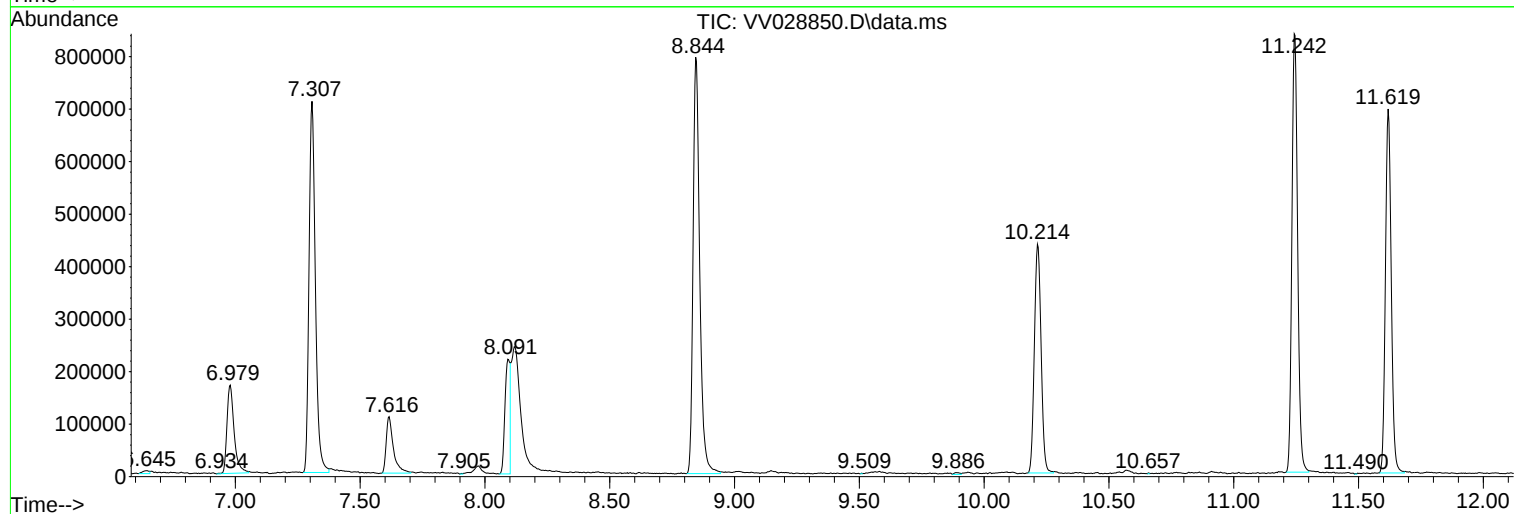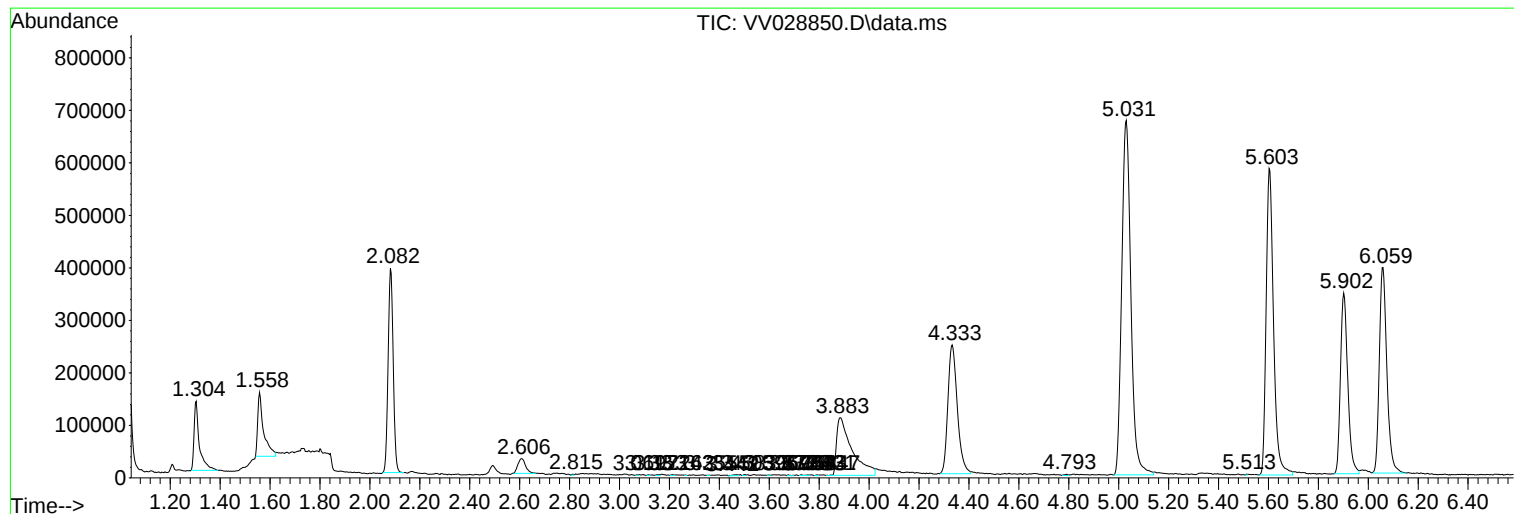

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
Data File : VV028850.D
Acq On : 03 Nov 2022 16:11
Operator : SY/MD
Sample : N5421-02ME
Misc : 4.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1114ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
Data File : VV028850.D
Acq On : 03 Nov 2022 16:11
Operator : SY/MD
Sample : N5421-02ME
Misc : 4.79g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1114ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------