
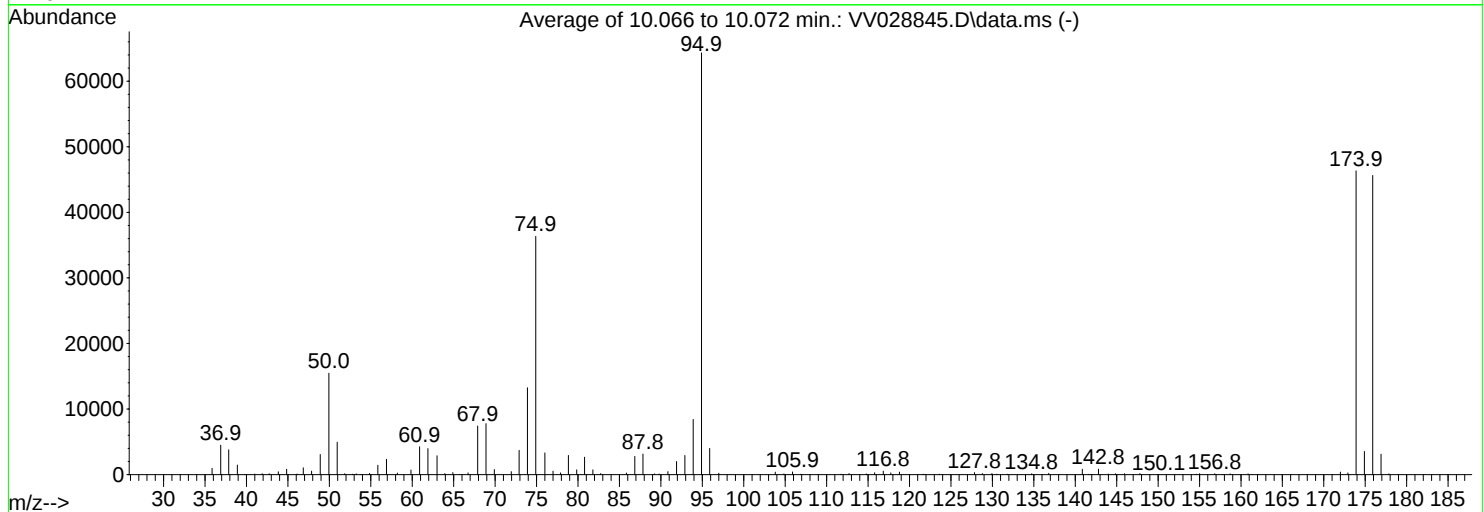


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110322\
 Data File : VV028845.D
 Acq On : 03 Nov 2022 09:01
 Operator : SY/MD
 Sample : BFB335
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB335

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 04 04:43:26 2022

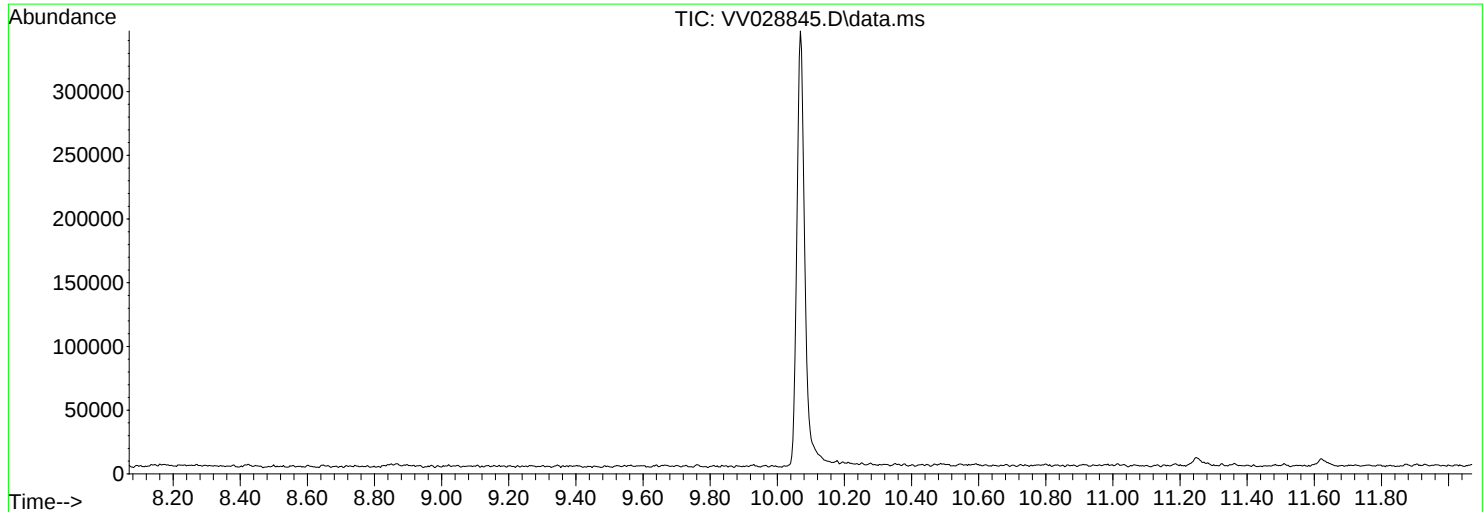

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	15473	PASS
75	95	30	80	56.5	36339	PASS
95	95	100	100	100.0	64320	PASS
96	95	5	9	6.2	4009	PASS
173	174	0.00	2	0.6	270	PASS
174	95	50	120	72.0	46339	PASS
175	174	5	9	7.7	3548	PASS
176	174	95	105	98.5	45637	PASS
177	176	5	10	6.8	3121	PASS

m/z	Abundance
35.90	360.0
37.80	217.0
38.90	260.0
39.80	1213.0
40.70	122.0
41.50	116.0
42.30	129.0
43.00	166.0
43.80	641.0
45.10	136.0
46.10	160.0
46.70	142.0
47.40	115.0
48.10	107.0
49.00	160.0
49.70	130.0
50.90	120.0
51.80	174.0
54.40	159.0
54.90	161.0
57.20	139.0
59.20	159.0
60.10	120.0
64.10	116.0
65.70	110.0
70.30	111.0
75.70	141.0
78.10	110.0
80.40	113.0
99.50	116.0
135.30	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335

m/z	Abundance
35.90	1440.0
36.90	4612.0
37.90	4062.0
38.90	1602.0
39.80	1203.0
41.00	138.0
41.90	157.0
42.70	216.0
43.90	1117.0
44.80	848.0
46.10	254.0
46.90	1075.0
47.90	524.0
48.90	3453.0
49.90	15307.0
51.00	5181.0
51.90	329.0
52.80	108.0
53.30	124.0
53.80	119.0
54.90	342.0
55.90	1477.0
56.90	2398.0
58.20	266.0
59.10	121.0
59.90	758.0
60.90	4084.0
61.90	3841.0
63.00	2916.0
63.90	258.0
64.80	322.0
65.70	140.0
66.80	259.0
67.90	7177.0
68.90	7817.0
69.90	668.0
72.00	504.0
72.90	3625.0
73.90	13055.0
74.90	35632.0
76.00	3195.0
77.00	450.0
77.90	378.0
78.90	2766.0
79.80	663.0
80.80	2709.0
81.80	713.0
82.80	205.0
85.80	216.0
86.90	2542.0
87.90	3048.0
89.30	120.0
90.90	453.0
91.90	1927.0
92.90	2906.0
93.90	8570.0
94.90	62552.0
95.90	4115.0
97.10	184.0
103.80	399.0
104.90	111.0
105.90	402.0
106.90	120.0
112.70	161.0
114.80	103.0
115.80	337.0
116.90	511.0
117.70	290.0
118.80	392.0
123.60	127.0
127.80	350.0
128.90	190.0
129.90	181.0
134.80	131.0
136.70	194.0
140.80	722.0
141.90	134.0
142.80	827.0
144.90	118.0
146.00	164.0
147.80	168.0
154.90	138.0
156.80	178.0
160.80	118.0
172.00	401.0
173.90	43944.0
174.90	3437.0
175.90	43776.0
176.90	3031.0
177.80	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335

m/z	Abundance
35.90	1361.0
36.90	4668.0
37.90	4158.0
38.90	1798.0
39.80	1229.0
41.00	125.0
41.30	119.0
41.90	162.0
42.80	207.0
43.90	1113.0
44.80	850.0
46.10	278.0
46.90	1214.0
47.90	550.0
48.90	3265.0
50.00	15995.0
51.00	5202.0
51.90	317.0
52.80	110.0
53.20	112.0
54.90	380.0
55.90	1488.0
56.90	2447.0
58.20	200.0
59.90	694.0
60.90	4420.0
61.90	4104.0
63.00	2981.0
63.90	297.0
64.90	336.0
65.70	131.0
66.80	280.0
67.90	7678.0
68.90	8039.0
69.90	808.0
72.00	472.0
72.90	3865.0
73.90	13763.0
74.90	37464.0
76.00	3446.0
77.00	567.0
77.90	392.0
78.80	3004.0
79.80	775.0
80.80	2723.0
81.80	781.0
82.80	193.0
85.80	275.0
86.80	2847.0
87.80	3283.0
89.30	125.0
89.80	133.0
90.80	479.0
91.90	2059.0
92.90	3000.0
93.90	8723.0
94.90	66808.0
95.90	4023.0
97.00	237.0
103.80	417.0
104.80	127.0
105.90	437.0
106.90	115.0
111.80	112.0
112.70	173.0
114.80	131.0
115.80	312.0
116.80	549.0
117.70	296.0
118.80	392.0
121.70	121.0
123.60	106.0
127.80	294.0
128.80	183.0
130.00	172.0
130.60	120.0
131.80	124.0
134.80	133.0
136.80	202.0
140.90	898.0
141.60	124.0
142.80	875.0
144.00	128.0
144.80	157.0
146.00	179.0
147.80	161.0
150.10	112.0
154.60	116.0
155.00	149.0
156.80	161.0
158.70	146.0
160.90	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335

172.00	407.0
173.90	48088.0
174.90	3649.0
175.90	47632.0
176.90	3223.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335

m/z	Abundance
35.90	1246.0
36.90	4209.0
37.90	3775.0
38.90	1798.0
39.80	1255.0
41.40	149.0
41.90	146.0
43.00	190.0
43.90	1043.0
44.90	776.0
46.10	246.0
46.90	1274.0
47.80	531.0
48.90	2969.0
50.00	15117.0
51.00	4812.0
51.90	306.0
53.20	101.0
54.20	113.0
54.80	354.0
55.80	1344.0
56.90	2204.0
58.00	144.0
58.30	146.0
59.80	648.0
60.90	4215.0
61.90	4000.0
63.00	2775.0
63.90	323.0
65.00	322.0
65.70	115.0
66.70	269.0
67.90	7409.0
68.90	7487.0
69.90	903.0
71.90	394.0
72.90	3676.0
73.90	12914.0
74.90	35920.0
76.00	3288.0
77.00	583.0
77.90	343.0
78.80	3015.0
79.90	770.0
80.80	2568.0
81.80	739.0
82.70	139.0
85.90	282.0
86.80	2967.0
87.80	3153.0
89.20	124.0
89.80	165.0
90.80	463.0
91.90	2005.0
92.90	2872.0
93.90	7993.0
94.90	63600.0
95.90	3889.0
96.90	229.0
103.80	359.0
104.80	127.0
105.90	395.0
111.00	114.0
111.70	140.0
112.70	172.0
114.80	147.0
115.80	236.0
116.80	538.0
117.80	257.0
118.80	375.0
121.60	114.0
121.90	120.0
127.90	284.0
128.70	156.0
130.00	187.0
130.50	140.0
131.80	122.0
134.70	145.0
136.90	195.0
140.90	880.0
142.80	828.0
144.00	151.0
144.80	176.0
145.90	127.0
147.80	178.0
148.90	107.0
154.60	140.0
155.10	159.0
156.90	137.0
157.80	109.0
158.70	204.0
160.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335

169.00	115.0
172.00	376.0
172.90	809.0
173.90	46984.0
174.90	3558.0
175.90	45504.0
176.90	3109.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB335