


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110323\
Data File : VV032831.D
Acq On : 02 Nov 2023 08:23
Operator : SY/MD
Sample : BFB253
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB253

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM101323.M
Title : TRACE VOA SOM01.0
Last Update : Mon Oct 16 02:50:34 2023

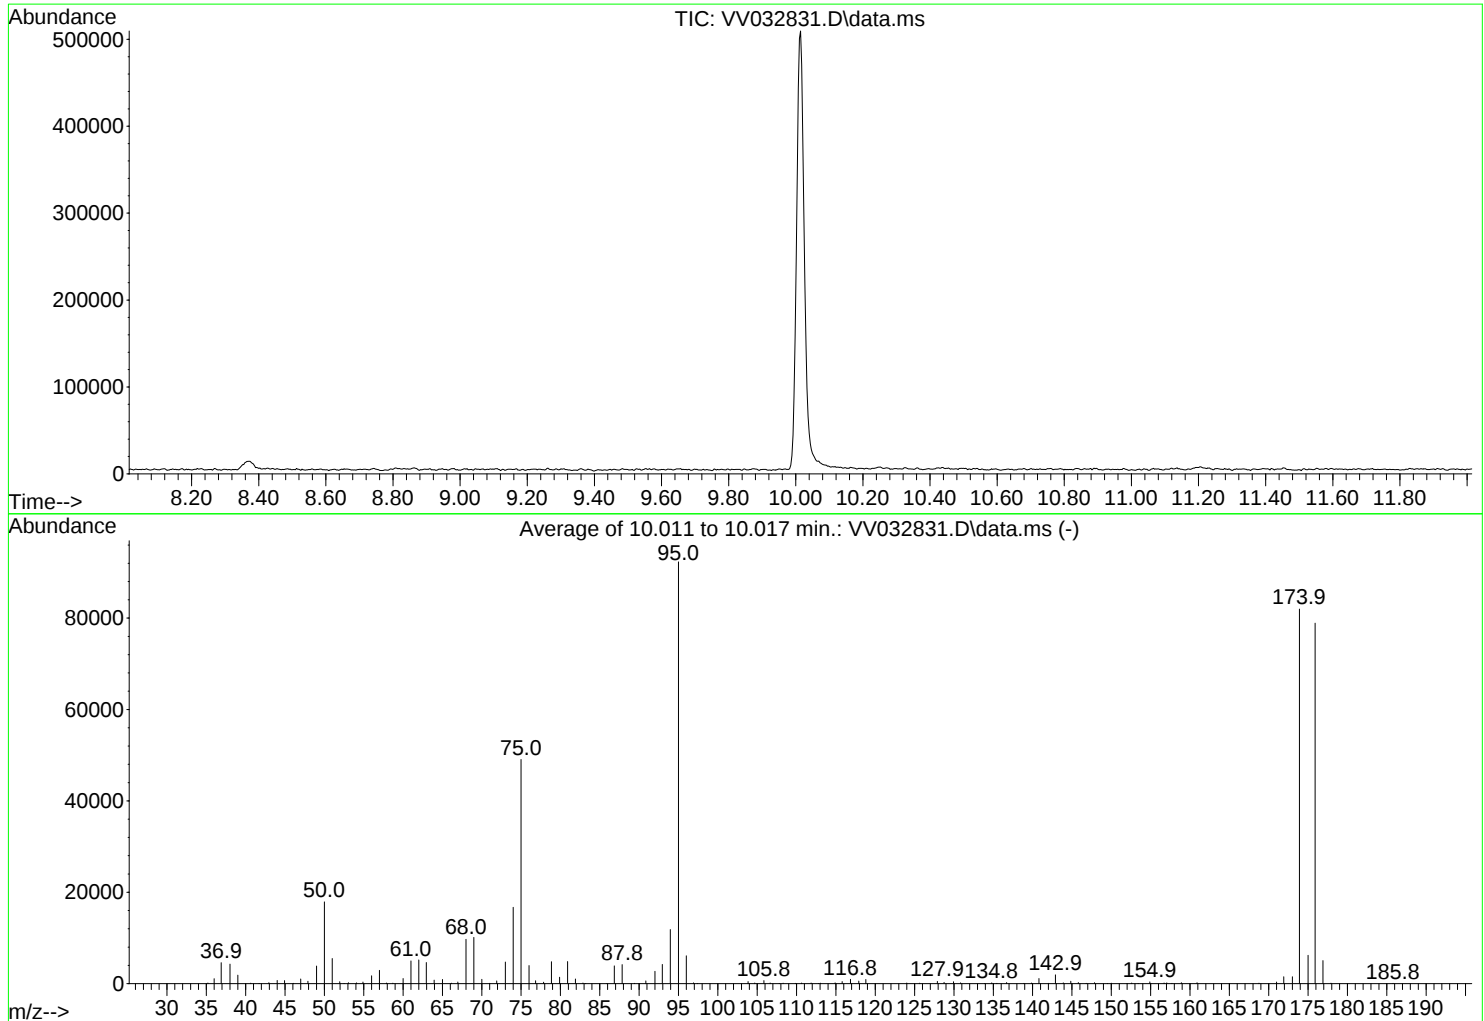

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	17909	PASS
75	95	30	80	53.2	49077	PASS
95	95	100	100	100.0	92315	PASS
96	95	5	9	6.6	6085	PASS
173	174	0.00	2	1.8	1509	PASS
174	95	50	120	88.8	81987	PASS
175	174	5	9	7.6	6204	PASS
176	174	95	101	96.2	78901	PASS
177	176	5	9	6.4	5053	PASS

m/z	Abundance
35.50	185.0
36.90	183.0
37.60	132.0
38.50	236.0
39.80	307.0
41.10	150.0
41.80	125.0
42.70	186.0
43.30	145.0
44.00	465.0
45.00	149.0
46.00	133.0
47.40	154.0
48.40	175.0
49.10	107.0
49.70	167.0
53.20	107.0
55.60	129.0
58.00	139.0
64.40	116.0
65.20	125.0
65.60	121.0
66.40	107.0
67.60	102.0
75.30	139.0
78.80	121.0
81.10	101.0
82.30	153.0
84.10	139.0
85.30	100.0
103.00	145.0
104.60	144.0
110.00	104.0
144.10	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
35.20	239.0
36.00	1222.0
36.90	4952.0
38.00	4493.0
39.00	1997.0
39.90	332.0
41.60	182.0
42.50	135.0
43.00	216.0
44.00	1131.0
44.90	831.0
47.10	958.0
47.90	529.0
49.00	3967.0
50.00	18640.0
51.00	5578.0
51.90	423.0
53.00	335.0
54.10	218.0
54.90	359.0
56.00	1642.0
57.00	3080.0
57.90	290.0
58.70	101.0
60.00	1110.0
61.00	5036.0
62.00	5262.0
62.90	4771.0
63.90	885.0
65.00	1117.0
65.80	199.0
66.90	386.0
68.00	10155.0
69.00	10374.0
70.00	947.0
71.90	665.0
73.00	5006.0
74.00	16768.0
75.00	50704.0
76.00	4139.0
77.00	607.0
77.80	544.0
78.90	5073.0
79.90	1455.0
80.90	4836.0
81.90	1065.0
82.90	157.0
85.90	162.0
86.80	4039.0
87.90	4177.0
89.40	114.0
90.00	110.0
90.80	525.0
92.00	2639.0
93.00	4521.0
94.00	11645.0
95.00	94424.0
96.00	6343.0
96.90	180.0
103.90	473.0
104.80	298.0
105.90	791.0
106.70	129.0
108.30	101.0
109.90	162.0
110.70	127.0
111.80	165.0
112.80	156.0
114.80	218.0
115.80	453.0
116.80	931.0
117.90	648.0
118.80	953.0
124.00	216.0
125.70	113.0
127.90	509.0
128.70	279.0
129.90	438.0
130.90	195.0
134.90	176.0
136.70	198.0
138.90	104.0
139.80	143.0
140.80	1070.0
142.90	2066.0
143.90	255.0
144.90	567.0
145.80	199.0
146.80	109.0
147.90	231.0
152.60	120.0
153.40	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

154.90	323.0
156.70	152.0
157.00	189.0
158.90	110.0
160.80	156.0
168.70	110.0
171.00	316.0
171.90	1388.0
173.00	1403.0
173.90	81976.0
175.00	6499.0
175.90	78528.0
176.90	5034.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
35.20	193.0
36.00	1112.0
36.90	4890.0
38.00	4378.0
39.00	1844.0
40.00	277.0
40.60	161.0
41.60	148.0
42.90	206.0
44.00	1187.0
44.90	821.0
46.20	297.0
46.90	1037.0
47.90	513.0
49.00	4108.0
50.00	18472.0
51.00	5599.0
52.00	430.0
53.00	330.0
54.10	190.0
54.90	380.0
56.00	1805.0
57.00	2946.0
57.90	301.0
58.70	117.0
60.00	1168.0
61.00	5136.0
62.00	5275.0
63.00	4757.0
64.00	768.0
65.00	1066.0
66.10	171.0
66.90	363.0
68.00	9985.0
69.00	10563.0
70.00	965.0
71.00	130.0
71.90	584.0
73.00	4925.0
74.00	17216.0
75.00	50648.0
76.00	4053.0
76.80	649.0
77.90	409.0
78.90	5070.0
79.90	1447.0
80.90	5170.0
81.90	1042.0
82.90	124.0
83.20	131.0
86.90	4001.0
87.90	4291.0
89.40	125.0
90.80	614.0
92.00	2760.0
92.90	4264.0
93.90	12185.0
95.00	95312.0
96.00	6290.0
96.90	184.0
103.80	469.0
104.80	292.0
105.80	686.0
106.60	129.0
108.30	119.0
109.80	173.0
110.60	130.0
111.80	145.0
113.00	164.0
114.90	183.0
115.80	488.0
116.80	956.0
117.90	599.0
118.80	954.0
124.00	155.0
125.70	133.0
127.90	502.0
128.70	308.0
130.00	434.0
130.80	193.0
134.80	196.0
135.40	107.0
136.70	250.0
138.90	102.0
139.80	165.0
140.80	1174.0
142.90	1976.0
143.90	280.0
144.90	525.0
145.80	280.0
146.80	112.0
147.90	220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

149.50	112.0
150.00	131.0
152.60	128.0
154.90	301.0
156.70	151.0
157.10	189.0
157.70	112.0
158.90	219.0
160.90	197.0
168.80	127.0
171.00	332.0
171.90	1586.0
173.00	1595.0
173.90	84880.0
175.00	6475.0
175.90	81328.0
176.90	5305.0
177.90	120.0
185.80	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

m/z	Abundance
36.00	884.0
37.00	4431.0
38.00	3935.0
39.00	1700.0
39.90	248.0
40.70	171.0
41.30	128.0
41.70	131.0
42.90	204.0
44.00	1138.0
45.00	809.0
46.10	301.0
47.00	1096.0
47.90	541.0
49.00	3818.0
50.00	16616.0
51.00	5293.0
52.00	392.0
52.50	166.0
53.00	277.0
54.10	125.0
54.90	353.0
56.00	1736.0
57.00	2656.0
57.90	261.0
58.70	128.0
60.00	1070.0
61.00	4798.0
62.00	4996.0
63.00	4300.0
64.00	669.0
65.00	922.0
66.20	140.0
67.00	299.0
68.00	8988.0
69.00	9476.0
70.00	885.0
71.00	130.0
71.90	510.0
73.00	4286.0
74.00	16115.0
75.00	45880.0
76.00	3680.0
76.80	616.0
78.90	4615.0
79.90	1306.0
80.90	4807.0
81.90	985.0
82.70	100.0
86.90	3637.0
87.80	3992.0
90.90	678.0
92.00	2724.0
92.90	3826.0
93.90	11661.0
95.00	87208.0
96.00	5622.0
96.90	164.0
97.40	112.0
103.80	472.0
104.80	234.0
105.80	556.0
106.60	159.0
107.80	117.0
108.30	113.0
109.80	144.0
110.60	134.0
111.90	128.0
113.10	187.0
115.00	132.0
115.80	456.0
116.90	933.0
117.90	467.0
118.80	857.0
125.60	121.0
127.90	470.0
128.80	290.0
130.00	358.0
130.80	193.0
133.90	102.0
134.70	204.0
135.50	106.0
136.70	280.0
139.90	142.0
140.80	1133.0
142.00	207.0
142.90	1793.0
143.90	310.0
144.80	459.0
145.80	275.0
147.70	216.0
150.00	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253

152.00	110.0
152.60	155.0
154.70	274.0
155.00	271.0
156.70	160.0
157.10	190.0
157.70	124.0
158.90	297.0
161.00	249.0
168.80	129.0
171.00	370.0
171.90	1549.0
173.00	1530.0
173.90	79104.0
175.00	5637.0
175.90	76848.0
176.90	4820.0
177.90	108.0
185.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB253