

m/z	Abundance
35.10	174.0
36.00	2186.0
37.00	10419.0
38.00	8812.0
39.00	4035.0
40.00	1443.0
41.10	272.0
42.20	196.0
43.00	337.0
44.00	2116.0
45.00	2018.0
46.00	443.0
47.10	3128.0
48.00	1216.0
49.00	8595.0
50.00	38904.0
51.10	12095.0
52.00	675.0
52.80	406.0
53.90	167.0
54.90	568.0
56.00	3052.0
57.00	5213.0
57.90	387.0
58.40	224.0
58.90	223.0
60.00	1800.0
61.00	9972.0
62.00	9383.0
63.10	7437.0
64.00	1515.0
65.00	1829.0
66.20	259.0
67.00	929.0
68.00	20560.0
69.00	19616.0
70.00	1517.0
72.10	1562.0
73.00	9171.0
74.00	33280.0
75.00	102904.0
76.00	9102.0
77.00	1460.0
77.90	1192.0
79.00	6108.0
80.00	1887.0
80.90	6321.0
81.90	1222.0
82.90	290.0
85.10	145.0
85.90	382.0
87.00	9335.0
88.00	9024.0
89.40	112.0
90.90	908.0
92.00	5460.0
93.00	9627.0
94.00	24400.0
95.00	204224.0
96.00	14004.0
97.00	458.0
102.70	178.0
103.10	205.0
103.90	914.0
105.00	256.0
105.90	811.0
106.80	287.0
108.10	179.0
109.10	115.0
109.80	208.0
111.00	239.0
111.90	184.0
112.70	267.0
115.00	241.0
115.80	904.0
117.00	1478.0
117.90	615.0
118.90	1659.0
119.90	128.0
120.50	132.0
124.00	207.0
126.00	119.0
127.80	672.0
128.90	364.0
129.80	781.0
130.90	425.0
133.80	125.0
134.20	119.0
135.00	709.0
136.80	326.0
137.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

138.90	132.0
139.60	293.0
140.10	183.0
141.00	2091.0
143.00	3101.0
144.00	206.0
144.90	1102.0
145.80	371.0
146.80	162.0
148.00	556.0
148.80	232.0
150.00	268.0
152.10	197.0
152.80	121.0
153.00	119.0
153.80	154.0
155.10	531.0
155.70	131.0
156.40	143.0
157.10	517.0
159.00	303.0
160.90	273.0
166.80	145.0
168.70	114.0
170.10	237.0
171.20	461.0
171.90	2587.0
174.00	187904.0
175.00	14147.0
175.90	178880.0
176.90	11591.0
178.00	502.0
194.10	120.0
207.20	184.0
218.80	148.0
221.60	106.0
227.00	123.0
232.00	108.0
284.90	104.0
295.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
35.10	195.0
36.00	2373.0
37.00	10503.0
38.10	9374.0
39.00	4125.0
40.00	1420.0
41.20	260.0
42.20	219.0
43.00	330.0
44.10	2184.0
45.00	2045.0
46.00	412.0
47.10	3151.0
48.00	1404.0
49.00	8891.0
50.00	40400.0
51.10	12765.0
52.00	843.0
52.80	349.0
53.40	165.0
53.70	144.0
55.00	545.0
56.00	3029.0
57.00	5351.0
58.00	394.0
59.00	222.0
60.00	1992.0
61.00	10409.0
62.00	10524.0
63.00	8314.0
64.00	1466.0
65.10	1995.0
66.10	268.0
67.00	773.0
68.00	22280.0
69.00	20768.0
70.00	1689.0
71.10	253.0
72.00	1607.0
73.00	9408.0
74.00	35920.0
75.00	108448.0
76.00	9874.0
77.00	1449.0
77.90	1309.0
78.90	6202.0
80.00	1988.0
80.90	6717.0
81.90	1367.0
83.00	313.0
83.90	108.0
85.10	130.0
87.00	8928.0
88.00	9328.0
89.80	104.0
91.00	943.0
92.00	5945.0
93.00	9968.0
94.00	25960.0
95.00	218944.0
96.00	14743.0
97.00	451.0
102.60	224.0
103.20	212.0
103.90	998.0
105.00	278.0
105.90	889.0
106.80	298.0
108.00	217.0
109.10	109.0
109.90	210.0
111.00	331.0
112.00	212.0
112.70	210.0
113.80	103.0
115.00	310.0
115.80	875.0
117.00	1510.0
117.90	693.0
118.90	1675.0
120.50	125.0
122.50	101.0
123.90	252.0
124.80	103.0
125.80	107.0
127.90	841.0
129.00	393.0
129.90	737.0
130.90	423.0
131.90	108.0
133.00	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

134.20	132.0
135.00	724.0
136.20	107.0
136.80	440.0
138.90	143.0
139.70	322.0
141.00	2212.0
141.90	339.0
142.90	3266.0
143.90	251.0
145.00	1253.0
145.80	467.0
146.80	144.0
148.00	599.0
148.80	232.0
149.70	244.0
150.20	303.0
151.70	128.0
152.20	171.0
153.10	161.0
153.90	181.0
155.10	585.0
157.10	570.0
158.70	302.0
159.10	293.0
160.90	364.0
166.90	128.0
170.10	246.0
170.70	475.0
172.00	2548.0
173.00	2852.0
174.00	203776.0
175.00	15388.0
175.90	194176.0
176.90	12434.0
178.00	424.0
194.00	125.0
207.20	180.0
226.90	103.0
232.20	140.0
233.20	106.0
244.10	141.0
270.40	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
35.80	278.0
36.80	102.0
37.70	160.0
40.00	1255.0
41.00	253.0
42.00	209.0
43.10	237.0
43.90	1405.0
46.00	142.0
46.80	128.0
47.90	104.0
48.70	137.0
49.50	165.0
51.30	119.0
53.30	145.0
54.60	127.0
54.90	132.0
56.20	177.0
59.50	115.0
61.10	142.0
63.00	229.0
64.20	143.0
64.90	120.0
65.40	119.0
66.20	105.0
66.90	169.0
68.30	135.0
70.80	102.0
73.50	136.0
74.40	107.0
75.30	127.0
77.00	114.0
79.20	106.0
81.20	124.0
87.30	132.0
88.90	141.0
89.80	138.0
90.70	117.0
93.60	148.0
95.40	142.0
96.00	149.0
96.80	115.0
99.70	102.0
102.00	138.0
107.40	137.0
116.50	125.0
118.40	166.0
122.50	119.0
125.80	109.0
133.00	178.0
136.20	125.0
138.90	130.0
140.40	127.0
144.00	130.0
151.60	104.0
153.70	123.0
158.30	113.0
160.30	120.0
177.10	109.0
194.00	143.0
196.90	161.0
197.90	166.0
206.90	130.0
210.00	101.0
212.60	117.0
217.40	122.0
226.30	164.0
238.90	103.0
239.50	133.0
240.50	106.0
241.50	114.0
260.60	103.0
265.10	103.0
281.10	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	2298.0
37.00	9916.0
38.10	8972.0
39.00	3902.0
40.00	1393.0
41.30	222.0
42.10	211.0
42.40	215.0
43.00	345.0
44.10	2293.0
45.00	1858.0
46.00	281.0
47.10	2822.0
48.00	1447.0
49.00	8271.0
50.10	37624.0
51.10	12208.0
52.00	834.0
52.80	284.0
53.40	200.0
55.00	538.0
56.00	2886.0
57.00	5158.0
58.00	438.0
59.00	209.0
60.00	1978.0
61.00	9898.0
62.00	10549.0
63.00	8089.0
64.00	1280.0
65.10	2050.0
65.90	301.0
67.00	603.0
68.00	21464.0
69.00	19624.0
70.00	1749.0
71.10	257.0
72.00	1421.0
73.00	9095.0
74.00	34232.0
75.00	103448.0
76.00	9148.0
77.00	1240.0
78.00	1136.0
78.90	5968.0
80.00	1813.0
80.90	6401.0
81.90	1353.0
83.00	288.0
83.80	130.0
85.30	157.0
86.20	441.0
87.00	8092.0
88.00	8774.0
89.90	116.0
91.00	859.0
92.00	6119.0
93.00	9408.0
94.00	24912.0
95.00	212864.0
96.00	13981.0
97.00	387.0
100.80	119.0
102.60	236.0
103.20	224.0
103.90	882.0
105.00	309.0
106.00	900.0
106.80	331.0
108.00	184.0
109.20	105.0
109.90	199.0
111.00	397.0
111.90	230.0
112.90	155.0
113.90	105.0
115.00	303.0
115.90	784.0
116.90	1421.0
117.90	729.0
118.90	1454.0
120.40	130.0
121.10	123.0
124.00	250.0
124.90	140.0
125.70	124.0
127.90	878.0
129.10	364.0
129.90	738.0
130.80	452.0
131.90	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

133.00	117.0
135.00	630.0
135.70	102.0
136.10	132.0
136.80	514.0
138.50	119.0
138.90	126.0
139.70	265.0
141.00	2064.0
142.00	308.0
142.90	3207.0
143.90	260.0
145.00	1229.0
145.90	541.0
146.80	122.0
147.90	561.0
148.80	180.0
149.70	194.0
150.20	300.0
151.70	132.0
152.10	117.0
153.10	183.0
154.00	216.0
155.10	539.0
155.80	112.0
157.00	563.0
158.70	390.0
159.10	323.0
160.90	411.0
170.30	228.0
170.70	503.0
171.20	511.0
172.00	2542.0
173.00	2640.0
174.00	200128.0
175.00	15115.0
176.00	191744.0
177.00	12394.0
178.10	349.0
207.20	108.0
232.20	117.0
244.10	149.0
280.80	103.0


Instrument :
MSVOA_V
ClientSampleId :
BFB54

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110419\
 Data File : VV013475.D
 Acq On : 04 Nov 2019 14:11
 Operator : SY/MD
 Sample : BFB54
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB54

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR103119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Nov 05 07:17:32 2019

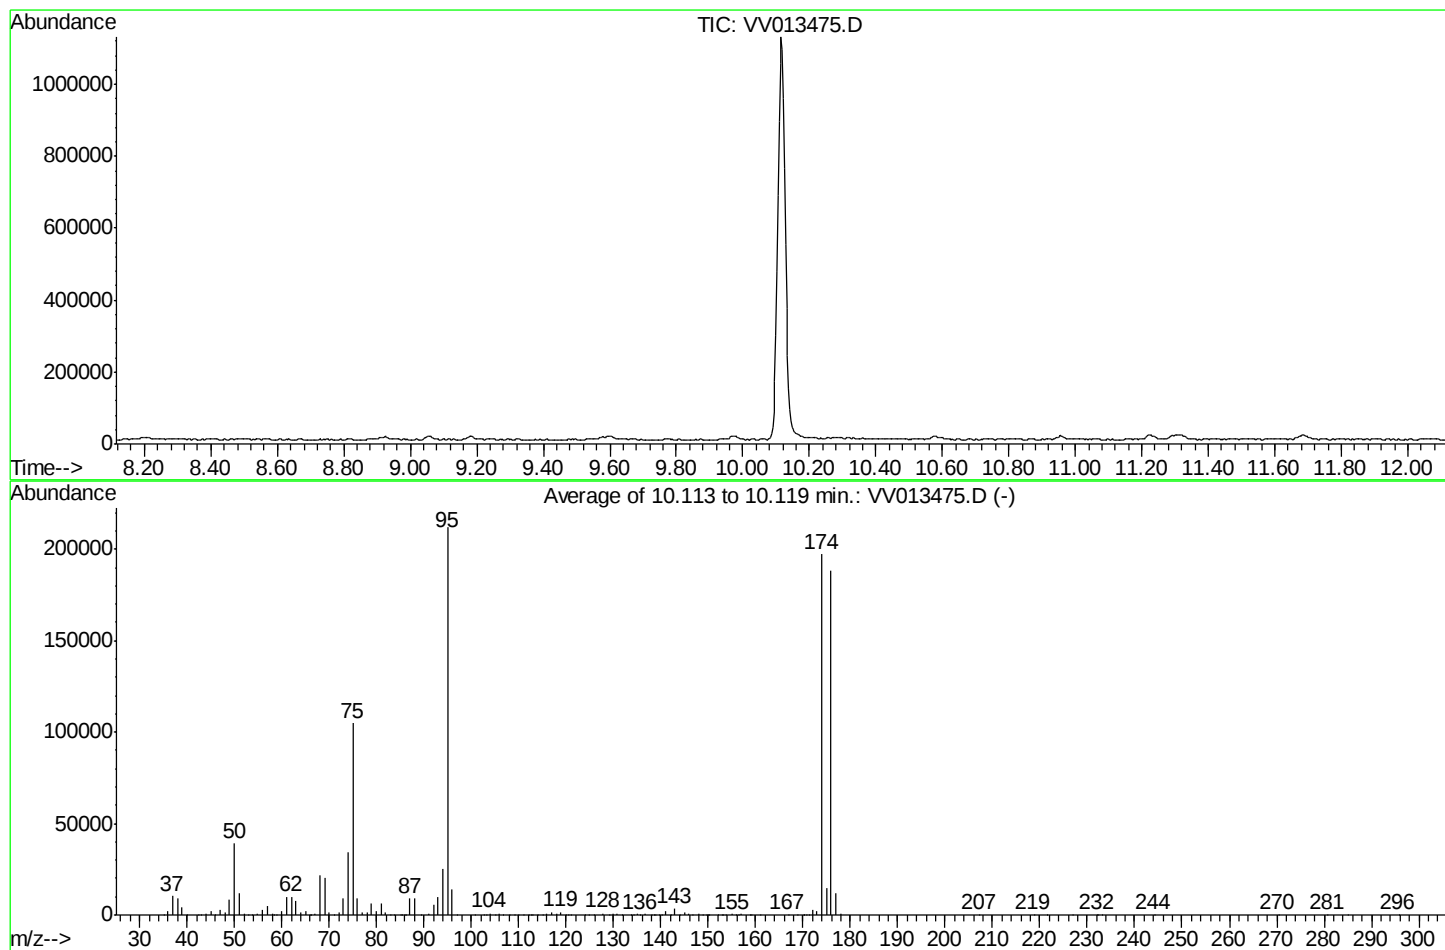

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	38976	PASS
75	95	30	80	49.5	104933	PASS
95	95	100	100	100.0	212010	PASS
96	95	5	9	6.6	14093	PASS
173	174	0.00	2	0.9	1830	PASS
174	95	50	120	93.0	197269	PASS
175	174	5	9	7.5	14883	PASS
176	174	95	101	95.4	188266	PASS
177	176	5	9	6.4	12030	PASS