

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110420\
 Data File : VV019231.D
 Acq On : 03 Nov 2020 12:50
 Operator : SY/MD
 Sample : VV1104WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK312

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	86	rVB	142902	142765	14.36%	1.904%
2	1.579	144	152	164	rBV	126705	143067	14.39%	1.908%
3	2.122	311	321	349	rVB	258631	382921	38.51%	5.106%
4	2.309	374	379	386	rVB3	799	1085	0.11%	0.014%
5	2.521	441	445	454	rVB4	986	1420	0.14%	0.019%
6	2.598	467	469	473	rBV	221	103	0.01%	0.001%
7	2.640	478	482	485	rBV3	386	334	0.03%	0.004%
8	2.746	512	515	519	rBV2	199	174	0.02%	0.002%
9	2.843	543	545	547	rVB	222	91	0.01%	0.001%
10	2.859	547	550	551	rBV	252	143	0.01%	0.002%
11	2.920	566	569	571	rBV2	173	129	0.01%	0.002%
12	2.962	578	582	585	rBV2	262	204	0.02%	0.003%
13	3.071	614	616	617	rBV2	121	51	0.01%	0.001%
14	3.151	637	641	643	rBV	309	263	0.03%	0.004%
15	3.306	687	689	690	rBV	161	51	0.01%	0.001%
16	3.547	757	764	769	rBV2	372	517	0.05%	0.007%
17	3.798	839	842	848	rBV	181	111	0.01%	0.001%
18	3.823	848	850	852	rBV	109	69	0.01%	0.001%
19	3.859	857	861	866	rBV2	254	298	0.03%	0.004%
20	3.907	866	876	919	rBV	64145	189473	19.06%	2.526%
21	4.373	1007	1021	1048	rVB2	161447	393413	39.57%	5.246%
22	4.550	1073	1076	1077	rBV	217	119	0.01%	0.002%
23	4.611	1092	1095	1097	rBV2	240	185	0.02%	0.002%
24	4.772	1142	1145	1148	rVB2	197	160	0.02%	0.002%
25	4.788	1149	1150	1153	rBV	127	69	0.01%	0.001%
26	4.843	1164	1167	1170	rVB	249	160	0.02%	0.002%
27	4.862	1170	1173	1174	rBV	306	205	0.02%	0.003%
28	4.994	1209	1214	1220	rVB2	285	344	0.03%	0.005%
29	5.071	1220	1238	1263	rBV2	383319	994264	100.00%	13.257%
30	5.315	1309	1314	1316	rBV	471	368	0.04%	0.005%
31	5.434	1349	1351	1356	rVB2	334	182	0.02%	0.002%
32	5.457	1356	1358	1359	rBV2	201	81	0.01%	0.001%
33	5.640	1402	1415	1442	rBV	297510	592940	59.64%	7.906%
34	5.929	1496	1505	1523	rVB3	8738	18058	1.82%	0.241%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110420\
 Data File : VV019231.D
 Acq On : 03 Nov 2020 12:50
 Operator : SY/MD
 Sample : VV1104WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK312

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
 Title : VOC Analysis

35	6.093	1542	1556	1576	rBV	214248	431798	43.43%	5.757%
36	6.341	1630	1633	1634	rBV	102	50	0.01%	0.001%
37	6.373	1640	1643	1645	rBV2	214	151	0.02%	0.002%
38	6.402	1651	1652	1654	rVB	141	37	0.00%	0.000%
39	6.412	1654	1655	1659	rVB	139	61	0.01%	0.001%
40	6.534	1688	1693	1694	rBV	232	193	0.02%	0.003%
41	6.611	1715	1717	1721	rBV	193	163	0.02%	0.002%
42	6.769	1764	1766	1769	rVB	176	121	0.01%	0.002%
43	6.788	1769	1772	1774	rBV	267	182	0.02%	0.002%
44	6.852	1789	1792	1795	rVB	307	212	0.02%	0.003%
45	6.881	1795	1801	1802	rBV	273	205	0.02%	0.003%
46	6.961	1824	1826	1829	rVB2	260	147	0.01%	0.002%
47	7.007	1829	1840	1859	rBV	128008	230140	23.15%	3.069%
48	7.138	1879	1881	1883	rVB2	521	139	0.01%	0.002%
49	7.209	1902	1903	1904	rVB2	185	36	0.00%	0.000%
50	7.228	1907	1909	1912	rVV	306	106	0.01%	0.001%
51	7.338	1931	1943	1963	rBV	459152	787601	79.21%	10.501%
52	7.563	2011	2013	2017	rBV2	313	248	0.02%	0.003%
53	7.640	2027	2037	2066	rBV	91020	161677	16.26%	2.156%
54	7.839	2096	2099	2102	rVB3	403	293	0.03%	0.004%
55	7.936	2127	2129	2131	rBV	180	105	0.01%	0.001%
56	8.010	2150	2152	2154	rBV	160	73	0.01%	0.001%
57	8.045	2162	2163	2165	rVB	205	71	0.01%	0.001%
58	8.106	2172	2182	2217	rBV	215677	393412	39.57%	5.246%
59	8.392	2269	2271	2273	rBV2	246	147	0.01%	0.002%
60	8.524	2311	2312	2313	rBV	228	64	0.01%	0.001%
61	8.678	2352	2360	2362	rBV2	281	391	0.04%	0.005%
62	8.695	2362	2365	2367	rVV2	181	117	0.01%	0.002%
63	8.762	2379	2386	2389	rBV	468	544	0.05%	0.007%
64	8.871	2408	2420	2445	rBV	452829	727191	73.14%	9.696%
65	9.228	2527	2531	2535	rBV	309	342	0.03%	0.005%
66	9.286	2547	2549	2552	rBV2	142	100	0.01%	0.001%
67	9.322	2557	2560	2565	rVB	358	283	0.03%	0.004%
68	9.473	2605	2607	2611	rVB	226	134	0.01%	0.002%
69	9.559	2632	2634	2636	rBV	150	59	0.01%	0.001%
70	9.576	2636	2639	2642	rBV2	269	218	0.02%	0.003%
71	9.852	2722	2725	2729	rBV	265	223	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110420\
 Data File : VV019231.D
 Acq On : 03 Nov 2020 12:50
 Operator : SY/MD
 Sample : VV1104WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK312

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
 Title : VOC Analysis

72	9.997	2767	2770	2774	rVB	337	243	0.02%	0.003%
73	10.022	2775	2778	2782	rVV	290	204	0.02%	0.003%
74	10.077	2790	2795	2798	rBV	303	348	0.04%	0.005%
75	10.112	2803	2806	2807	rBV	237	159	0.02%	0.002%
76	10.141	2811	2815	2816	rBV	685	517	0.05%	0.007%
77	10.235	2832	2844	2860	rBV	262523	413744	41.61%	5.517%
78	10.341	2875	2877	2882	rVB2	342	176	0.02%	0.002%
79	10.405	2894	2897	2902	rBV2	168	201	0.02%	0.003%
80	10.624	2963	2965	2969	rBV	314	160	0.02%	0.002%
81	10.659	2970	2976	2979	rBV	238	299	0.03%	0.004%
82	10.733	2997	2999	3003	rVB	347	200	0.02%	0.003%
83	10.768	3003	3010	3013	rBV2	276	358	0.04%	0.005%
84	10.945	3057	3065	3070	rBV3	783	1054	0.11%	0.014%
85	10.987	3076	3078	3081	rBV	285	143	0.01%	0.002%
86	11.209	3144	3147	3150	rBV2	524	306	0.03%	0.004%
87	11.270	3154	3166	3188	rBV	472372	721301	72.55%	9.617%
88	11.392	3202	3204	3207	rBV2	373	229	0.02%	0.003%
89	11.534	3246	3248	3250	rBV	179	92	0.01%	0.001%
90	11.646	3271	3283	3307	rBV	487436	757340	76.17%	10.098%
91	12.045	3400	3407	3409	rBV2	348	351	0.04%	0.005%
92	12.344	3497	3500	3503	rBV2	253	208	0.02%	0.003%
93	12.646	3592	3594	3597	rBV	252	150	0.02%	0.002%
94	12.659	3597	3598	3601	rVV	295	170	0.02%	0.002%
95	13.328	3803	3806	3807	rBV	206	134	0.01%	0.002%
96	13.611	3890	3894	3901	rBV2	424	486	0.05%	0.006%
97	13.807	3953	3955	3957	rBV	314	191	0.02%	0.003%
98	14.353	4120	4125	4127	rBV2	443	373	0.04%	0.005%


Sum of corrected areas: 7499988

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110420\
Data File : VV019231.D
Acq On : 03 Nov 2020 12:50
Operator : SY/MD
Sample : VV1104WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK312

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

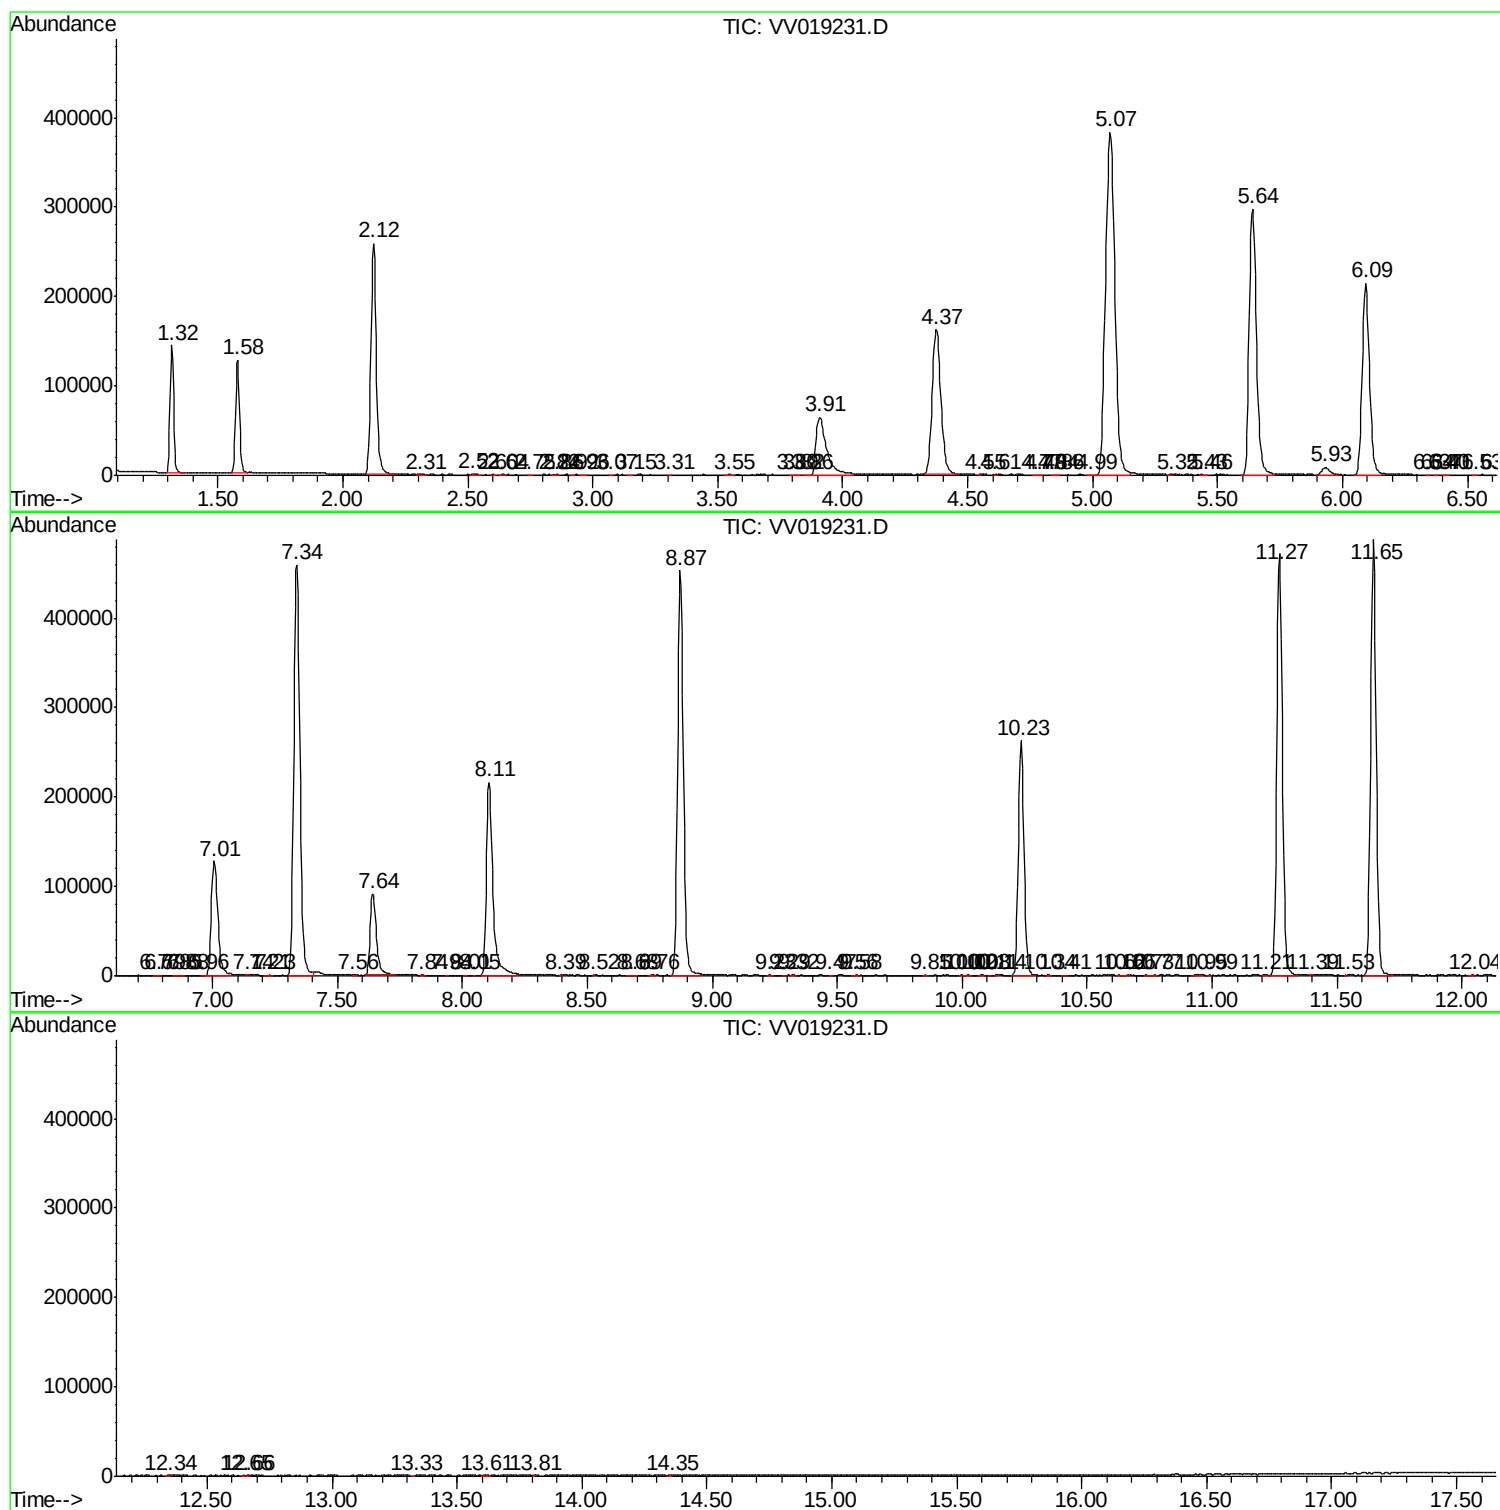

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110420\
Data File : VV019231.D
Acq On : 03 Nov 2020 12:50
Operator : SY/MD
Sample : VV1104WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK312

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110420\
Data File : VV019231.D
Acq On : 03 Nov 2020 12:50
Operator : SY/MD
Sample : VV1104WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK312

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
