


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV110420\
 Data File : VV019227.D
 Acq On : 03 Nov 2020 09:36
 Operator : SY/MD
 Sample : BFB99
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB303

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
 Title : VOC Analysis
 Last Update : Wed Nov 04 09:43:49 2020

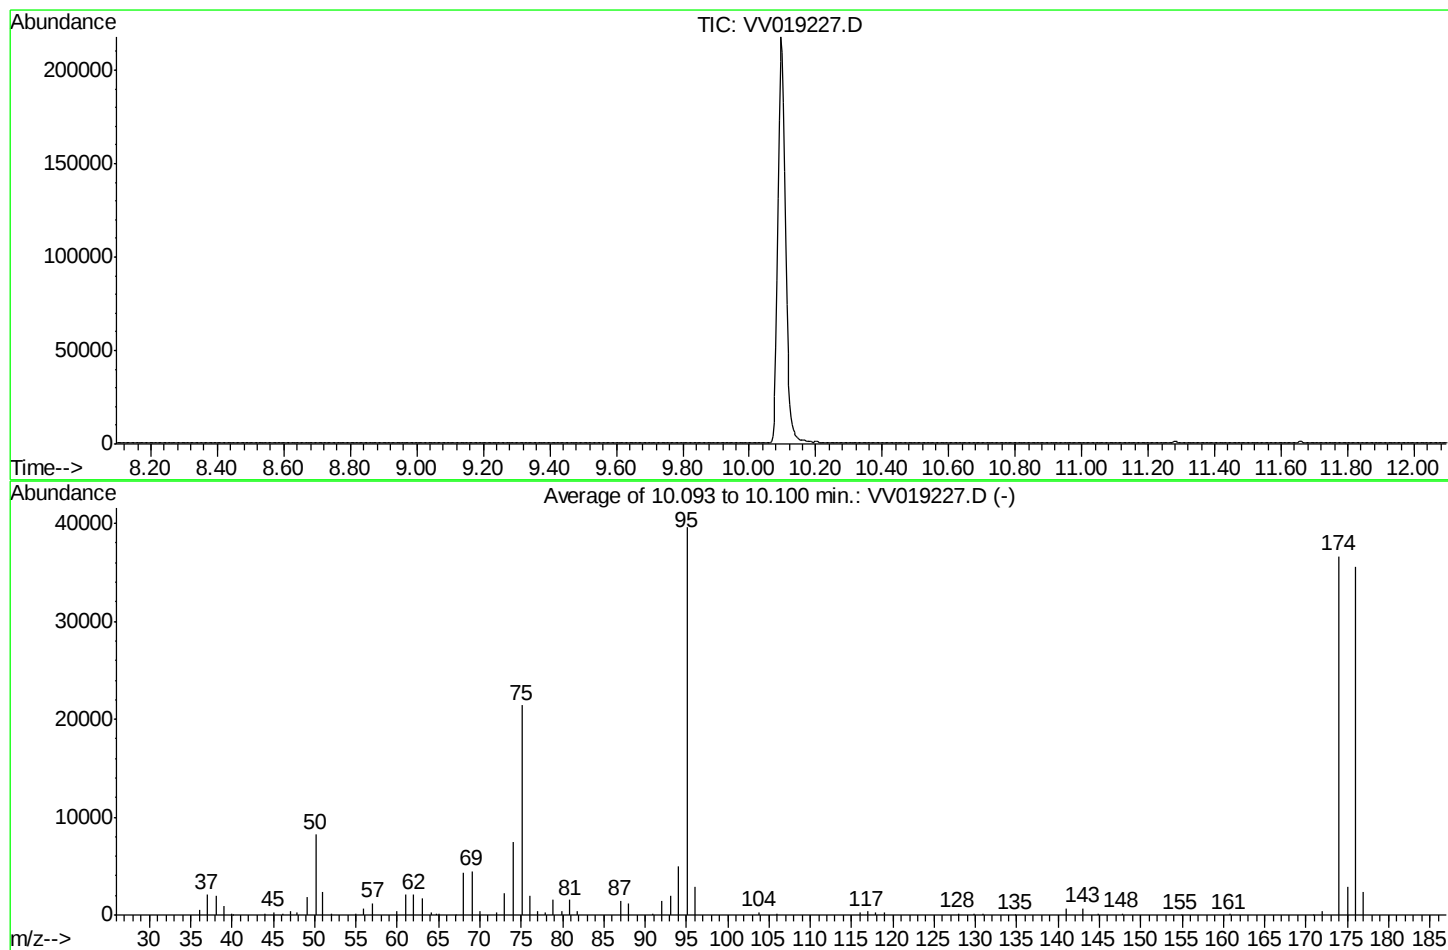

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	8207	PASS
75	95	30	80	54.0	21400	PASS
95	95	100	100	100.0	39610	PASS
96	95	5	9	7.2	2858	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.6	36682	PASS
175	174	5	9	7.9	2893	PASS
176	174	95	101	96.9	35541	PASS
177	176	5	9	6.8	2419	PASS

m/z	Abundance
36.00	486.0
37.00	2154.0
38.00	1952.0
39.00	905.0
39.90	118.0
44.00	742.0
45.00	309.0
46.10	107.0
47.00	399.0
47.90	337.0
49.00	1919.0
50.10	8456.0
51.00	2473.0
52.00	110.0
54.90	160.0
55.90	642.0
57.00	1255.0
60.00	448.0
61.00	2105.0
62.00	2140.0
63.10	1819.0
64.10	206.0
65.10	223.0
68.00	4419.0
69.00	4655.0
70.00	400.0
71.90	240.0
73.00	2274.0
74.10	7688.0
75.10	22144.0
76.00	2122.0
77.00	373.0
78.00	247.0
78.90	1623.0
79.90	411.0
80.90	1633.0
81.90	366.0
87.00	1540.0
88.00	1212.0
90.90	145.0
92.00	1451.0
93.10	1941.0
94.00	5146.0
95.10	40848.0
96.10	3005.0
103.80	275.0
106.00	192.0
116.00	240.0
116.90	347.0
117.90	218.0
118.90	319.0
127.90	166.0
129.80	124.0
130.90	105.0
140.90	629.0
143.00	749.0
144.80	162.0
147.70	143.0
160.80	108.0
170.90	111.0
172.00	370.0
174.00	37952.0
175.00	2970.0
176.00	36784.0
177.00	2513.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.00	435.0
37.00	2121.0
38.00	1965.0
39.00	819.0
39.90	122.0
44.00	672.0
45.00	345.0
46.10	113.0
47.00	431.0
47.90	341.0
49.00	1785.0
50.10	8272.0
51.00	2465.0
52.10	110.0
55.00	163.0
55.90	617.0
57.10	1188.0
60.00	407.0
61.00	2104.0
62.00	2071.0
63.10	1709.0
64.10	265.0
64.80	224.0
68.00	4212.0
69.00	4385.0
70.00	422.0
72.00	218.0
73.00	2182.0
74.00	7445.0
75.10	20864.0
76.00	1962.0
77.00	321.0
78.00	241.0
78.90	1584.0
79.90	424.0
80.90	1504.0
81.80	321.0
87.00	1469.0
88.10	1127.0
90.80	143.0
92.00	1347.0
93.10	1892.0
94.00	4869.0
95.10	38912.0
96.10	2826.0
103.80	278.0
106.00	194.0
116.00	226.0
117.00	352.0
117.80	203.0
118.90	292.0
127.90	150.0
129.80	120.0
130.90	108.0
134.80	110.0
141.00	554.0
143.00	725.0
144.80	155.0
147.70	108.0
160.80	105.0
172.10	354.0
174.00	35104.0
175.00	2801.0
176.00	33496.0
177.00	2248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.00	474.0
37.00	1978.0
38.10	1872.0
39.00	854.0
40.10	142.0
44.00	830.0
45.00	276.0
47.00	384.0
47.90	298.0
49.10	1802.0
50.10	7893.0
51.00	2272.0
52.00	113.0
54.90	170.0
55.90	639.0
57.00	1282.0
60.00	447.0
61.00	1978.0
62.00	2049.0
63.00	1725.0
64.00	151.0
65.10	237.0
67.00	116.0
68.00	4146.0
69.10	4401.0
70.10	314.0
71.90	232.0
73.00	2148.0
74.10	7315.0
75.00	21192.0
76.00	2009.0
76.90	357.0
77.90	210.0
78.90	1507.0
79.90	367.0
80.90	1562.0
81.90	384.0
87.00	1405.0
88.00	1244.0
91.00	162.0
92.00	1375.0
93.00	1885.0
94.00	4829.0
95.10	39072.0
96.10	2744.0
103.80	257.0
106.00	161.0
115.90	253.0
117.00	300.0
117.90	201.0
118.90	291.0
127.90	155.0
129.80	130.0
140.90	624.0
143.00	673.0
144.80	161.0
147.80	153.0
154.90	105.0
171.90	402.0
174.00	36992.0
175.00	2910.0
176.00	36344.0
177.00	2498.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
44.00	655.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303