
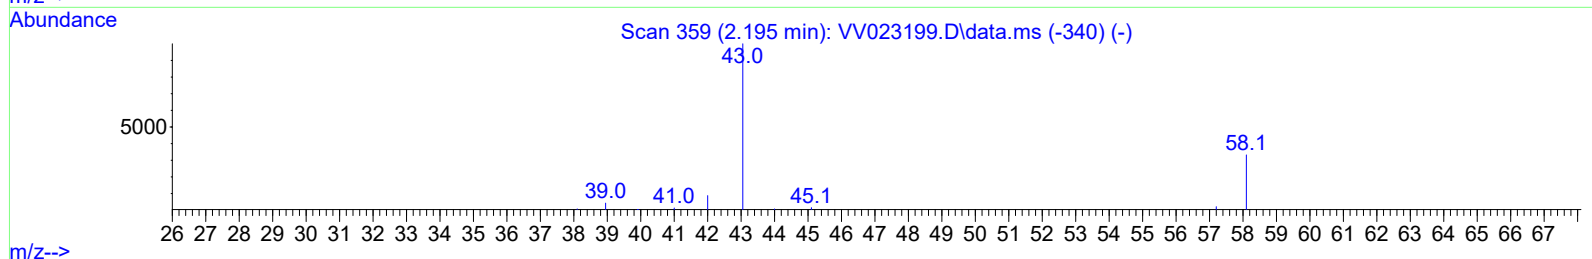
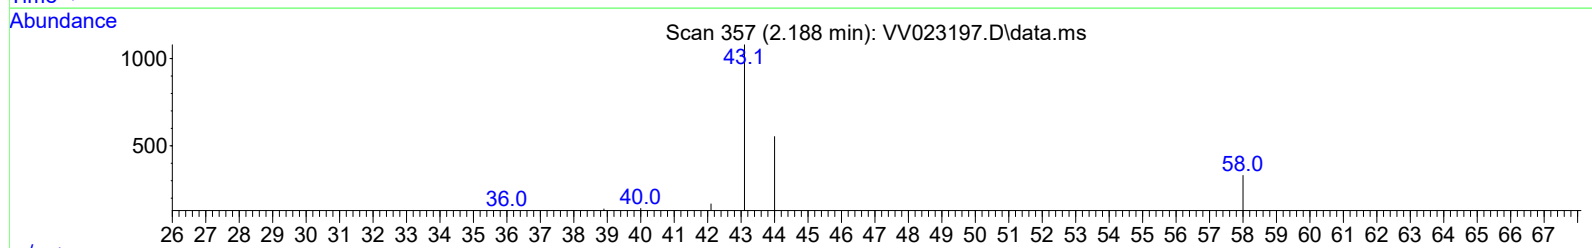


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023197.D
Acq On : 04 Nov 2021 12:24
Operator : SY/MD
Sample : VSTD0.547
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 12:49:02 2021
Response via : Initial Calibration

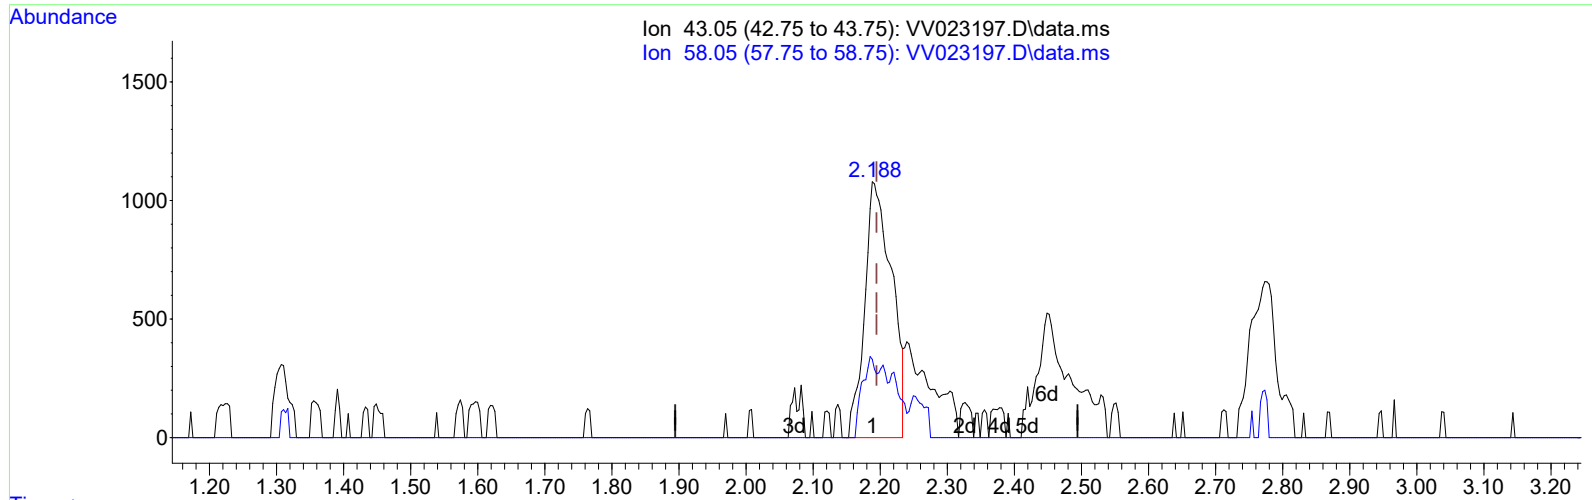

TIC: VV023197.D\data.ms

(13) Acetone (T)




2.188min (-0.006) 3.24 ug/L

response 3008

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	16.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023197.D
Acq On : 04 Nov 2021 12:24
Operator : SY/MD
Sample : VSTD0.547
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 12:49:02 2021
Response via : Initial Calibration

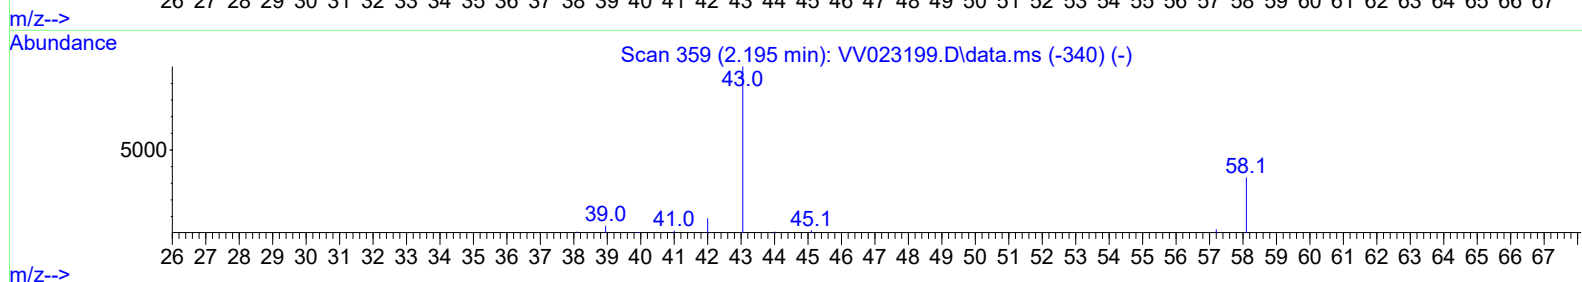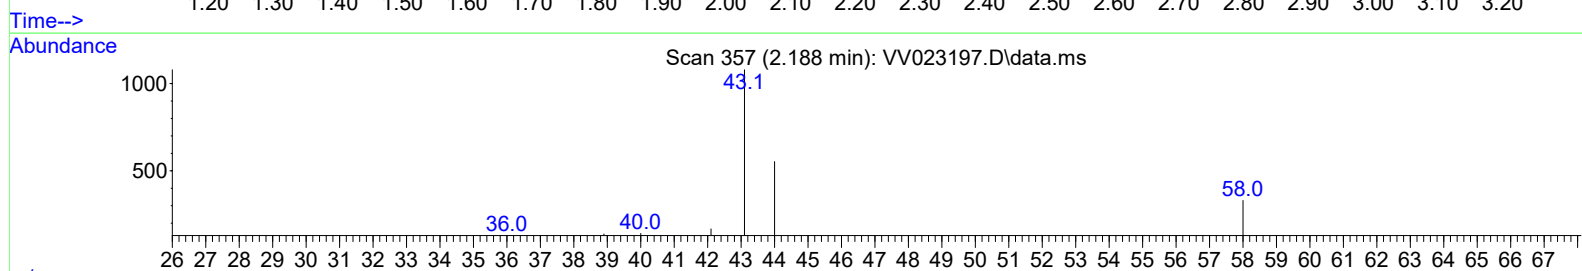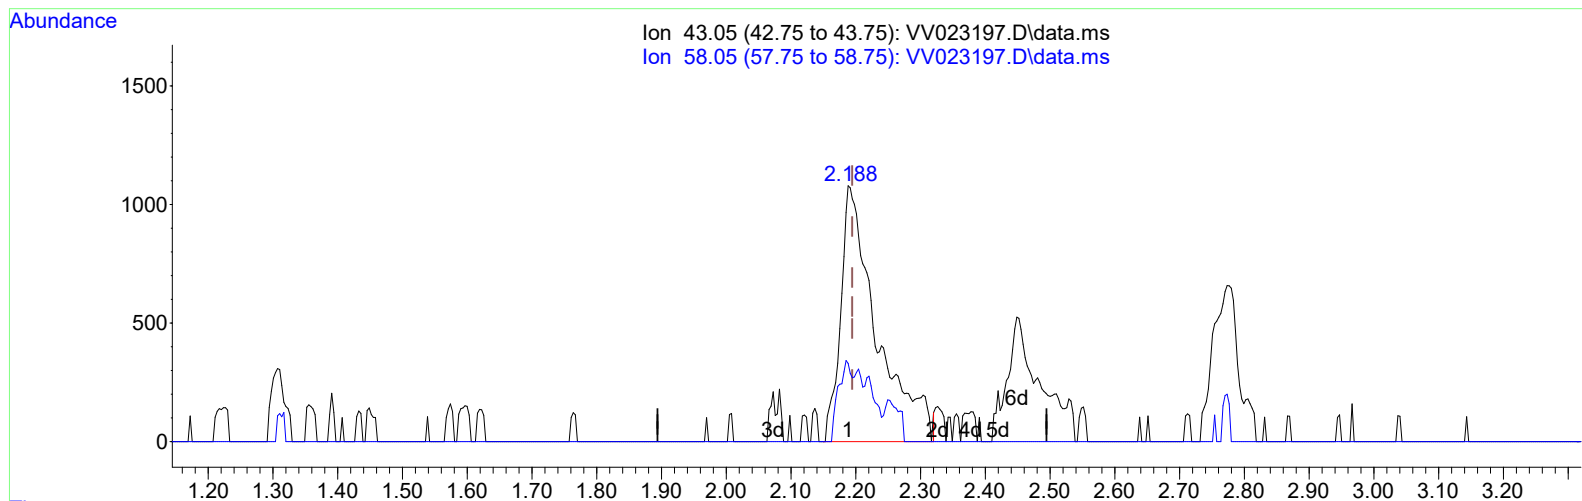

TIC: VV023197.D\data.ms

(13) Acetone (T)




2.188min (-0.006) 4.50 ug/L m

response 4186

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	11.63
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023197.D
Acq On : 04 Nov 2021 12:24
Operator : SY/MD
Sample : VSTD0.547
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 12:49:02 2021
Response via : Initial Calibration

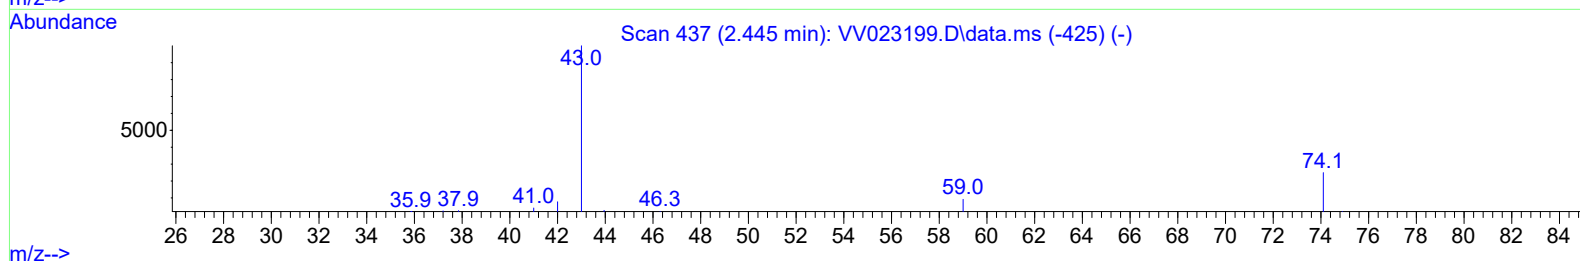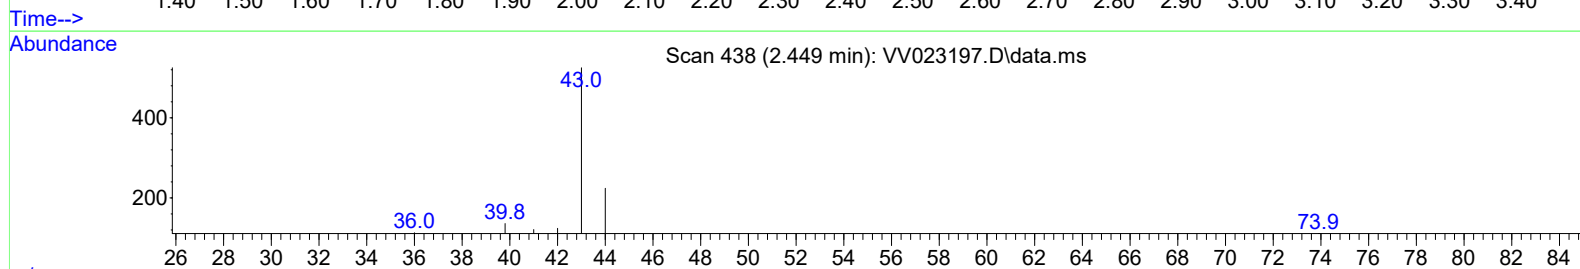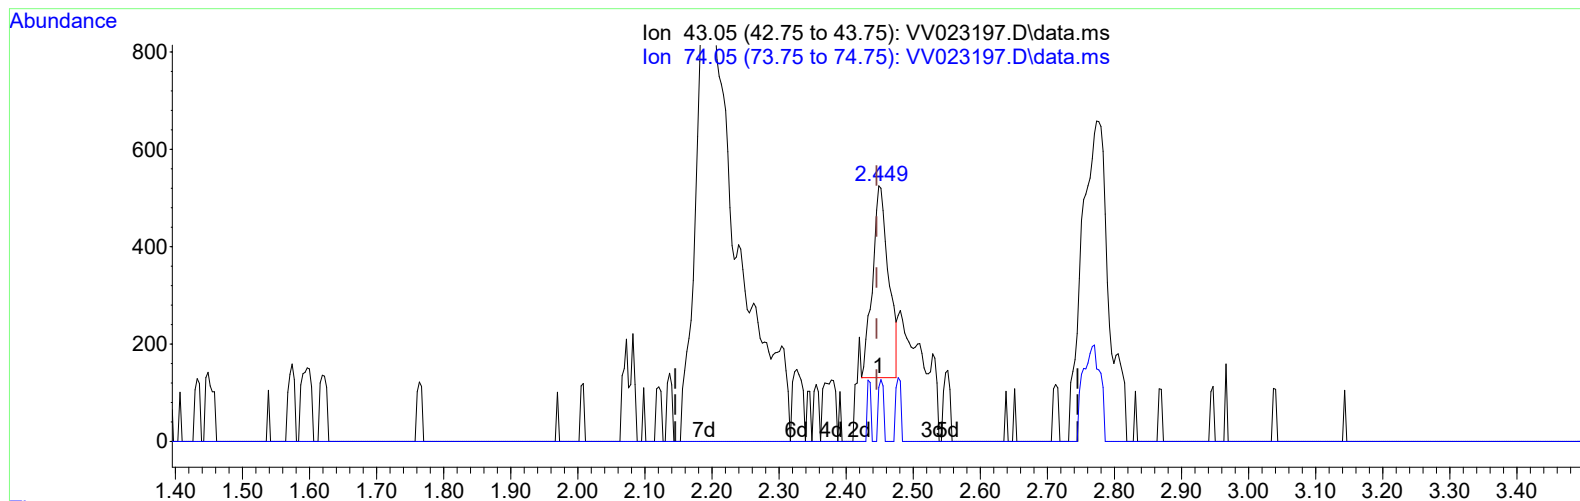

TIC: VV023197.D\data.ms

(15) Methyl Acetate (T)




2.449min (+ 0.003) 0.18 ug/L

response 654

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	27.70	10.40#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023197.D
Acq On : 04 Nov 2021 12:24
Operator : SY/MD
Sample : VSTD0.547
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 12:49:02 2021
Response via : Initial Calibration

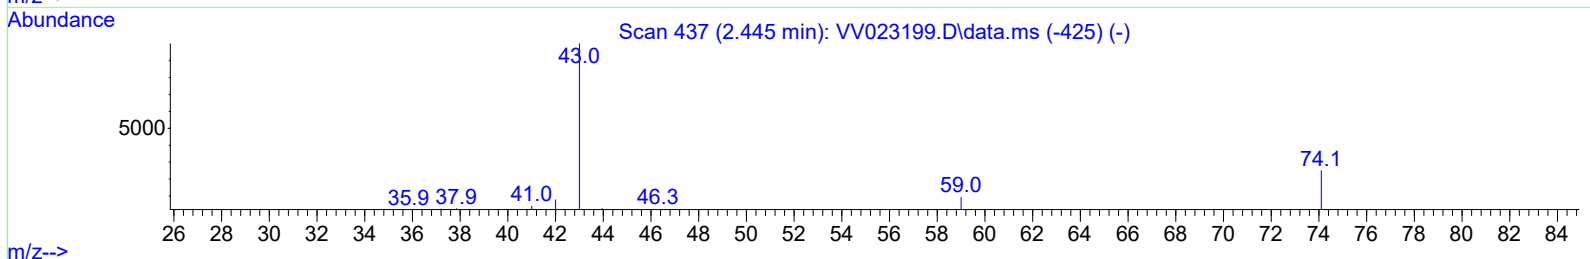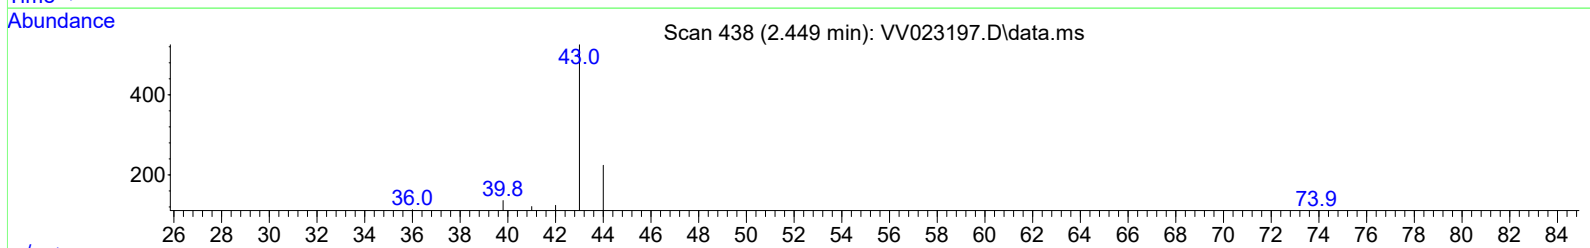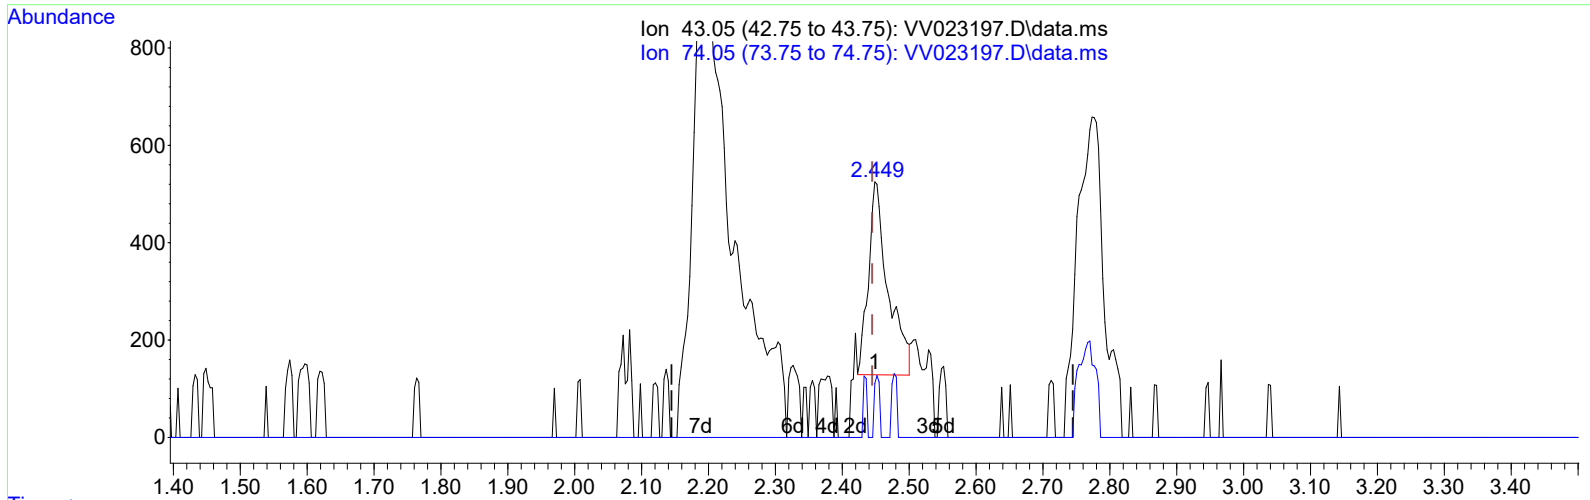

TIC: VV023197.D\data.ms

(15) Methyl Acetate (T)




2.449min (+ 0.003) 0.23 ug/L m

response 811

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	27.70	8.38#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023197.D
Acq On : 04 Nov 2021 12:24
Operator : SY/MD
Sample : VSTD0.547
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 12:49:02 2021
Response via : Initial Calibration

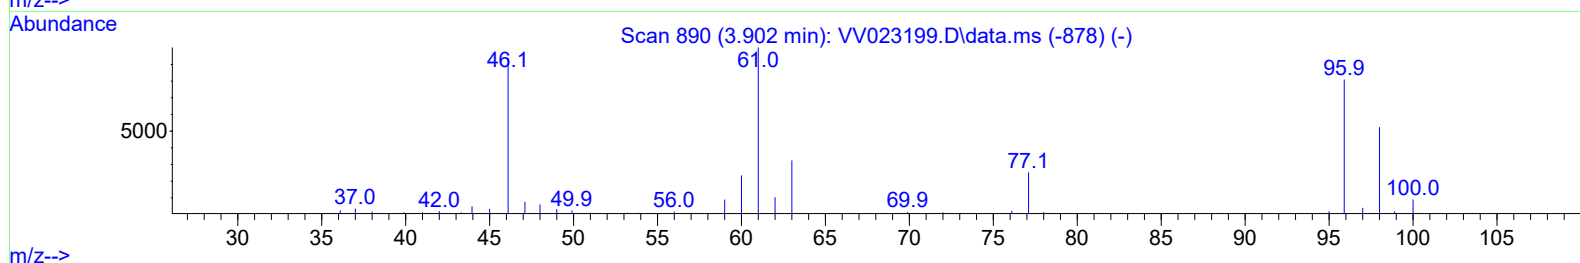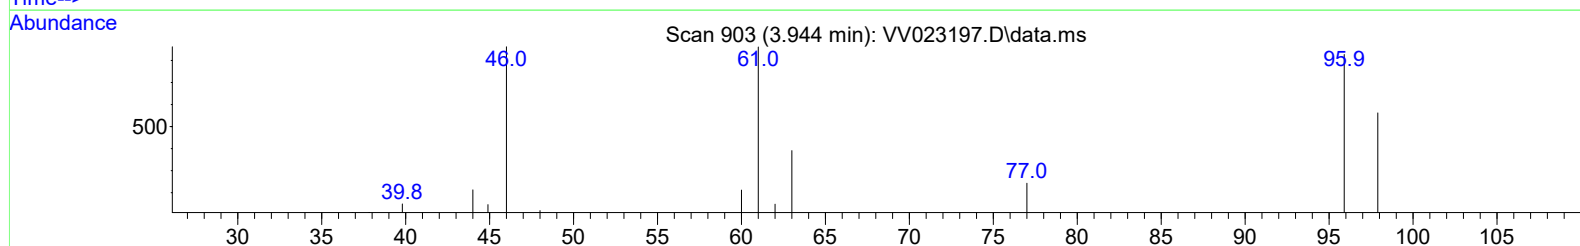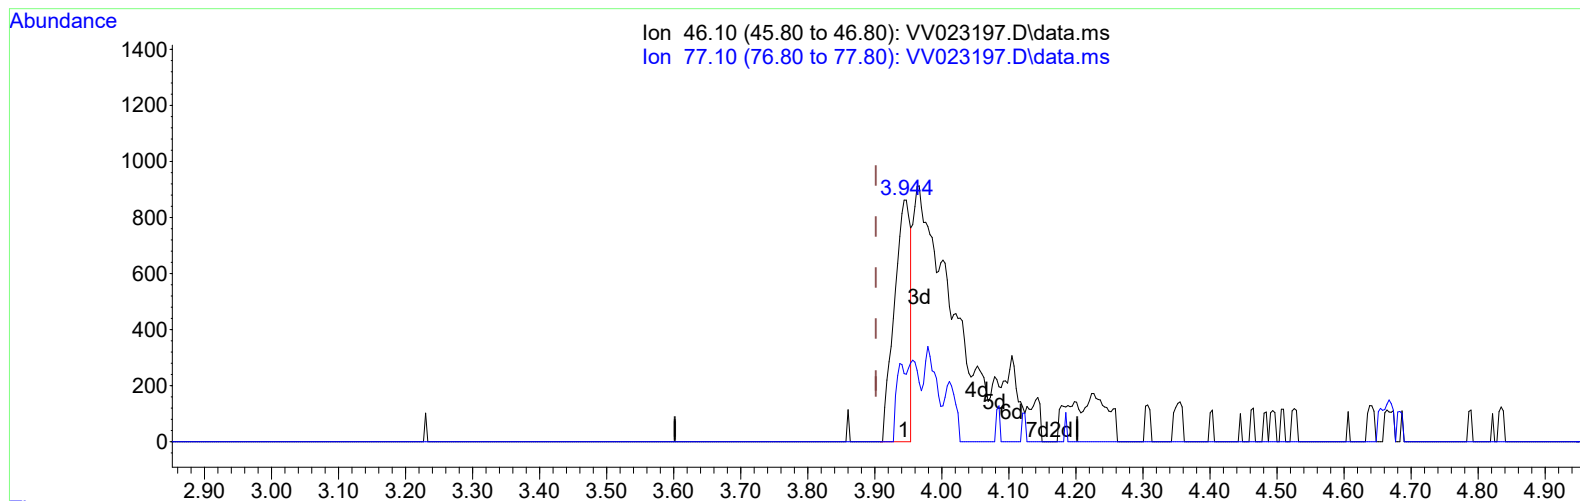

TIC: VV023197.D\data.ms

(20) 2-Butanone-d5 (S)




3.944min (+ 0.042) 0.76 ug/L

response 1433

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	19.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023197.D
Acq On : 04 Nov 2021 12:24
Operator : SY/MD
Sample : VSTD0.547
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 12:49:02 2021
Response via : Initial Calibration

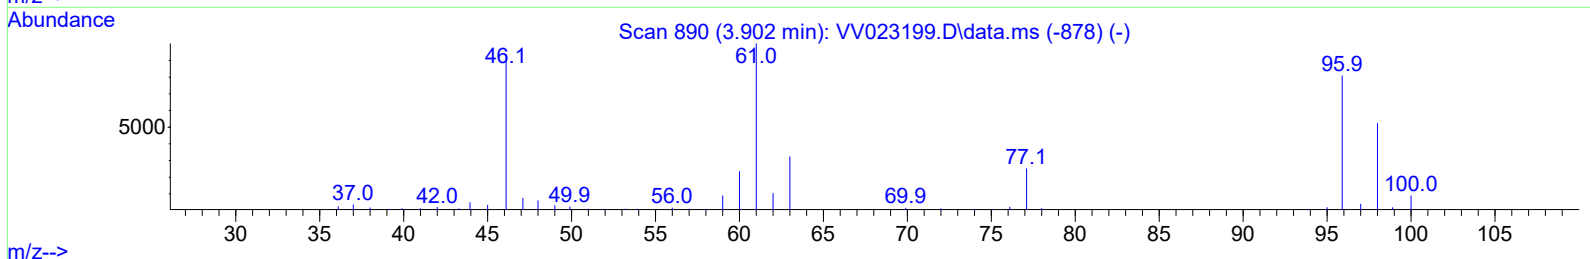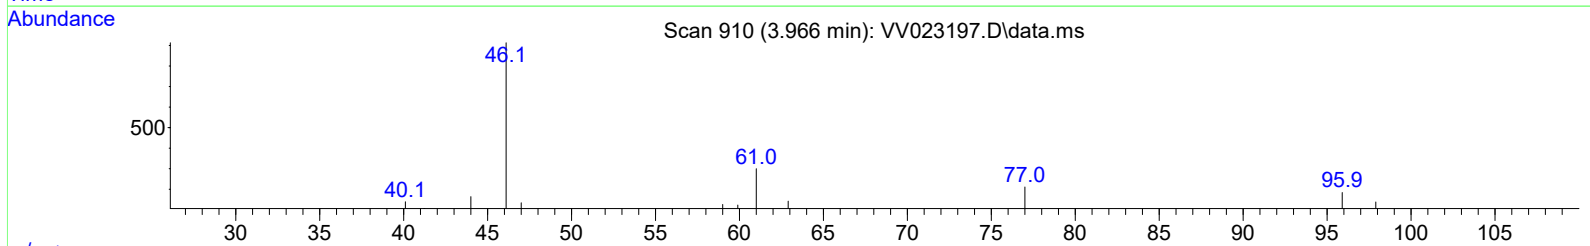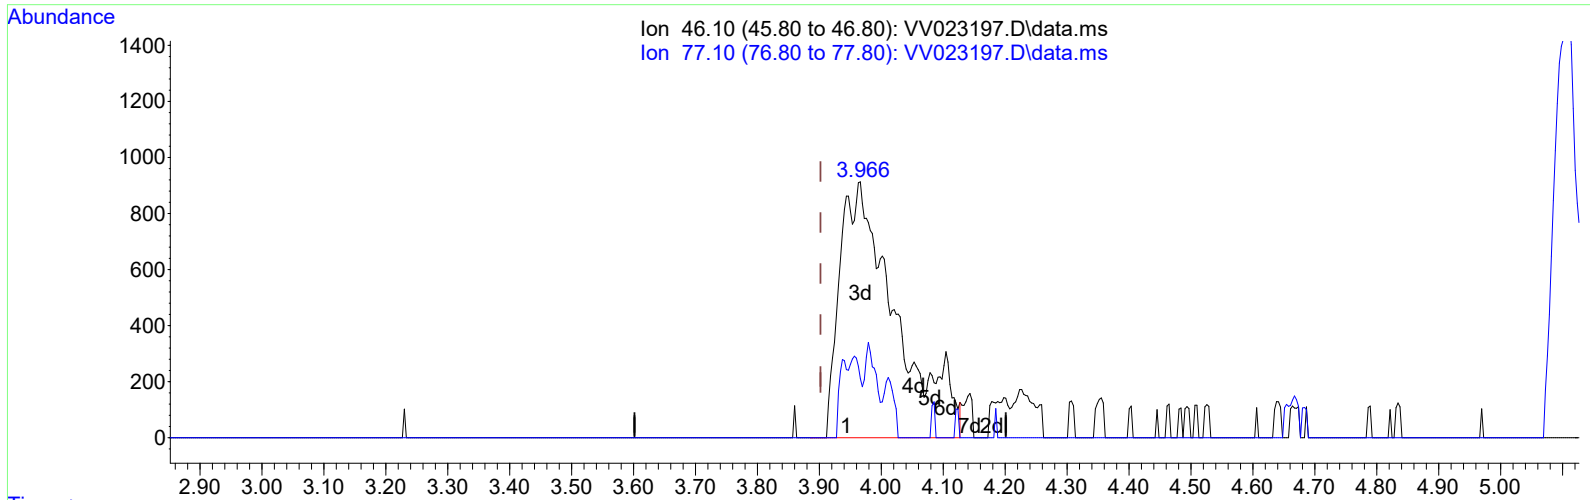

TIC: VV023197.D\data.ms

(20) 2-Butanone-d5 (S)




3.966min (+ 0.064) 3.00 ug/L m

response 5688

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	4.89#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023197.D
Acq On : 04 Nov 2021 12:24
Operator : SY/MD
Sample : VSTD0.547
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 12:49:02 2021
Response via : Initial Calibration

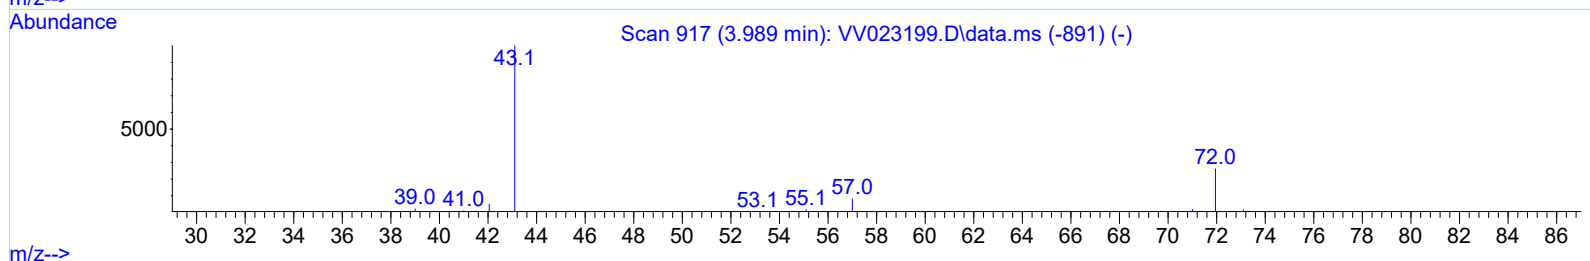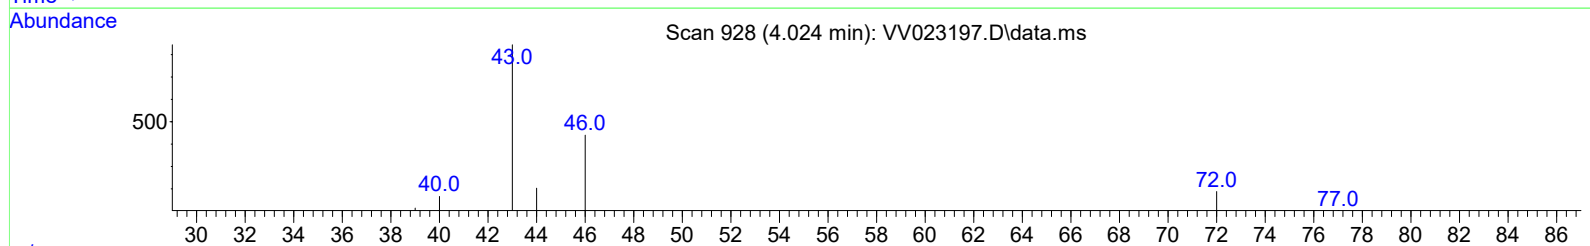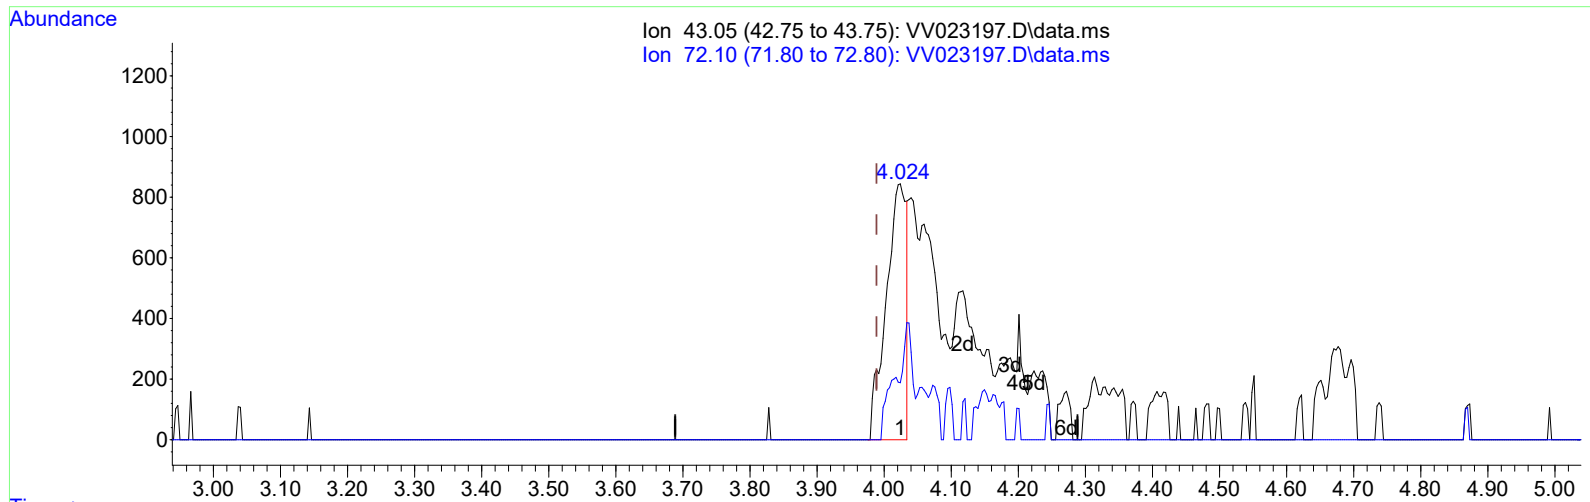

TIC: VV023197.D\data.ms

(21) 2-Butanone (T)




4.024min (+ 0.035) 0.97 ug/L

response 1760

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.90	16.99
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023197.D
Acq On : 04 Nov 2021 12:24
Operator : SY/MD
Sample : VSTD0.547
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 12:49:02 2021
Response via : Initial Calibration

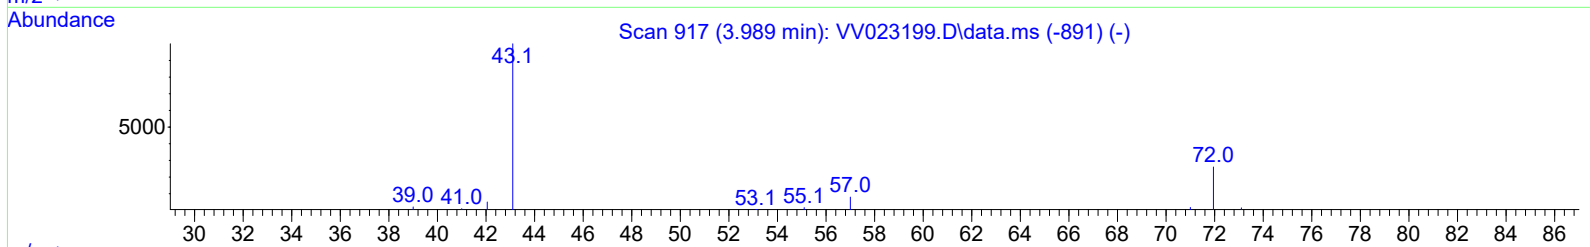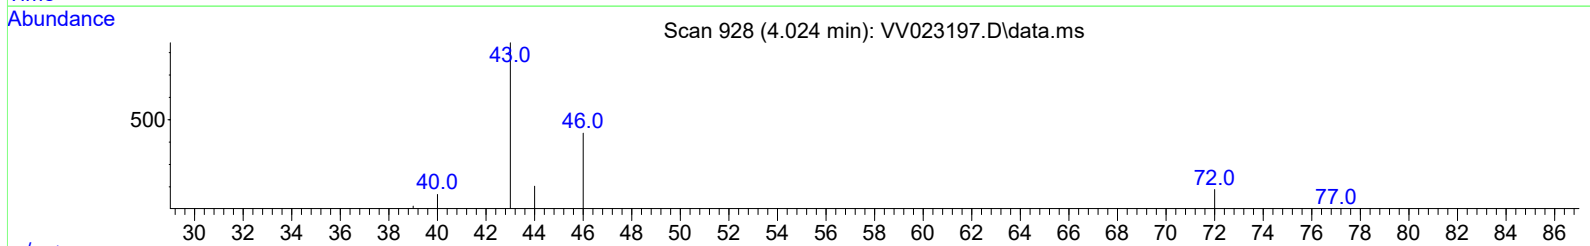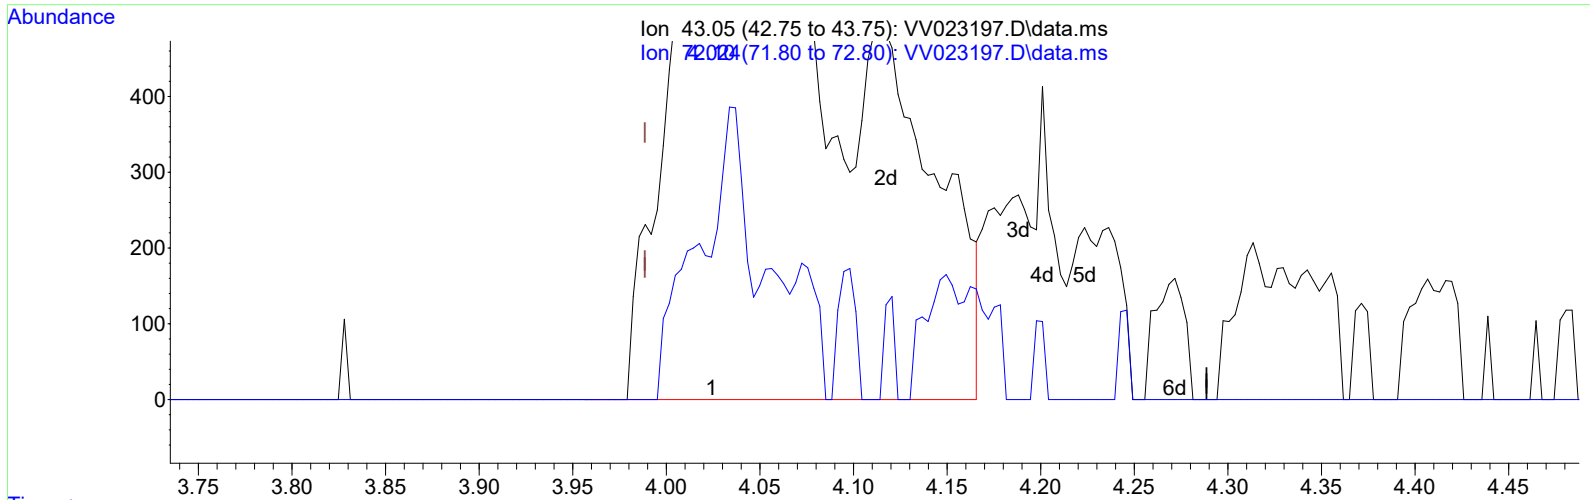

TIC: VV023197.D\data.ms

(21) 2-Butanone (T)

4.024min (+ 0.035) 2.96 ug/L m

response 5386

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.90	5.55#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023197.D
 Acq On : 04 Nov 2021 12:24
 Operator : SY/MD
 Sample : VSTD0.547
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 12:49:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	135179	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	131048	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66791	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	3814	0.32	ug/L	0.00
7) Chloroethane-d5	1.568	69	3269	0.45	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.108	63	7397	0.43	ug/L	0.00
20) 2-Butanone-d5	3.966	46	5688m	3.00	ug/L	0.06
24) Chloroform-d	4.359	84	8179	0.43	ug/L	0.00
26) 1,2-Dichloroethane-d4	5.047	65	3613	0.40	ug/L	0.00
32) Benzene-d6	5.056	84	14404	0.38	ug/L	0.00
36) 1,2-Dichloropropane-d6	6.075	67	4375	0.37	ug/L	0.00
41) Toluene-d8	7.320	98	12645	0.37	ug/L	0.00
43) trans-1,3-Dichloroprop...	7.635	79	1301	0.32	ug/L	0.00
46) 2-Hexanone-d5	8.104	63	4125	2.70	ug/L	0.01
56) 1,1,2,2-Tetrachloroeth...	10.220	84	3019	0.37	ug/L	0.00
66) 1,2-Dichlorobenzene-d4	11.625	152	5048	0.42	ug/L	0.00
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.130	85	6336	0.74	ug/L	93
3) Chloromethane	1.240	50	5605	0.60	ug/L	97
5) Vinyl chloride	1.310	62	5385	0.56	ug/L	100
6) Bromomethane	1.523	94	3494	0.72	ug/L	100
8) Chloroethane	1.584	64	3093	0.62	ug/L	93
9) Trichlorofluoromethane	1.754	101	8220	0.64	ug/L	97
10) 1,1,2-Trichloro-1,2,2-...	2.117	101	4172	0.57	ug/L	98
12) 1,1-Dichloroethene	2.121	96	3933	0.57	ug/L	86
13) Acetone	2.188	43	4186m	4.50	ug/L	
14) Carbon disulfide	2.294	76	14780	0.78	ug/L	99
16) Methylene chloride	2.506	84	8187	1.08	ug/L	94
17) Methyl tert-butyl Ether	2.767	73	7431	0.45	ug/L #	94
18) trans-1,2-Dichloroethene	2.760	96	4691	0.63	ug/L	92
19) 1,1-Dichloroethane	3.188	63	7817	0.58	ug/L	93
21) 2-Butanone	4.024	43	5386m	2.96	ug/L	
22) cis-1,2-Dichloroethene	3.915	96	4189	0.50	ug/L #	87
23) Bromochloromethane	4.246	128	1943	0.51	ug/L	69
25) Chloroform	4.375	83	8667	0.48	ug/L	86
27) 1,2-Dichloroethane	5.146	62	4239	0.45	ug/L	97
29) 1,1,1-Trichloroethane	4.606	97	7367	0.50	ug/L	97
30) Cyclohexane	4.674	56	5884	0.46	ug/L	98
31) Carbon tetrachloride	4.825	117	6527	0.51	ug/L	100
33) Benzene	5.104	78	15744	0.45	ug/L	100
34) Trichloroethene	5.921	95	4653	0.53	ug/L	95
35) Methylcyclohexane	6.127	83	6425	0.51	ug/L	99
37) 1,2-Dichloropropane	6.178	63	3846	0.43	ug/L #	85
38) Bromodichloromethane	6.516	83	5222	0.48	ug/L	94
39) cis-1,3-Dichloropropene	7.037	75	4995	0.45	ug/L	93
40) 4-Methyl-2-pentanone	7.233	43	14200	3.39	ug/L	98
42) Toluene	7.394	91	15440	0.43	ug/L	99
44) trans-1,3-Dichloropropene	7.657	75	3663	0.40	ug/L	94
45) 1,1,2-Trichloroethane	7.844	97	2792	0.45	ug/L	90

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023197.D
 Acq On : 04 Nov 2021 12:24
 Operator : SY/MD
 Sample : VSTD0.547
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 08 12:54:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 12:49:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

47) Tetrachloroethene	7.976	164	3727	0.50	ug/L	98
48) 2-Hexanone	8.149	43	7655	2.46	ug/L #	92
49) Dibromochloromethane	8.249	129	3233	0.44	ug/L	94
50) 1,2-Dibromoethane	8.362	107	2287	0.41	ug/L #	89
51) Chlorobenzene	8.886	112	11829	0.50	ug/L	95
52) Ethylbenzene	9.014	91	16351	0.46	ug/L	97
53) m,p-xylene	9.143	106	6560	0.46	ug/L	95
54) o-xylene	9.545	106	5676	0.42	ug/L	88
55) Styrene	9.567	104	9097	0.39	ug/L	97
57) 1,1,2,2-Tetrachloroethane	10.246	83	2710	0.39	ug/L #	89
59) Bromoform	9.734	173	1715	0.44	ug/L #	97
60) Isopropylbenzene	9.931	105	15391	0.46	ug/L	99
61) 1,2,3-Trichloropropane	10.275	75	1921	0.41	ug/L	94
62) 1,3,5-Trimethylbenzene	10.542	105	12418	0.46	ug/L	98
63) 1,2,4-Trimethylbenzene	10.918	105	11348	0.42	ug/L	98
64) 1,3-Dichlorobenzene	11.185	146	8506	0.48	ug/L	96
65) 1,4-Dichlorobenzene	11.275	146	9163	0.51	ug/L	95
67) 1,2-Dichlorobenzene	11.644	146	7488	0.45	ug/L	90
68) 1,2-Dibromo-3-chloropr...	12.432	75	401	0.43	ug/L #	79
69) 1,3,5-Trichlorobenzene	12.648	180	6734	0.50	ug/L	99
70) 1,2,4-trichlorobenzene	13.262	180	5508	0.54	ug/L	99
71) Naphthalene	13.506	128	7400	0.48	ug/L	98
72) 1,2,3-Trichlorobenzene	13.747	180	4566	0.49	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110421\  
Data File : VW023197.D  
Acq On    : 04 Nov 2021 12:24  
Operator  : SY/MD  
Sample    : VSTD0.547  
Misc      : 25.0mL/MSVOA_V/WATER  
ALS Vial  : 3 Sample Multiplier: 1
```

Quant Time: Nov 08 12:54:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 12:49:02 2021
Response via : Initial Calibration

