

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110421\  
 Data File : VV023204.D  
 Acq On : 04 Nov 2021 15:59  
 Operator : SY/MD  
 Sample : M4464-16  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 GB7L4

Manual Integrations  
 APPROVED

Reviewed By : John Carlone 11/11/2021  
 Supervised By : Mahesh Dadoda 11/11/2021

Quant Time: Nov 09 01:08:43 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Mon Nov 08 13:19:52 2021  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 5.619  | 114   | 166749   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 8.854  | 117   | 164958   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152   | 79114    | 5.000    | ug/L   | 0.00     |
|                               |        |       |          |          |        |          |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.304  | 65    | 40958    | 3.921    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 78.400%  |
| 7) Chloroethane-d5            | 1.568  | 69    | 34071    | 4.002    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 80.000%  |
| 11) 1,1-Dichloroethene-d2     | 2.108  | 63    | 59081    | 3.021    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 60.400%  |
| 20) 2-Butanone-d5             | 3.905  | 46    | 70588    | 39.222   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 78.440%  |
| 24) Chloroform-d              | 4.352  | 84    | 86351    | 3.879    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 77.600%  |
| 26) 1,2-Dichloroethane-d4     | 5.037  | 65    | 40836    | 4.079    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 81.600%  |
| 32) Benzene-d6                | 5.053  | 84    | 173420   | 4.097    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 82.000%  |
| 36) 1,2-Dichloropropane-d6    | 6.072  | 67    | 51042    | 4.097    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 82.000%  |
| 41) Toluene-d8                | 7.317  | 98    | 149872   | 3.779    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 75.600%  |
| 43) trans-1,3-Dichloroprop... | 7.625  | 79    | 19040    | 4.030    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 80.600%  |
| 46) 2-Hexanone-d5             | 8.091  | 63    | 64502    | 37.108   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 74.220%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84    | 32117    | 3.584    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 71.600%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.625 | 152   | 58557    | 4.445    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 89.000%  |
|                               |        |       |          |          |        |          |
| Target Compounds              |        |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.188  | 43    | 4600m    | 4.183    | ug/L   |          |
| -----                         |        |       |          |          |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110421\  
Data File : VV023204.D  
Acq On : 04 Nov 2021 15:59  
Operator : SY/MD  
Sample : M4464-16  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 11 Sample Multiplier: 1


Instrument :  
MSVOA\_V  
ClientSampleId :  
GB7L4

Quant Time: Nov 09 01:08:43 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Mon Nov 08 13:19:52 2021  
Response via : Initial Calibration

Manual Integrations  
APPROVED


Reviewed By :John Carlone 11/11/2021  
Supervised By :Mahesh Dadoda 11/11/2021

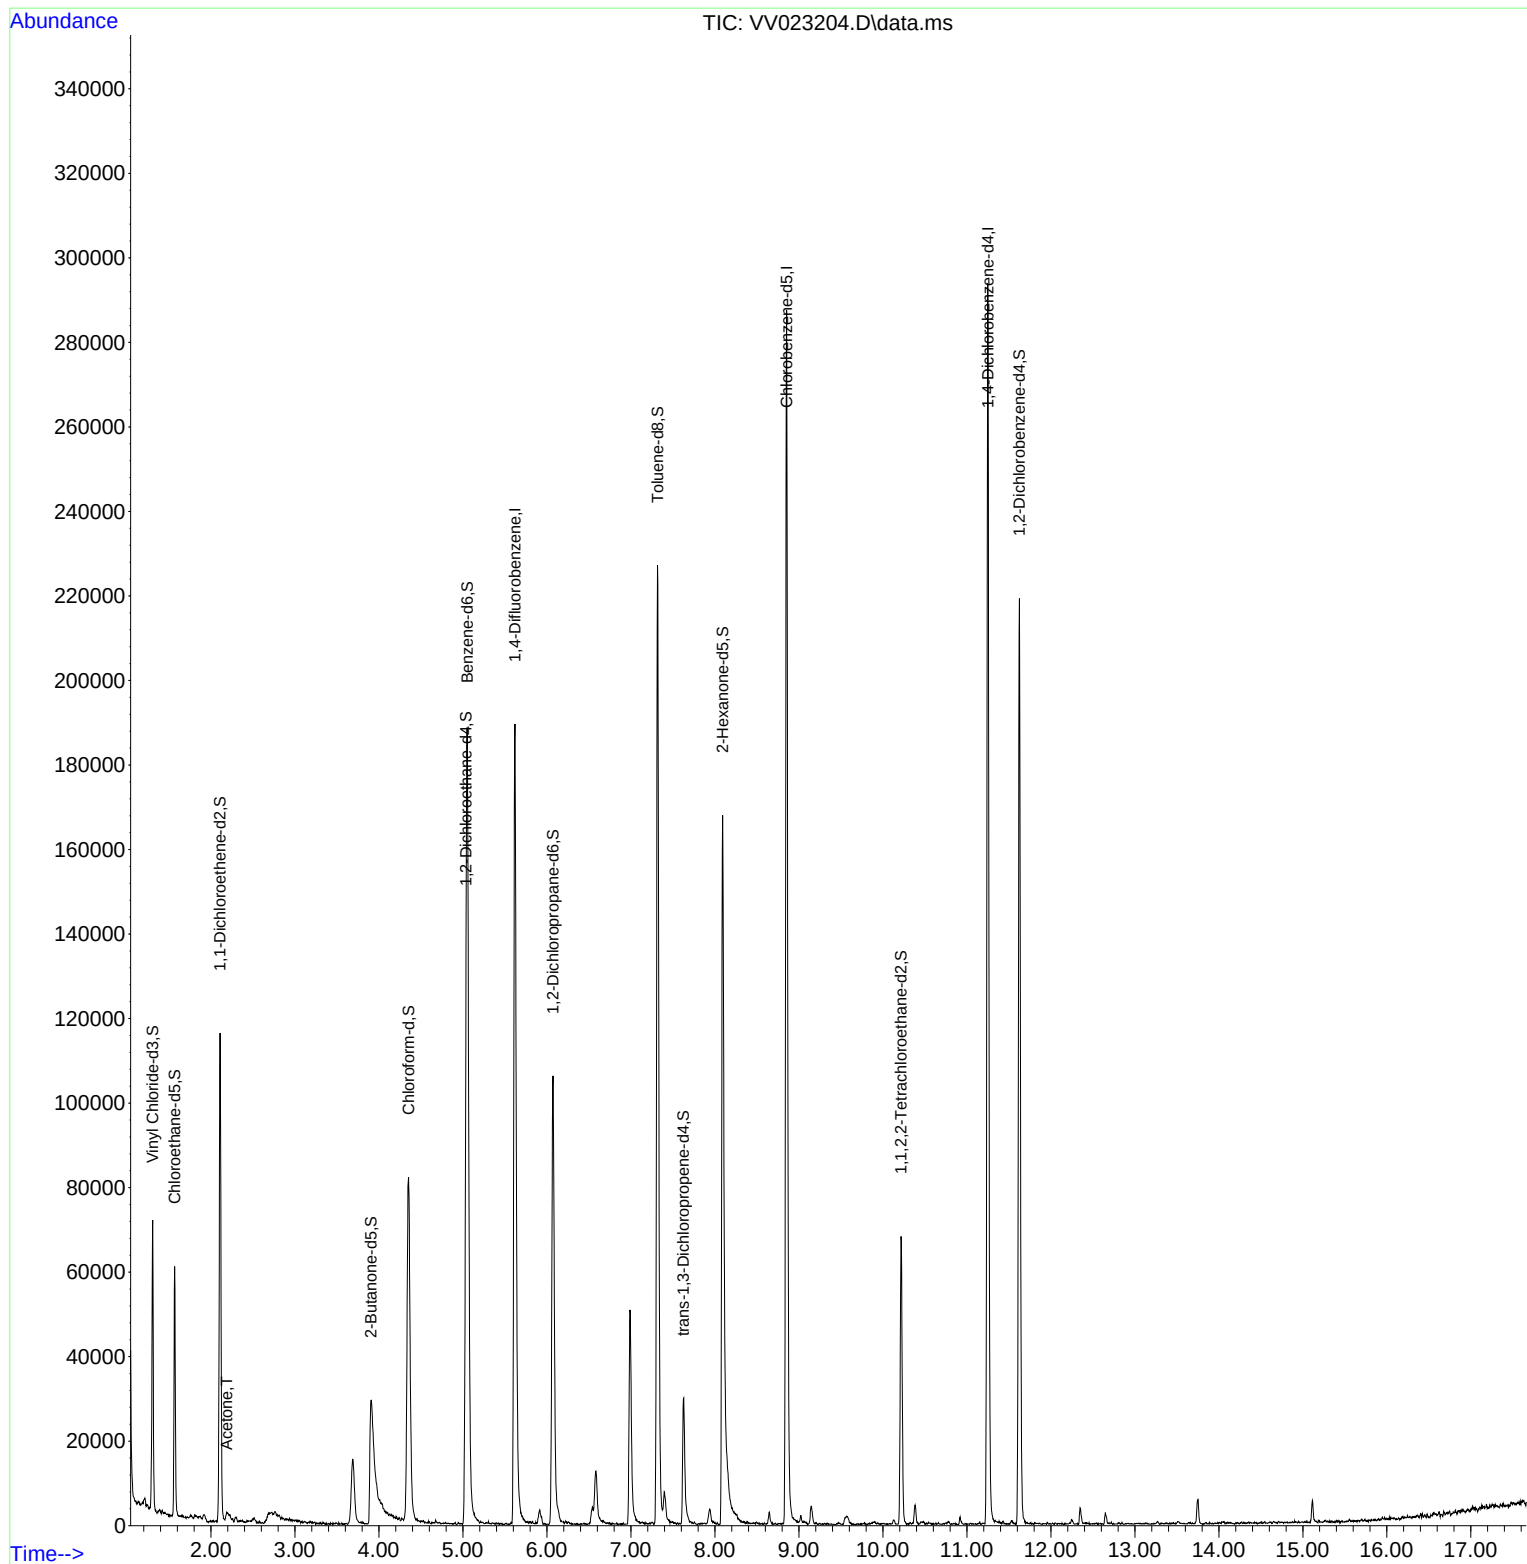

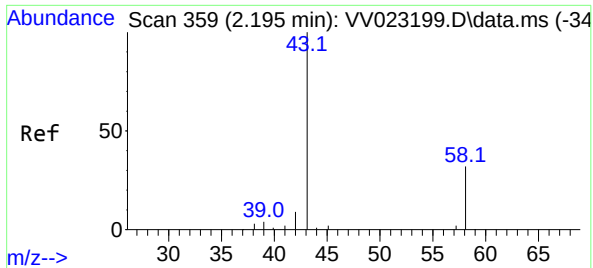

#13  
Acetone  
Concen: 4.183 ug/L m  
RT: 2.188 min Scan# 31  
Delta R.T. -0.006 min  
Lab File: VV023204.D  
Acq: 04 Nov 2021 15:59

Instrument :  
MSVOA\_V  
ClientSampleId :  
GB7L4

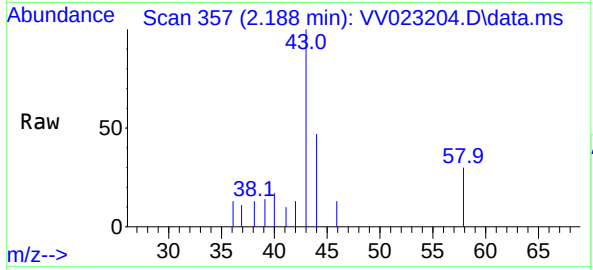

Tgt Ion: 43 Resp: 4600  
Ion Ratio Lower Upper  
43 100  
58 8.3 0.0 55.4

Manual Integrations  
APPROVED

Reviewed By :John Carlone 11/11/2021  
Supervised By :Mahesh Dadoda 11/11/2021

