

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110421\
 Data File : VW023206.D
 Acq On : 04 Nov 2021 16:46
 Operator : SY/MD
 Sample : M4445-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG382

Quant Time: Nov 09 01:13:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 13:19:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	138697	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	136287	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63698	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	43505	5.007	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.200%
7) Chloroethane-d5	1.568	69	35736	5.046	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.000%
11) 1,1-Dichloroethene-d2	2.111	63	59960	3.686	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.800%
20) 2-Butanone-d5	3.889	46	90008	60.128	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.260%
24) Chloroform-d	4.352	84	89820	4.851	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.000%
26) 1,2-Dichloroethane-d4	5.037	65	42581	5.114	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.200%
32) Benzene-d6	5.053	84	176875	5.058	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.200%
36) 1,2-Dichloropropane-d6	6.072	67	52953	5.144	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.800%
41) Toluene-d8	7.317	98	153177	4.674	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.400%
43) trans-1,3-Dichloroprop...	7.625	79	18495	4.738	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.800%
46) 2-Hexanone-d5	8.088	63	70459	49.063	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.120%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34779	4.698	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	59202	5.582	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.600%
Target Compounds					Qvalue	
13) Acetone	2.182	43	3937	4.304	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023206.D
Acq On : 04 Nov 2021 16:46
Operator : SY/MD
Sample : M4445-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG382


Quant Time: Nov 09 01:13:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 13:19:52 2021
Response via : Initial Calibration

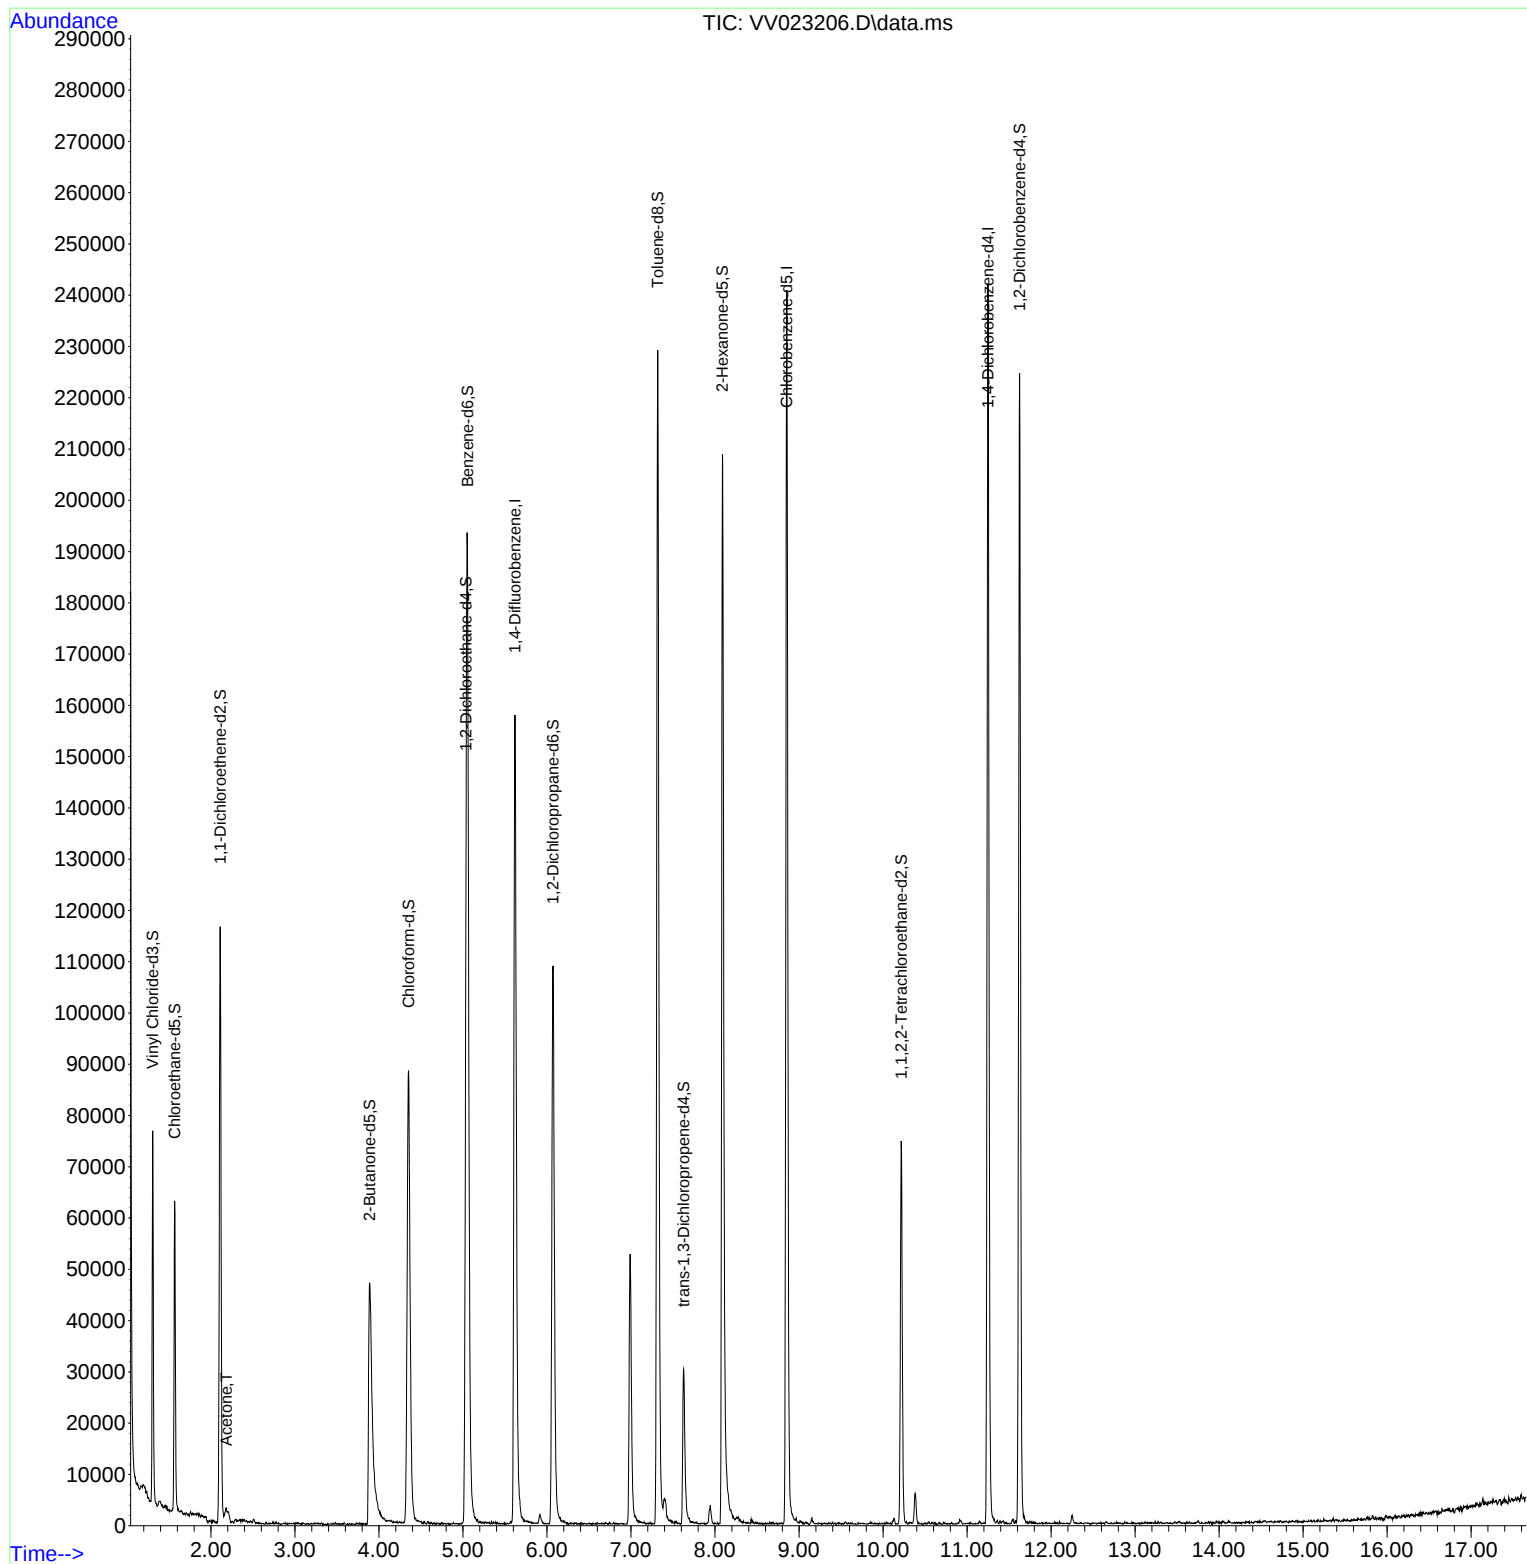

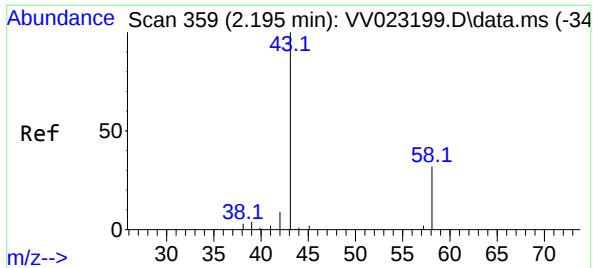

#13
 Acetone
 Concen: 4.304 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.013 min
 Lab File: VV023206.D
 Acq: 04 Nov 2021 16:46

Instrument :
 MSVOA_V
 ClientSampleId :
 BG382

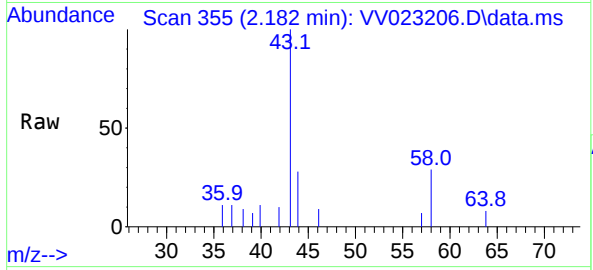

Tgt Ion: 43 Resp: 3937

Ion	Ratio	Lower	Upper
43	100		
58	30.2	0.0	55.4

