

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023207.D
 Acq On : 04 Nov 2021 17:09
 Operator : SY/MD
 Sample : M4445-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG383

Quant Time: Nov 09 01:15:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 13:19:52 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	133968	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	135477	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63080	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42760	5.095	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 101.800%		
7) Chloroethane-d5	1.568	69	35912	5.250	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 105.000%		
11) 1,1-Dichloroethene-d2	2.111	63	59370	3.779	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 75.600%		
20) 2-Butanone-d5	3.889	46	87295	60.375	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	= 120.740%		
24) Chloroform-d	4.352	84	87932	4.916	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 98.400%		
26) 1,2-Dichloroethane-d4	5.034	65	42124	5.237	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 104.800%		
32) Benzene-d6	5.053	84	171798	4.942	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 98.800%		
36) 1,2-Dichloropropane-d6	6.069	67	51270	5.010	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 100.200%		
41) Toluene-d8	7.317	98	147604	4.531	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 90.600%		
43) trans-1,3-Dichloroprop...	7.625	79	18524	4.774	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 95.400%		
46) 2-Hexanone-d5	8.088	63	68236	47.799	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 95.600%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34050	4.627	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 92.600%		
66) 1,2-Dichlorobenzene-d4	11.625	152	57987	5.521	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 110.400%		
Target Compounds						
13) Acetone	2.175	43	3328	3.767	ug/L	Qvalue 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023207.D
Acq On : 04 Nov 2021 17:09
Operator : SY/MD
Sample : M4445-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG383

Quant Time: Nov 09 01:15:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 13:19:52 2021
Response via : Initial Calibration

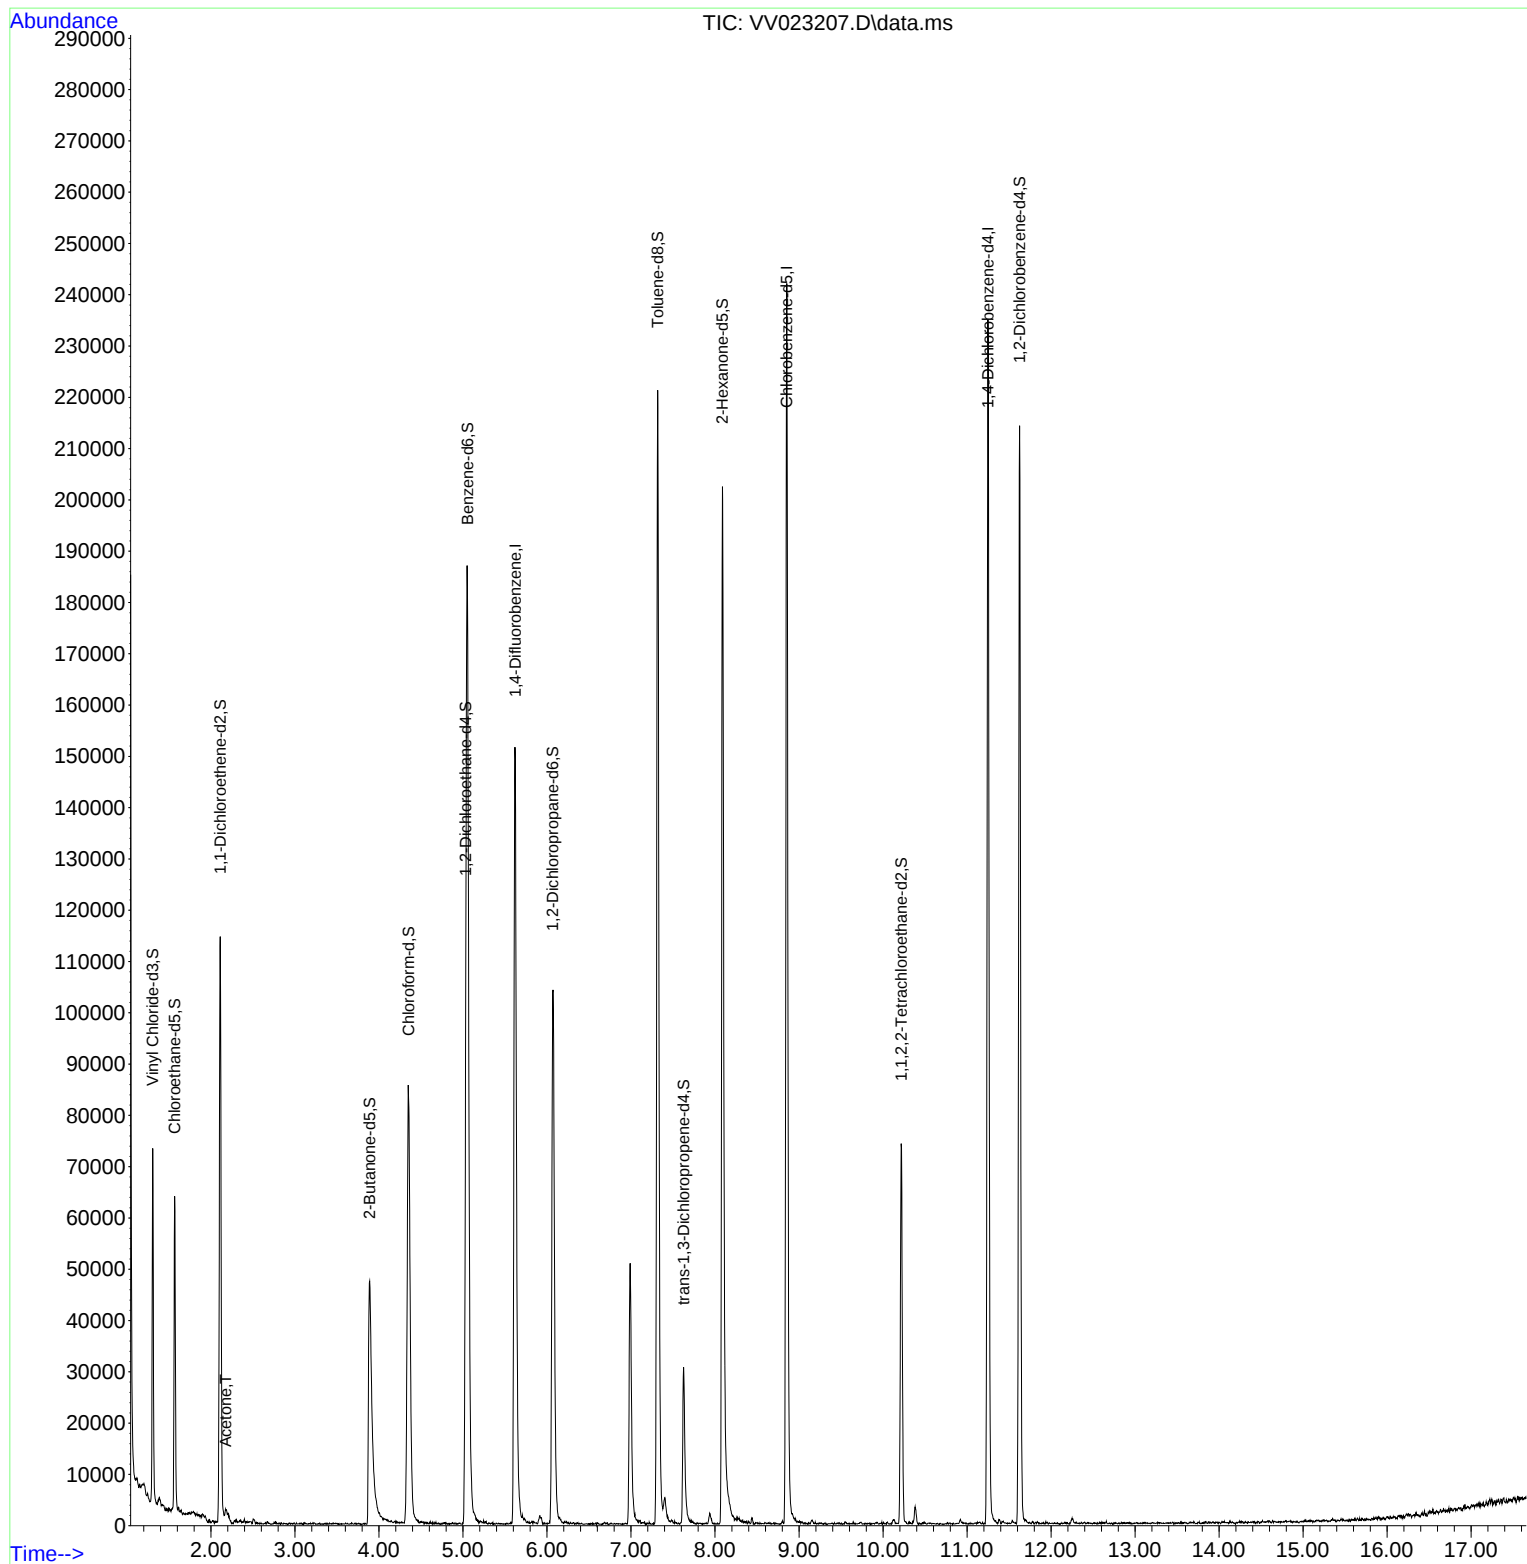

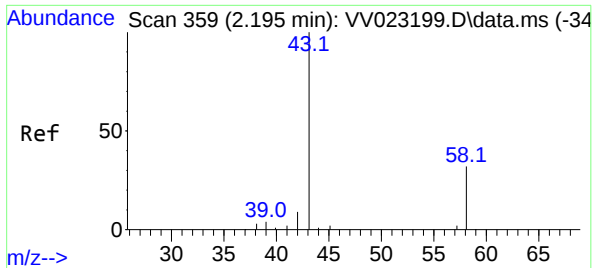

#13
 Acetone
 Concen: 3.767 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.019 min
 Lab File: VV023207.D
 Acq: 04 Nov 2021 17:09

Instrument :
 MSVOA_V
 ClientSampleId :
 BG383

Tgt Ion: 43 Resp: 3328
 Ion Ratio Lower Upper
 43 100
 58 37.0 0.0 55.4

