

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023208.D
 Acq On : 04 Nov 2021 17:33
 Operator : SY/MD
 Sample : M4445-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG384

Quant Time: Nov 09 01:17:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 13:19:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	134625	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	133582	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63305	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	44613	5.290	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	105.800%	
7) Chloroethane-d5	1.568	69	37366	5.436	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	108.800%	
11) 1,1-Dichloroethene-d2	2.111	63	61783	3.913	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.200%	
20) 2-Butanone-d5	3.889	46	89333	61.482	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	122.960%	
24) Chloroform-d	4.352	84	91390	5.085	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.600%	
26) 1,2-Dichloroethane-d4	5.034	65	43322	5.360	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.200%	
32) Benzene-d6	5.053	84	179407	5.234	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.600%	
36) 1,2-Dichloropropane-d6	6.072	67	52906	5.244	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.800%	
41) Toluene-d8	7.317	98	153908	4.792	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.800%	
43) trans-1,3-Dichloroprop...	7.625	79	18444	4.821	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.400%	
46) 2-Hexanone-d5	8.088	63	72236	51.319	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	102.640%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35398	4.879	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	59832	5.676	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	113.600%	
Target Compounds					Qvalue	
13) Acetone	2.182	43	2967	3.342	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023208.D
Acq On : 04 Nov 2021 17:33
Operator : SY/MD
Sample : M4445-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG384


Quant Time: Nov 09 01:17:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 13:19:52 2021
Response via : Initial Calibration

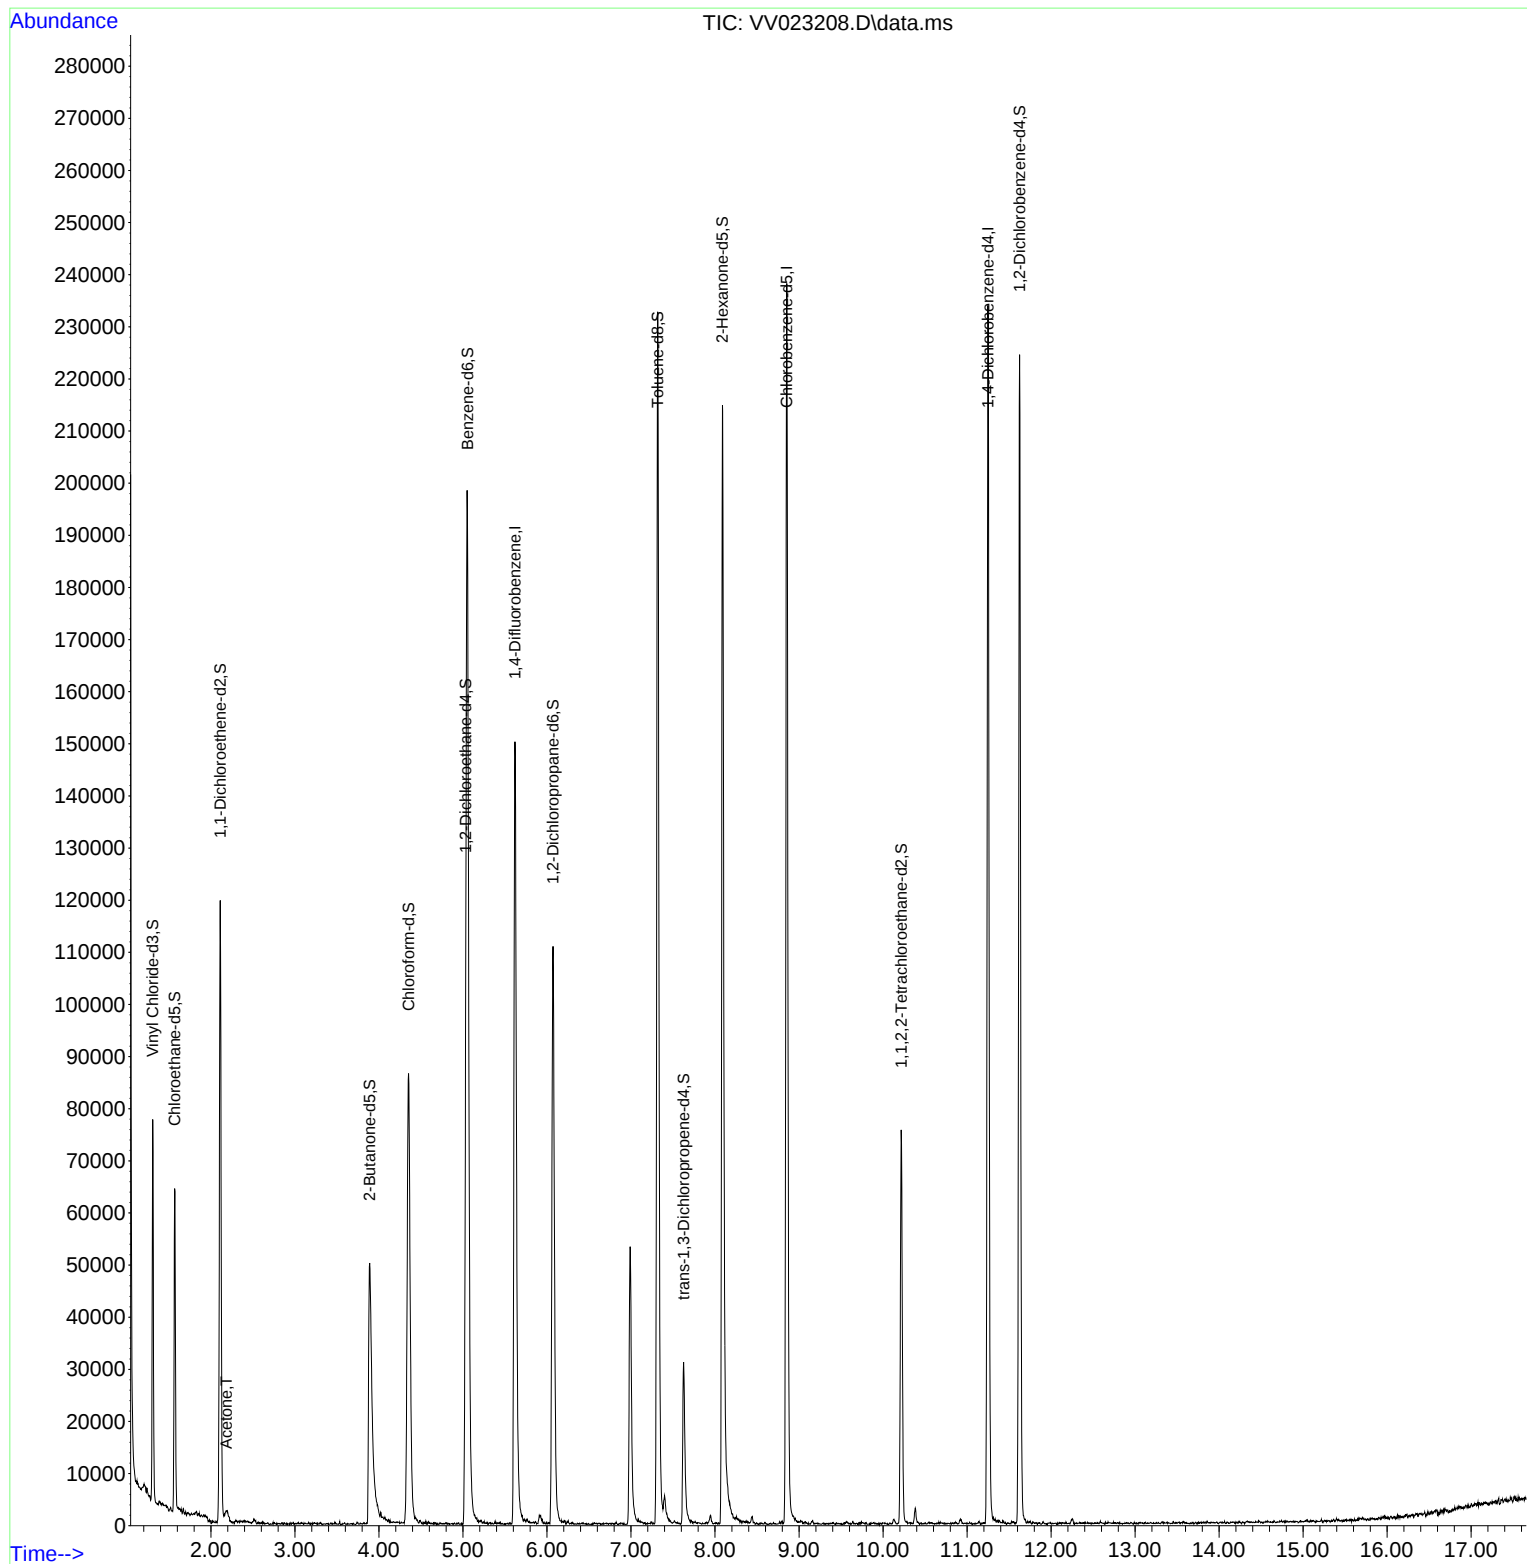


Abundance Scan 359 (2.195 min): VV023199.D\data.ms (-34

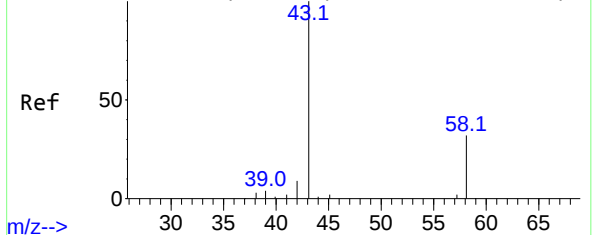

Abundance Scan 355 (2.182 min): VV023208.D\data.ms

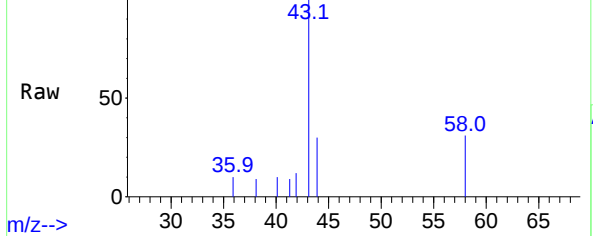

Abundance Scan 355 (2.182 min): VV023208.D\data.ms (-26

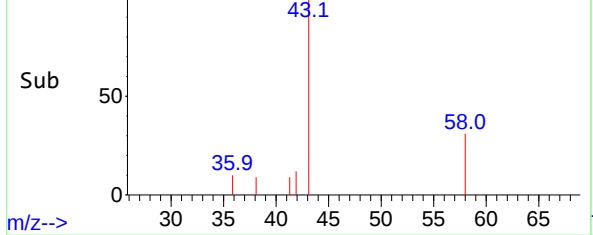

#13

Acetone

Concen: 3.342 ug/L

RT: 2.182 min Scan# 31

Delta R.T. -0.013 min

Lab File: VV023208.D

Acq: 04 Nov 2021 17:33

Instrument :

MSVOA_V

ClientSampleId :

BG384

Tgt Ion: 43 Resp: 2967

Ion Ratio Lower Upper

43 100

58 30.5 0.0 55.4

Abundance

