

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110421\  
 Data File : VV023209.D  
 Acq On : 04 Nov 2021 17:56  
 Operator : SY/MD  
 Sample : M4445-11  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BG385

Quant Time: Nov 09 01:21:35 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Mon Nov 08 13:19:52 2021  
 Response via : Initial Calibration


| Compound                      | R.T. QIon |                | Response | Conc       | Units | Dev(Min) |
|-------------------------------|-----------|----------------|----------|------------|-------|----------|
| -----                         |           |                |          |            |       |          |
| Internal Standards            |           |                |          |            |       |          |
| 1) 1,4-Difluorobenzene        | 5.619     | 114            | 133798   | 5.000      | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 8.854     | 117            | 132609   | 5.000      | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249    | 152            | 62974    | 5.000      | ug/L  | 0.00     |
|                               |           |                |          |            |       |          |
| System Monitoring Compounds   |           |                |          |            |       |          |
| 4) Vinyl Chloride-d3          | 1.307     | 65             | 44715    | 5.335      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 40 - 130 | Recovery | = 106.600% |       |          |
| 7) Chloroethane-d5            | 1.568     | 69             | 37152    | 5.438      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 65 - 130 | Recovery | = 108.800% |       |          |
| 11) 1,1-Dichloroethene-d2     | 2.108     | 63             | 62602    | 3.990      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 60 - 125 | Recovery | = 79.800%  |       |          |
| 20) 2-Butanone-d5             | 3.886     | 46             | 86317    | 59.774     | ug/L  | -0.02    |
| Spiked Amount                 | 50.000    | Range 40 - 130 | Recovery | = 119.540% |       |          |
| 24) Chloroform-d              | 4.352     | 84             | 92654    | 5.187      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 70 - 125 | Recovery | = 103.800% |       |          |
| 26) 1,2-Dichloroethane-d4     | 5.034     | 65             | 43301    | 5.391      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 70 - 130 | Recovery | = 107.800% |       |          |
| 32) Benzene-d6                | 5.053     | 84             | 181212   | 5.326      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 70 - 125 | Recovery | = 106.600% |       |          |
| 36) 1,2-Dichloropropane-d6    | 6.069     | 67             | 54772    | 5.468      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 60 - 140 | Recovery | = 109.400% |       |          |
| 41) Toluene-d8                | 7.317     | 98             | 158453   | 4.970      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 70 - 130 | Recovery | = 99.400%  |       |          |
| 43) trans-1,3-Dichloroprop... | 7.625     | 79             | 19629    | 5.168      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 55 - 130 | Recovery | = 103.400% |       |          |
| 46) 2-Hexanone-d5             | 8.088     | 63             | 70453    | 50.419     | ug/L  | 0.00     |
| Spiked Amount                 | 50.000    | Range 45 - 130 | Recovery | = 100.840% |       |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217    | 84             | 35857    | 4.978      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 65 - 120 | Recovery | = 99.600%  |       |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.625    | 152            | 61284    | 5.844      | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 80 - 120 | Recovery | = 116.800% |       |          |
|                               |           |                |          |            |       |          |
| Target Compounds              |           |                |          |            |       | Qvalue   |
| 13) Acetone                   | 2.182     | 43             | 2949     | 3.342      | ug/L  | 94       |
| -----                         |           |                |          |            |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110421\  
Data File : VV023209.D  
Acq On : 04 Nov 2021 17:56  
Operator : SY/MD  
Sample : M4445-11  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BG385

Quant Time: Nov 09 01:21:35 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Mon Nov 08 13:19:52 2021  
Response via : Initial Calibration

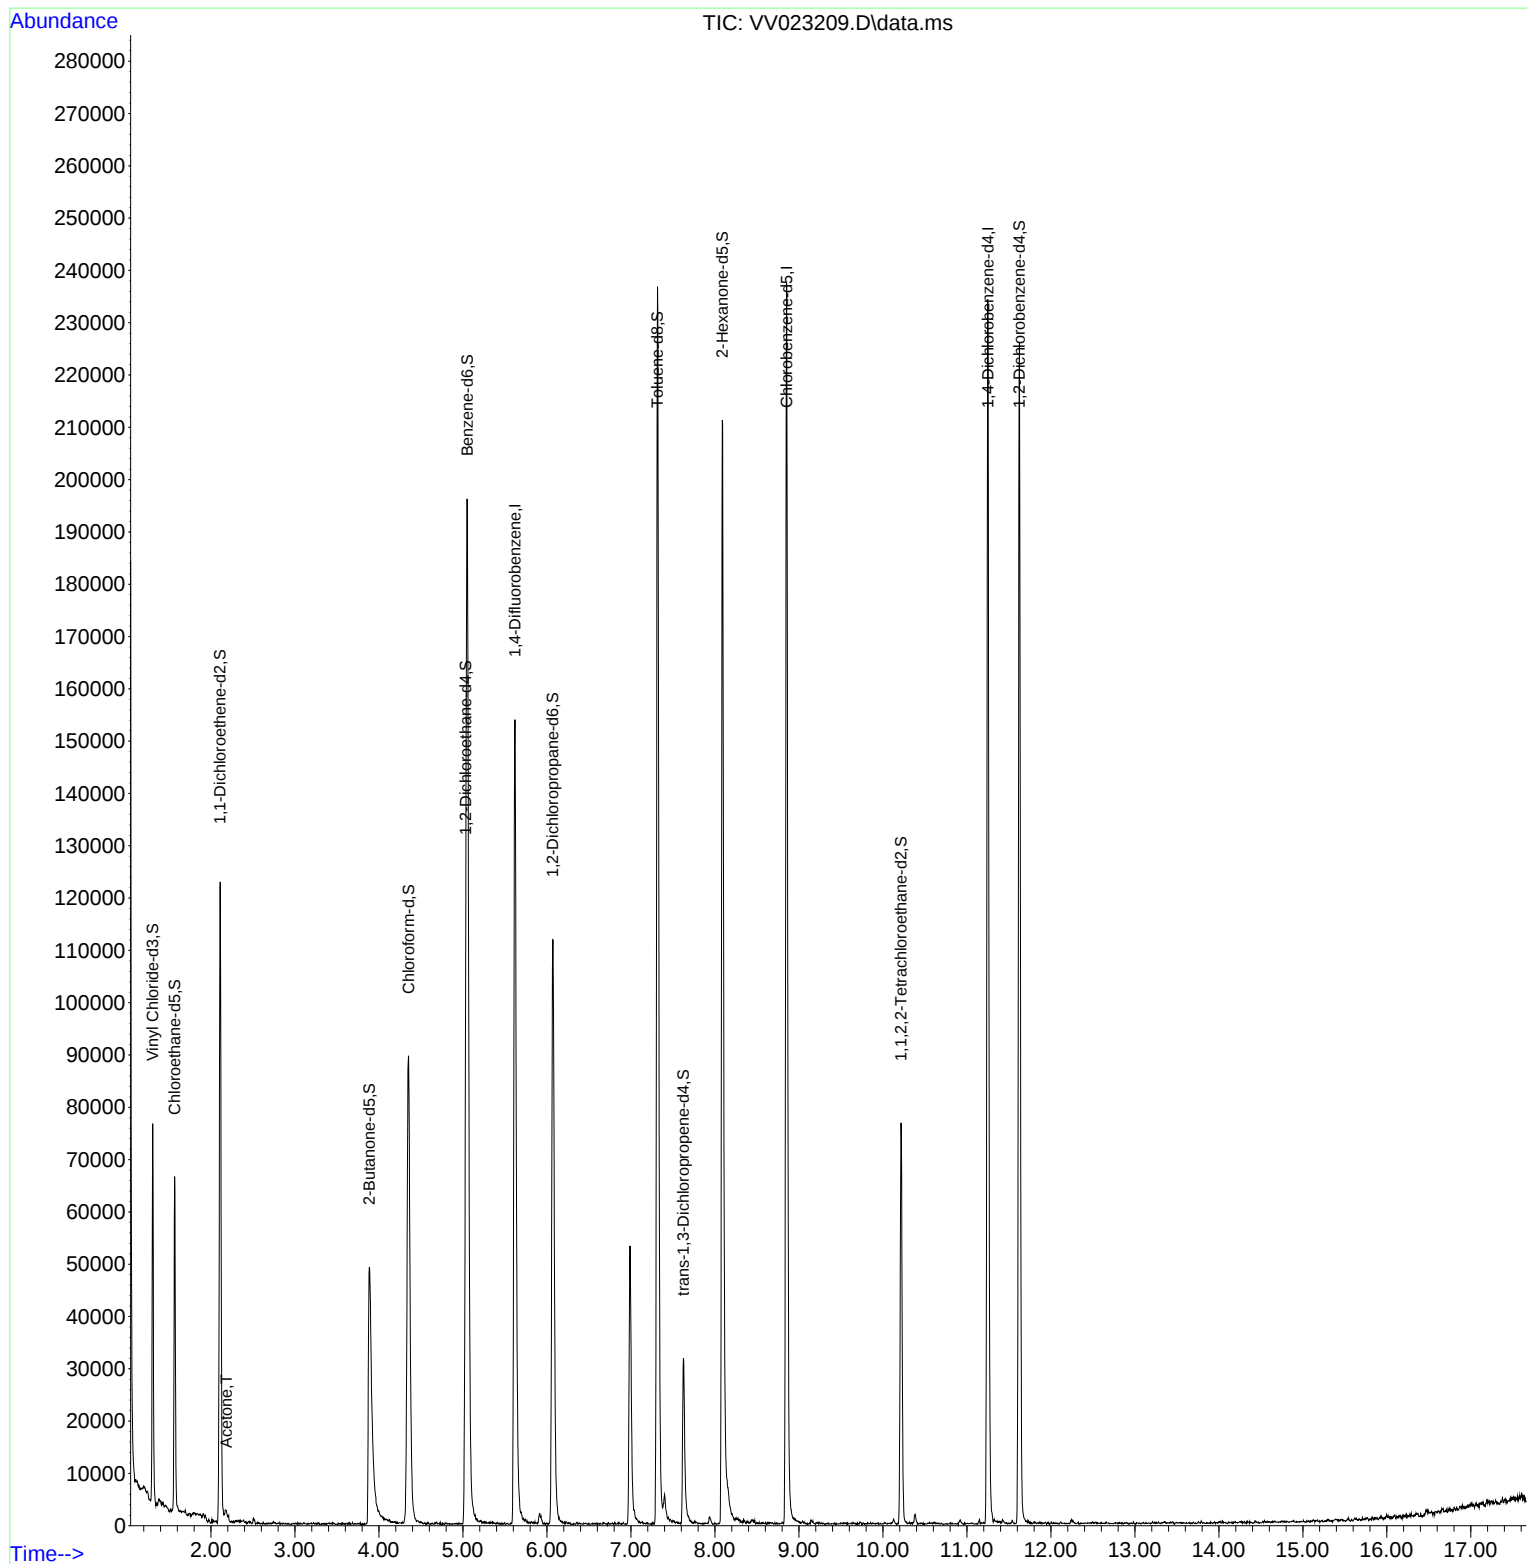

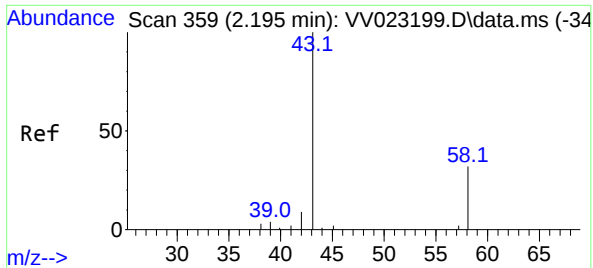

#13  
Acetone  
Concen: 3.342 ug/L  
RT: 2.182 min Scan# 31  
Delta R.T. -0.013 min  
Lab File: VV023209.D  
Acq: 04 Nov 2021 17:56

Instrument :  
MSVOA\_V  
ClientSampleId :  
BG385

Tgt Ion: 43 Resp: 2949  
Ion Ratio Lower Upper  
43 100  
58 30.8 0.0 55.4

