

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110421\  
 Data File : VV023210.D  
 Acq On : 04 Nov 2021 18:19  
 Operator : SY/MD  
 Sample : M4445-12  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BG386

Quant Time: Nov 09 01:23:59 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Mon Nov 08 13:19:52 2021  
 Response via : Initial Calibration


| Compound                      |        | R.T.   | QIon     | Response | Conc   | Units    | Dev(Min)  |
|-------------------------------|--------|--------|----------|----------|--------|----------|-----------|
| -----                         |        |        |          |          |        |          |           |
| Internal Standards            |        |        |          |          |        |          |           |
| 1) 1,4-Difluorobenzene        |        | 5.619  | 114      | 129739   | 5.000  | ug/L     | 0.00      |
| 28) Chlorobenzene-d5          |        | 8.853  | 117      | 129886   | 5.000  | ug/L     | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    |        | 11.249 | 152      | 61070    | 5.000  | ug/L     | 0.00      |
| System Monitoring Compounds   |        |        |          |          |        |          |           |
| 4) Vinyl Chloride-d3          |        | 1.307  | 65       | 41690    | 5.129  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 40 - 130 | Recovery | =      | 102.600% |           |
| 7) Chloroethane-d5            |        | 1.568  | 69       | 34822    | 5.257  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 65 - 130 | Recovery | =      | 105.200% |           |
| 11) 1,1-Dichloroethene-d2     |        | 2.111  | 63       | 58471    | 3.843  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 60 - 125 | Recovery | =      | 76.800%  |           |
| 20) 2-Butanone-d5             |        | 3.889  | 46       | 84687    | 60.480 | ug/L     | -0.01     |
| Spiked Amount                 | 50.000 | Range  | 40 - 130 | Recovery | =      | 120.960% |           |
| 24) Chloroform-d              |        | 4.352  | 84       | 85677    | 4.946  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 70 - 125 | Recovery | =      | 99.000%  |           |
| 26) 1,2-Dichloroethane-d4     |        | 5.034  | 65       | 40555    | 5.207  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 70 - 130 | Recovery | =      | 104.200% |           |
| 32) Benzene-d6                |        | 5.053  | 84       | 165337   | 4.961  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 70 - 125 | Recovery | =      | 99.200%  |           |
| 36) 1,2-Dichloropropane-d6    |        | 6.072  | 67       | 50196    | 5.117  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 60 - 140 | Recovery | =      | 102.400% |           |
| 41) Toluene-d8                |        | 7.317  | 98       | 146140   | 4.680  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 70 - 130 | Recovery | =      | 93.600%  |           |
| 43) trans-1,3-Dichloroprop... |        | 7.625  | 79       | 18564    | 4.990  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 55 - 130 | Recovery | =      | 99.800%  |           |
| 46) 2-Hexanone-d5             |        | 8.088  | 63       | 65237    | 47.665 | ug/L     | 0.00      |
| Spiked Amount                 | 50.000 | Range  | 45 - 130 | Recovery | =      | 95.340%  |           |
| 56) 1,1,2,2-Tetrachloroeth... |        | 10.217 | 84       | 33538    | 4.754  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 65 - 120 | Recovery | =      | 95.000%  |           |
| 66) 1,2-Dichlorobenzene-d4    |        | 11.625 | 152      | 55011    | 5.410  | ug/L     | 0.00      |
| Spiked Amount                 | 5.000  | Range  | 80 - 120 | Recovery | =      | 108.200% |           |
| Target Compounds              |        |        |          |          |        |          |           |
| 13) Acetone                   |        | 2.182  | 43       | 3984     | 4.656  | ug/L     | Qvalue 99 |
| -----                         |        |        |          |          |        |          |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110421\  
Data File : VV023210.D  
Acq On : 04 Nov 2021 18:19  
Operator : SY/MD  
Sample : M4445-12  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BG386

Quant Time: Nov 09 01:23:59 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Mon Nov 08 13:19:52 2021  
Response via : Initial Calibration

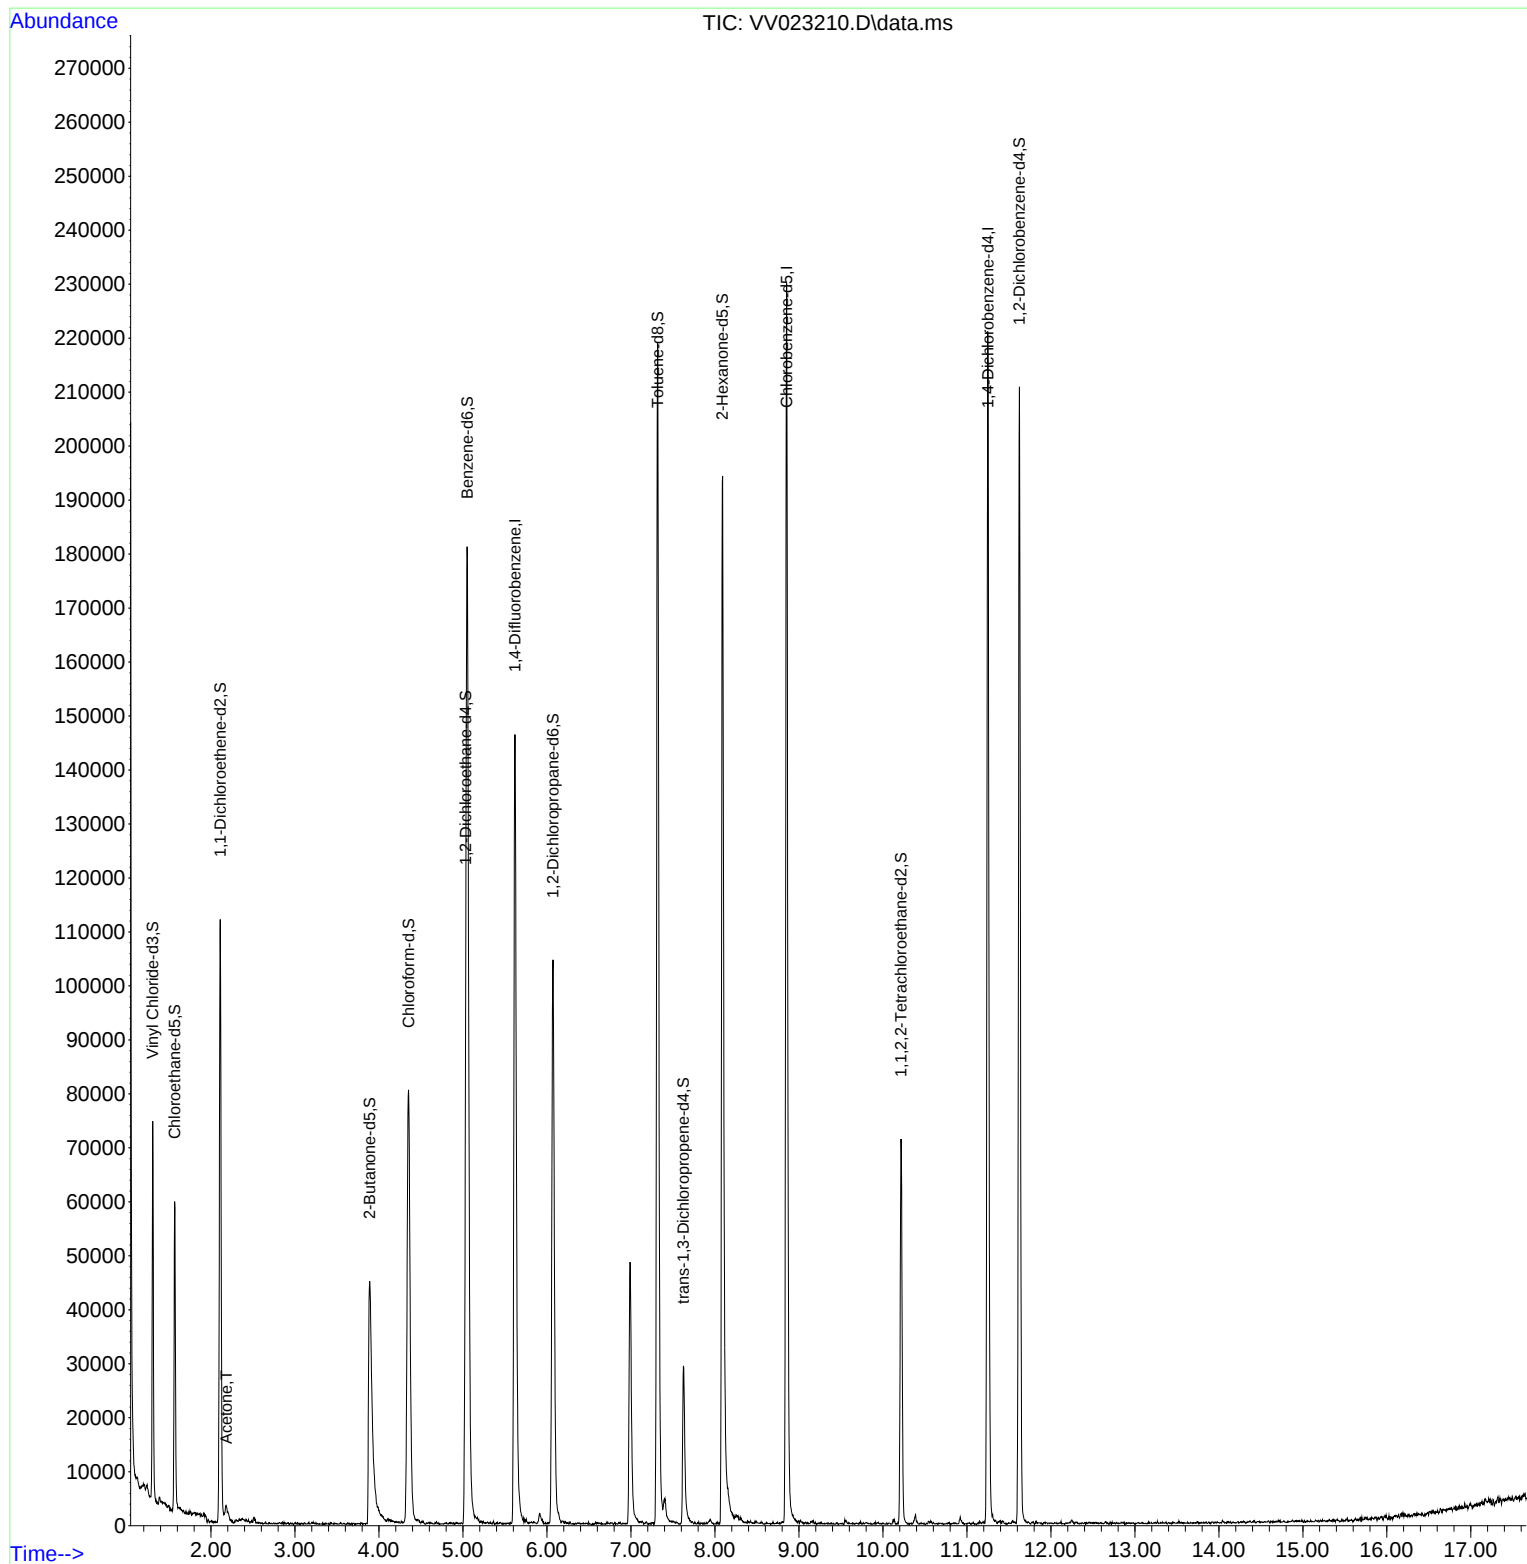

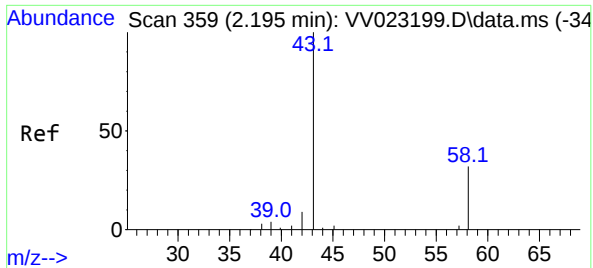

#13  
Acetone  
Concen: 4.656 ug/L  
RT: 2.182 min Scan# 31  
Delta R.T. -0.013 min  
Lab File: VV023210.D  
Acq: 04 Nov 2021 18:19

Instrument :  
MSVOA\_V  
ClientSampleId :  
BG386

Tgt Ion: 43 Resp: 3984  
Ion Ratio Lower Upper  
43 100  
58 28.1 0.0 55.4

