

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023211.D
 Acq On : 04 Nov 2021 18:43
 Operator : SY/MD
 Sample : M4445-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG387

Quant Time: Nov 09 01:25:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 13:19:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	133570	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	131917	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61869	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42565	5.087	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	101.800%	
7) Chloroethane-d5	1.568	69	35031	5.137	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	102.800%	
11) 1,1-Dichloroethene-d2	2.111	63	59819	3.819	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	76.400%	
20) 2-Butanone-d5	3.889	46	88142	61.142	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	122.280%	
24) Chloroform-d	4.352	84	89808	5.036	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.800%	
26) 1,2-Dichloroethane-d4	5.034	65	42032	5.242	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.800%	
32) Benzene-d6	5.053	84	172566	5.098	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.000%	
36) 1,2-Dichloropropane-d6	6.069	67	51349	5.154	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.000%	
41) Toluene-d8	7.317	98	151897	4.789	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.800%	
43) trans-1,3-Dichloroprop...	7.625	79	18647	4.936	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	98.800%	
46) 2-Hexanone-d5	8.088	63	69385	49.915	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.840%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34968	4.880	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	57976	5.628	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.600%	
Target Compounds					Qvalue	
13) Acetone	2.182	43	4018	4.561	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023211.D
Acq On : 04 Nov 2021 18:43
Operator : SY/MD
Sample : M4445-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG387

Quant Time: Nov 09 01:25:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 13:19:52 2021
Response via : Initial Calibration

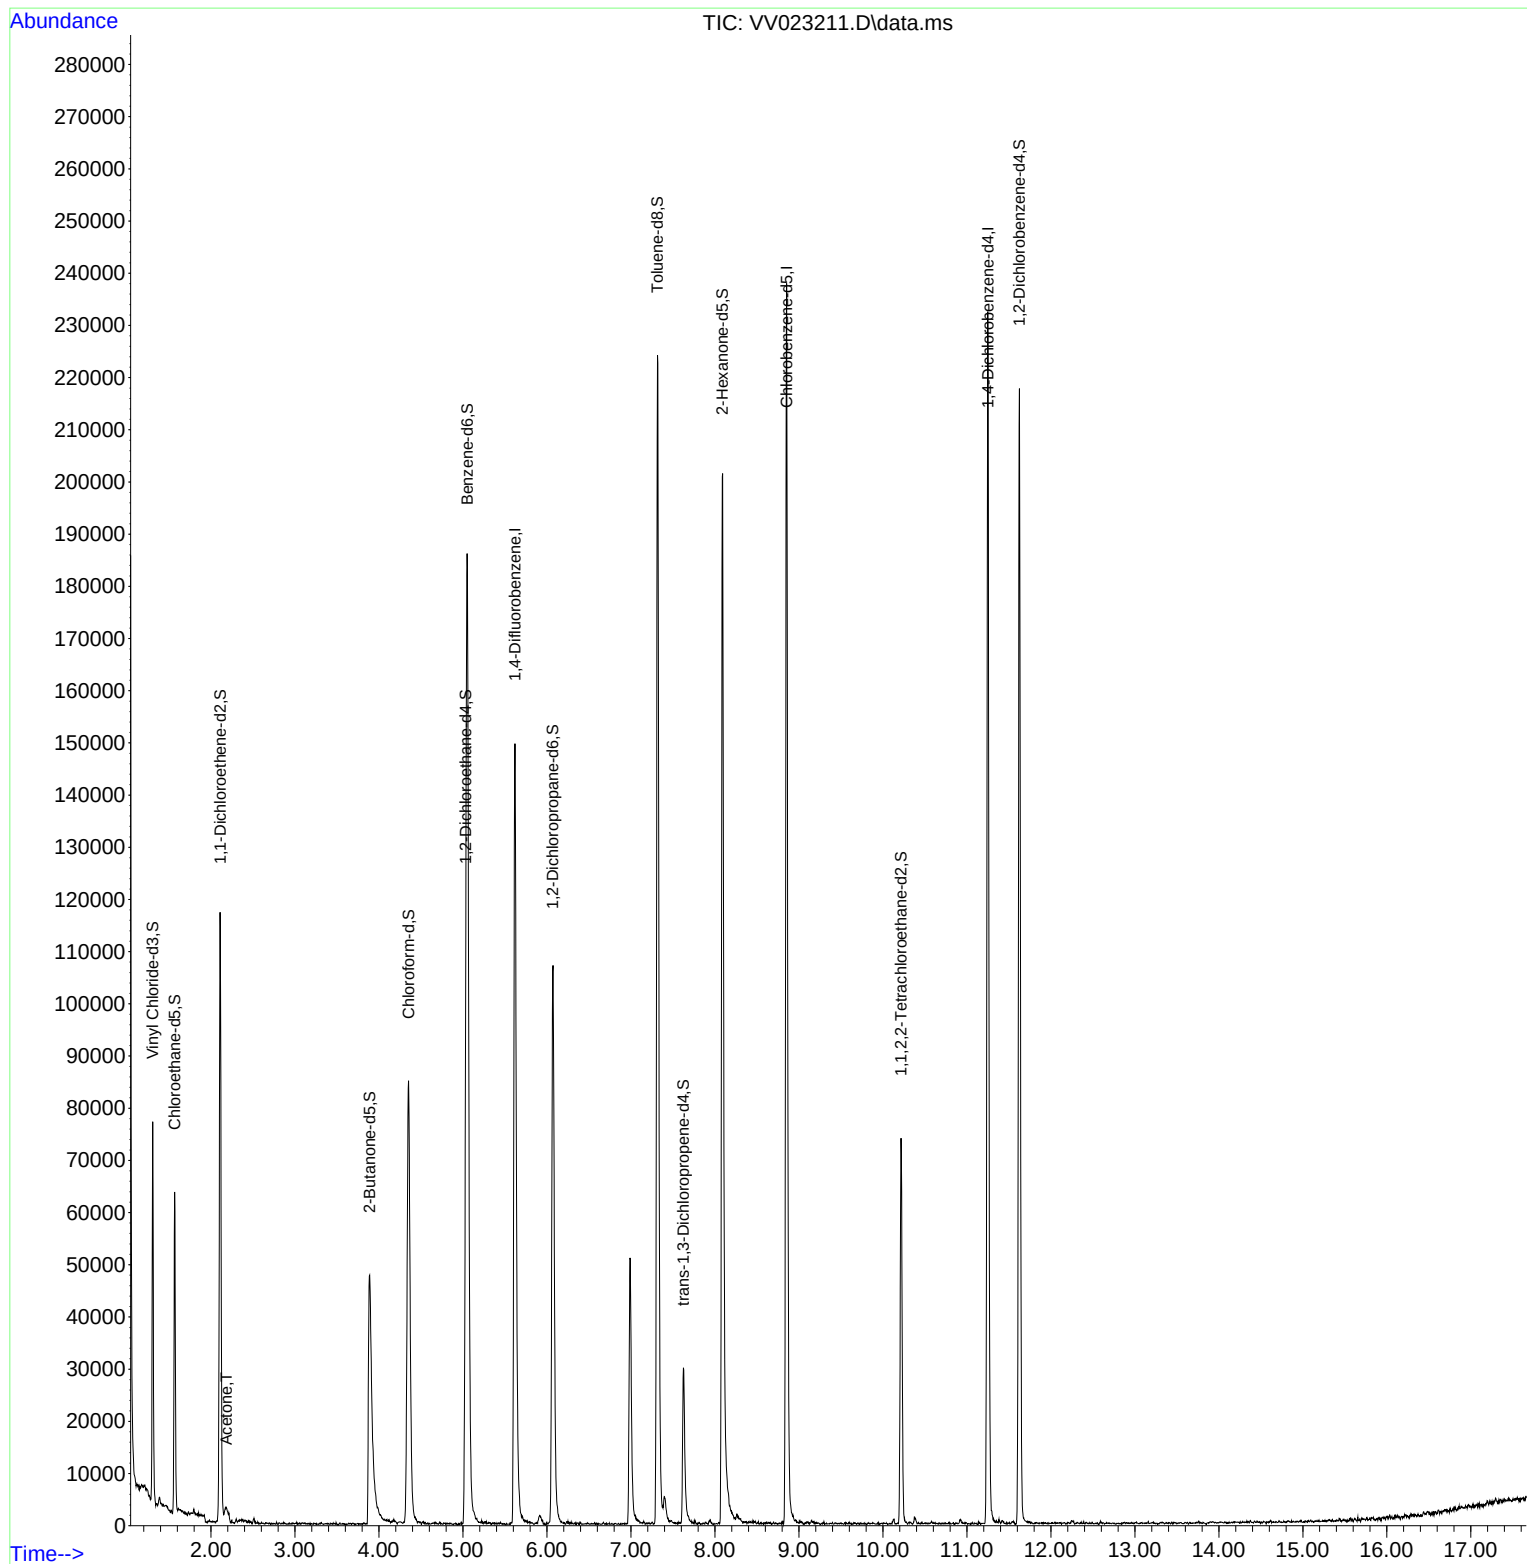

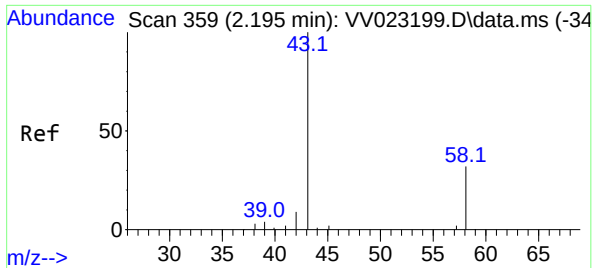

#13
Acetone
Concen: 4.561 ug/L
RT: 2.182 min Scan# 31
Delta R.T. -0.013 min
Lab File: VV023211.D
Acq: 04 Nov 2021 18:43

Instrument :
MSVOA_V
ClientSampleId :
BG387

Tgt Ion: 43 Resp: 4018
Ion Ratio Lower Upper
43 100
58 32.1 0.0 55.4

