

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023212.D
 Acq On : 04 Nov 2021 19:06
 Operator : SY/MD
 Sample : M4445-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG388

Quant Time: Nov 09 01:27:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 13:19:52 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	129371	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	129873	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59059	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	44887	5.538	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 110.800%		
7) Chloroethane-d5	1.568	69	35822	5.423	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 108.400%		
11) 1,1-Dichloroethene-d2	2.111	63	59414	3.916	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 78.400%		
20) 2-Butanone-d5	3.889	46	86765	62.140	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	= 124.280%		
24) Chloroform-d	4.352	84	89281	5.169	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 103.400%		
26) 1,2-Dichloroethane-d4	5.037	65	42367	5.455	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 109.000%		
32) Benzene-d6	5.053	84	173228	5.198	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 104.000%		
36) 1,2-Dichloropropane-d6	6.072	67	52325	5.334	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 106.600%		
41) Toluene-d8	7.317	98	151026	4.836	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 96.800%		
43) trans-1,3-Dichloroprop...	7.625	79	18305	4.921	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 98.400%		
46) 2-Hexanone-d5	8.088	63	67413	49.260	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 98.520%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34920	4.950	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 99.000%		
66) 1,2-Dichlorobenzene-d4	11.625	152	56856	5.782	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 115.600%		
Target Compounds						Qvalue
13) Acetone	2.175	43	2548	2.987	ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023212.D
Acq On : 04 Nov 2021 19:06
Operator : SY/MD
Sample : M4445-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG388

Quant Time: Nov 09 01:27:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 13:19:52 2021
Response via : Initial Calibration

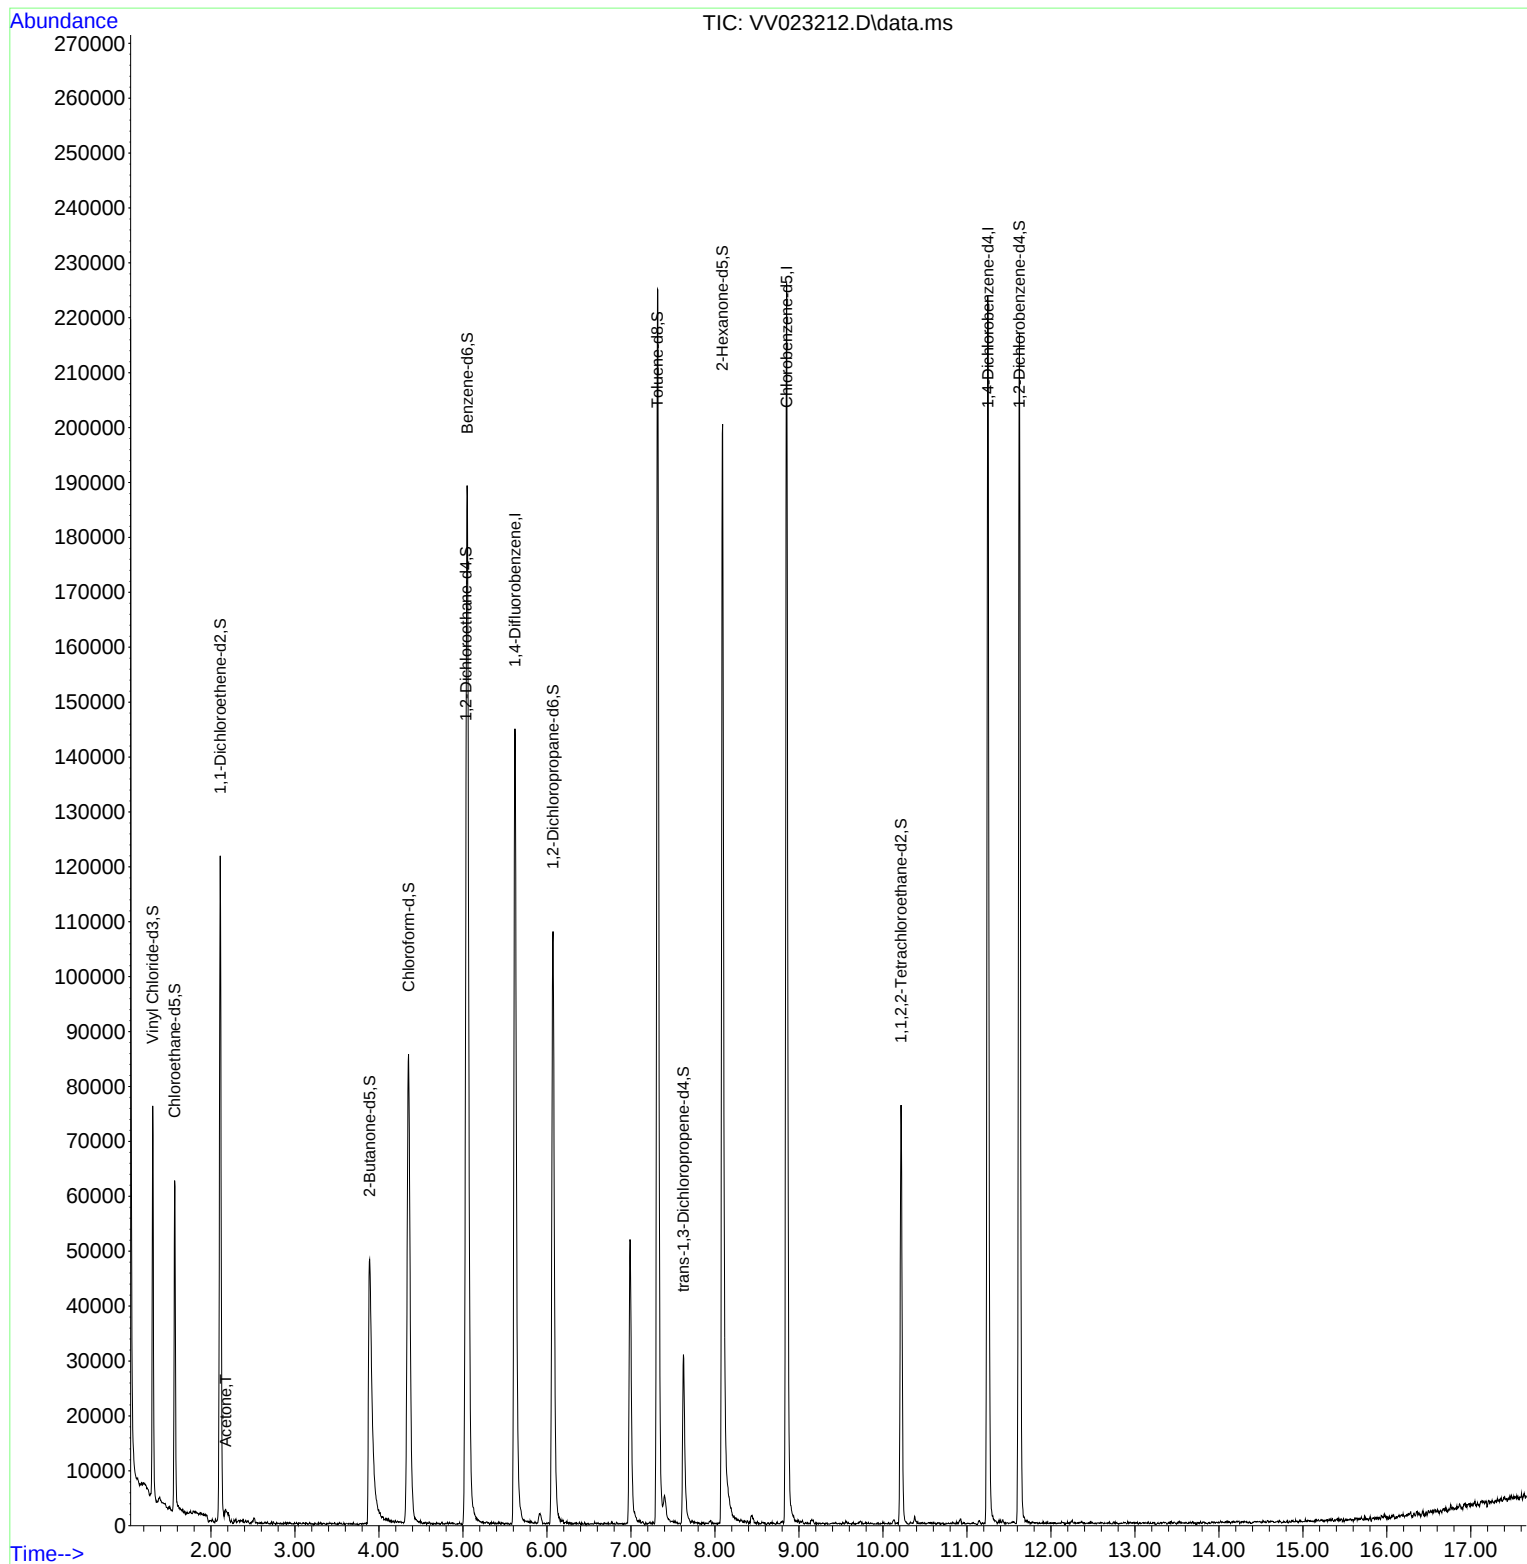

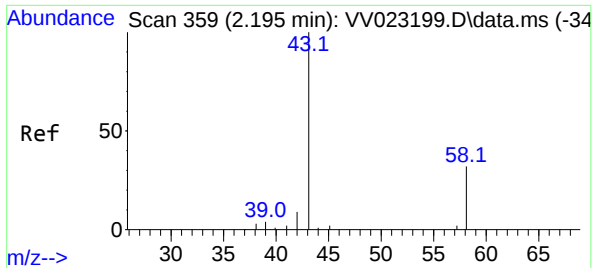

#13
Acetone
Concen: 2.987 ug/L
RT: 2.175 min Scan# 31
Delta R.T. -0.019 min
Lab File: VV023212.D
Acq: 04 Nov 2021 19:06

Instrument :
MSVOA_V
ClientSampleId :
BG388

Tgt Ion: 43 Resp: 2548
Ion Ratio Lower Upper
43 100
58 13.4 0.0 55.4

