

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023213.D
 Acq On : 04 Nov 2021 19:29
 Operator : SY/MD
 Sample : M4445-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG389

Quant Time: Nov 09 01:29:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 13:19:52 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	129798	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	129802	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61797	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	41818	5.143	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 102.800%		
7) Chloroethane-d5	1.568	69	35186	5.309	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 106.200%		
11) 1,1-Dichloroethene-d2	2.111	63	59924	3.937	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 78.800%		
20) 2-Butanone-d5	3.886	46	82576	58.946	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	= 117.900%		
24) Chloroform-d	4.352	84	88074	5.082	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 101.600%		
26) 1,2-Dichloroethane-d4	5.034	65	41938	5.382	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 107.600%		
32) Benzene-d6	5.053	84	168797	5.068	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 101.400%		
36) 1,2-Dichloropropane-d6	6.072	67	51086	5.211	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 104.200%		
41) Toluene-d8	7.317	98	150001	4.806	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 96.200%		
43) trans-1,3-Dichloroprop...	7.628	79	18364	4.940	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 98.800%		
46) 2-Hexanone-d5	8.088	63	66165	48.374	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 96.740%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34285	4.863	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 97.200%		
66) 1,2-Dichlorobenzene-d4	11.625	152	57393	5.578	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 111.600%		
Target Compounds						Qvalue
13) Acetone	2.185	43	3129	3.655	ug/L	92




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023213.D
Acq On : 04 Nov 2021 19:29
Operator : SY/MD
Sample : M4445-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG389

Quant Time: Nov 09 01:29:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 13:19:52 2021
Response via : Initial Calibration

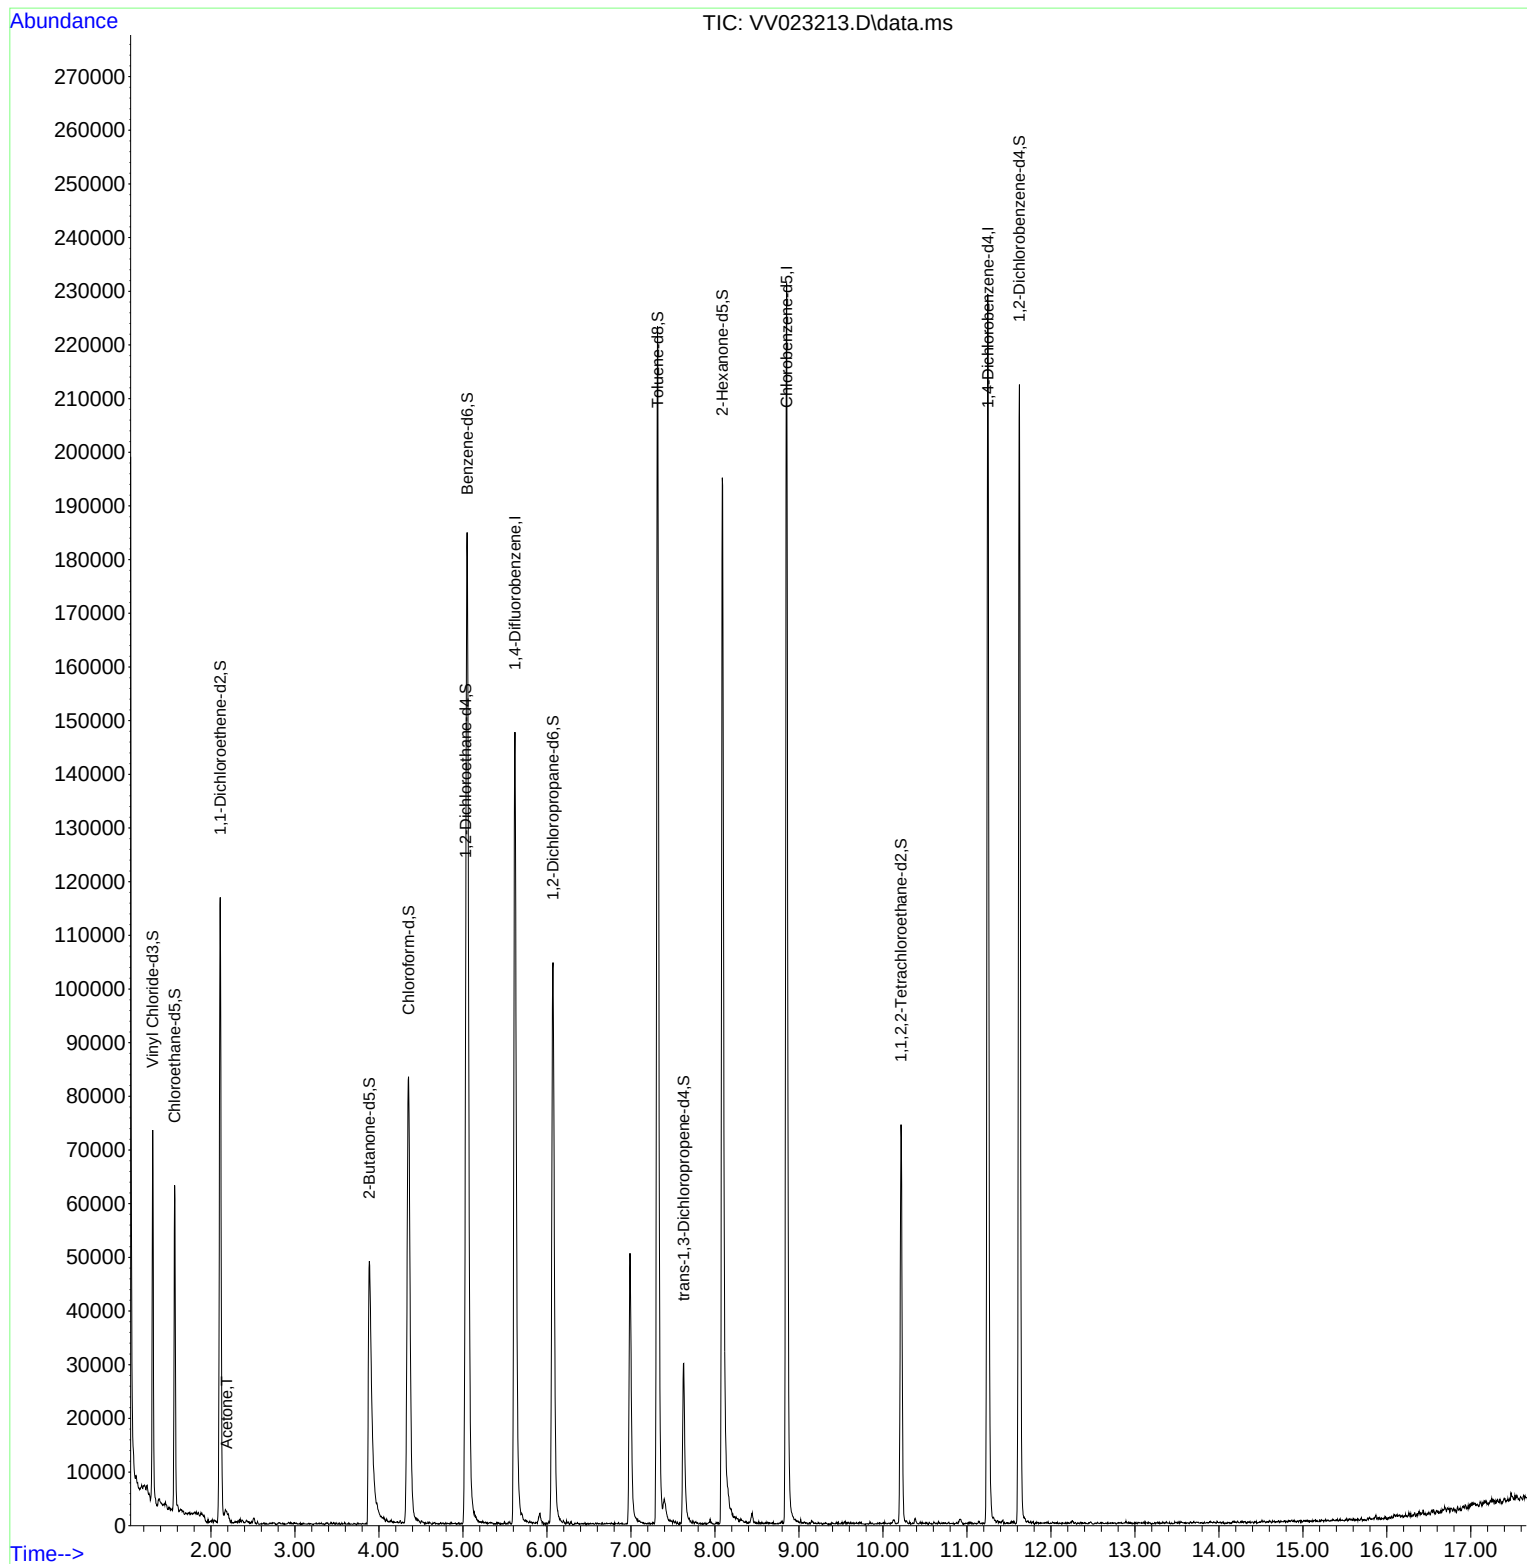

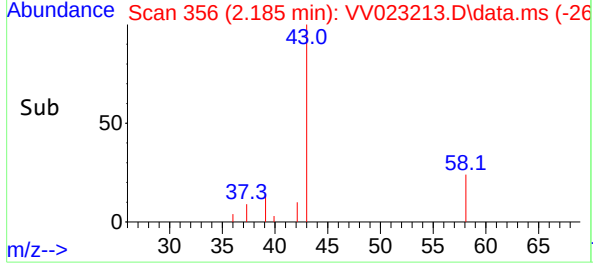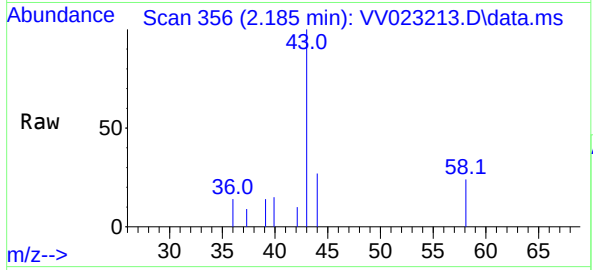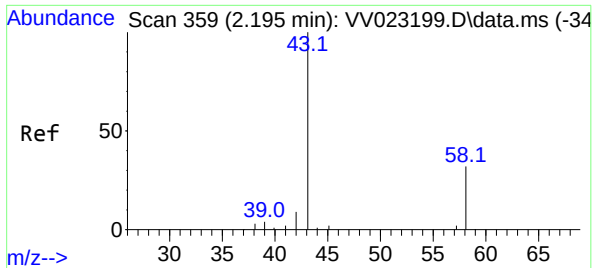

#13
 Acetone
 Concen: 3.655 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV023213.D
 Acq: 04 Nov 2021 19:29

Tgt Ion: 43 Resp: 3129
 Ion Ratio Lower Upper
 43 100
 58 23.4 0.0 55.4

Instrument :
 MSVOA_V
 ClientSampleId :
 BG389

