

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023214.D
 Acq On : 04 Nov 2021 19:53
 Operator : SY/MD
 Sample : M4445-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG390

Quant Time: Nov 09 01:30:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 13:19:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	131465	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	132654	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61422	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	44168	5.363	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	107.200%	
7) Chloroethane-d5	1.568	69	36077	5.375	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	107.400%	
11) 1,1-Dichloroethene-d2	2.111	63	59837	3.881	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	77.600%	
20) 2-Butanone-d5	3.889	46	89025	62.743	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	125.480%	
24) Chloroform-d	4.352	84	91068	5.189	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.800%	
26) 1,2-Dichloroethane-d4	5.034	65	42289	5.358	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.200%	
32) Benzene-d6	5.053	84	174069	5.114	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.200%	
36) 1,2-Dichloropropane-d6	6.072	67	53416	5.331	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.600%	
41) Toluene-d8	7.317	98	149044	4.673	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.400%	
43) trans-1,3-Dichloroprop...	7.625	79	18599	4.896	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	98.000%	
46) 2-Hexanone-d5	8.088	63	69174	49.487	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.980%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35353	4.907	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	58851	5.754	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	115.000%	
Target Compounds					Qvalue	
13) Acetone	2.179	43	3490	4.025	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023214.D
Acq On : 04 Nov 2021 19:53
Operator : SY/MD
Sample : M4445-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG390

Quant Time: Nov 09 01:30:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 13:19:52 2021
Response via : Initial Calibration

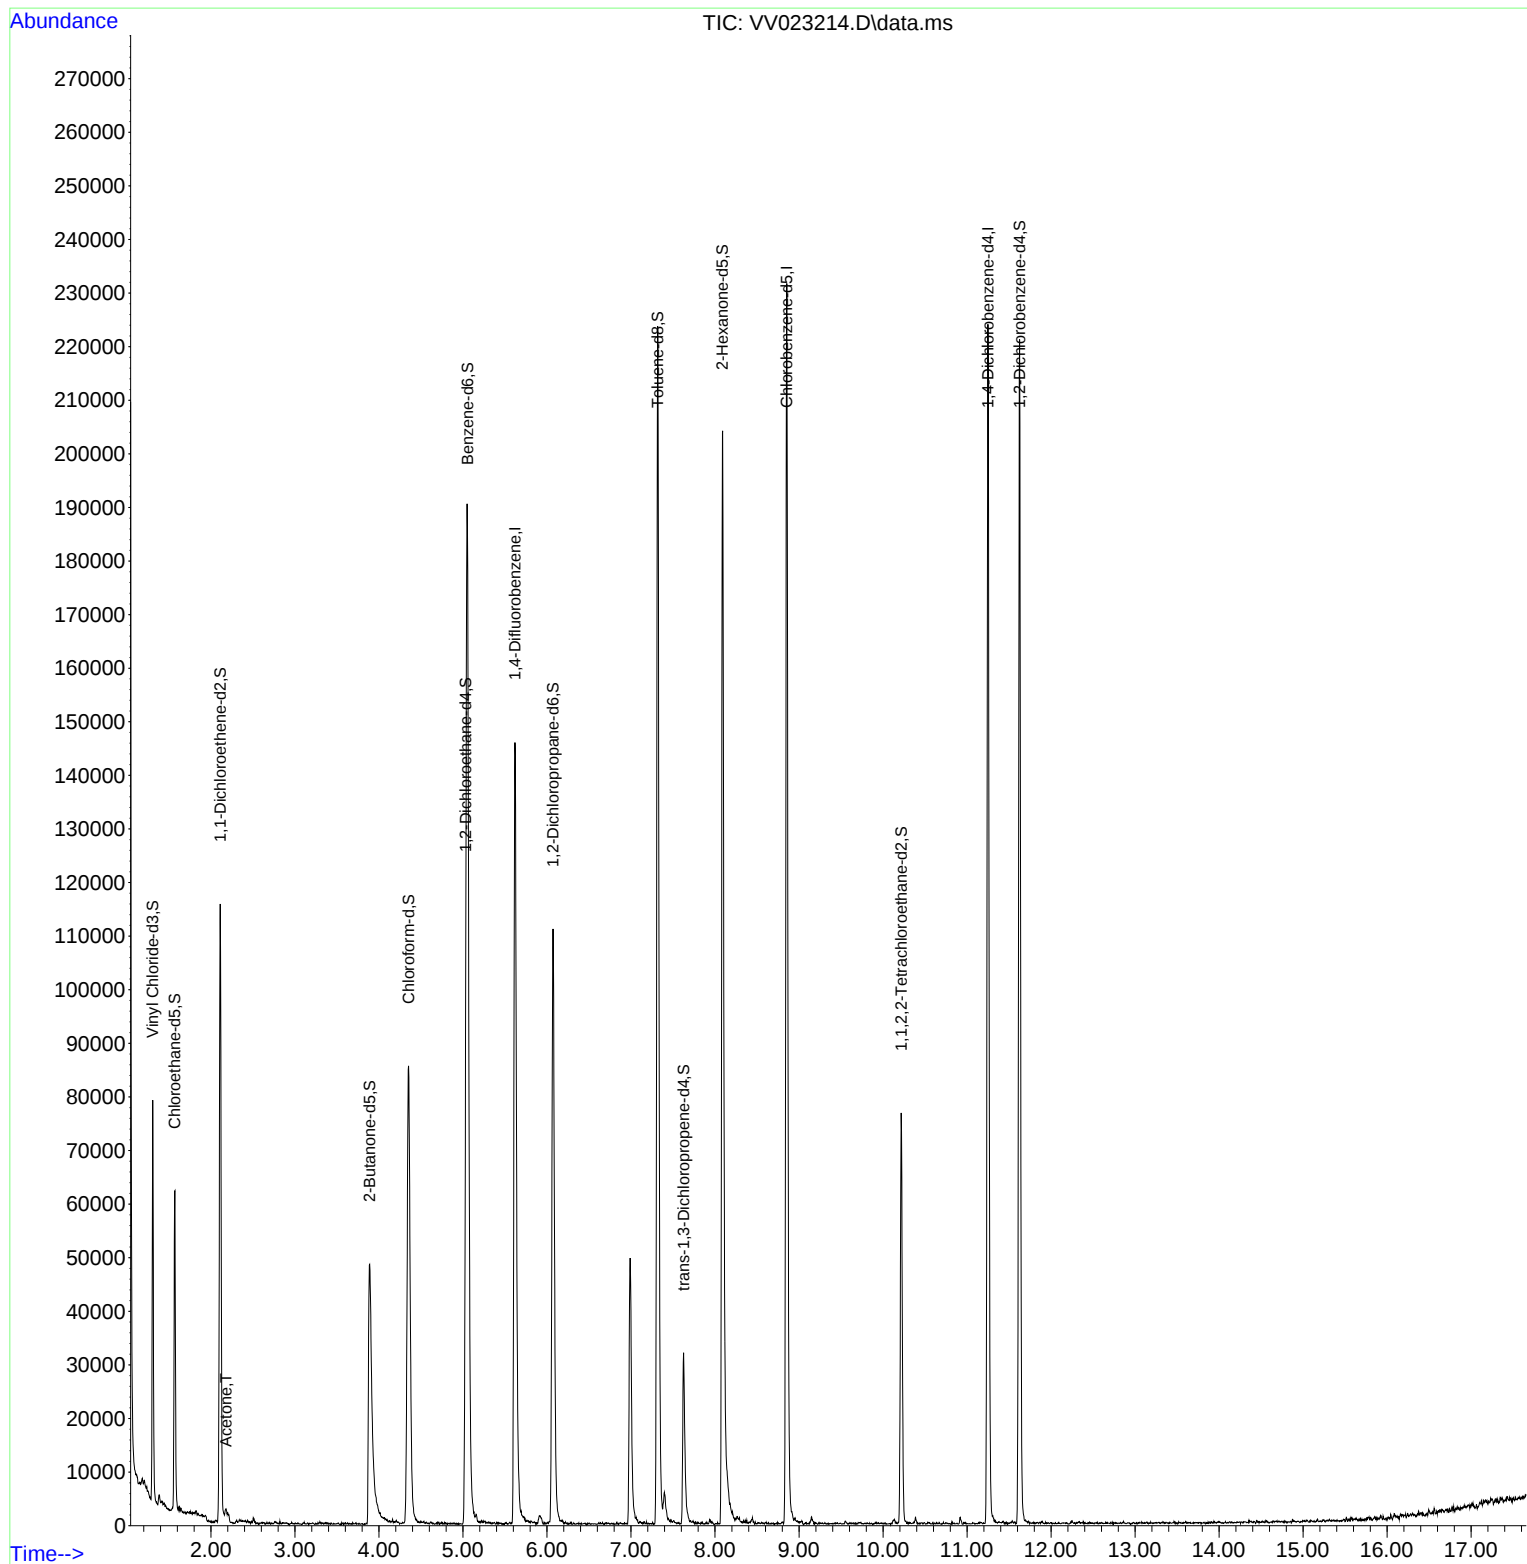

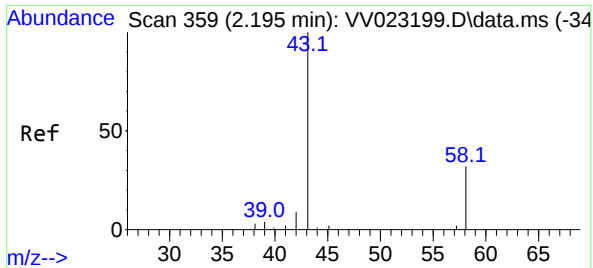

#13
Acetone
Concen: 4.025 ug/L
RT: 2.179 min Scan# 31
Delta R.T. -0.016 min
Lab File: VV023214.D
Acq: 04 Nov 2021 19:53

Instrument :
MSVOA_V
ClientSampleId :
BG390

Tgt Ion: 43 Resp: 3490
Ion Ratio Lower Upper
43 100
58 26.9 0.0 55.4

