

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023215.D
 Acq On : 04 Nov 2021 20:16
 Operator : SY/MD
 Sample : M4445-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG391

Quant Time: Nov 09 01:32:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 08 13:19:52 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.619	114	130297	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.853	117	129663	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.249	152	59805	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.307	65	41775	5.118	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.400%	
7) Chloroethane-d5		1.568	69	35028	5.265	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.400%	
11) 1,1-Dichloroethene-d2		2.111	63	57239	3.746	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.000%	
20) 2-Butanone-d5		3.886	46	84539	60.116	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.240%	
24) Chloroform-d		4.352	84	86699	4.984	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%	
26) 1,2-Dichloroethane-d4		5.037	65	41276	5.277	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.600%	
32) Benzene-d6		5.053	84	168856	5.075	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%	
36) 1,2-Dichloropropane-d6		6.072	67	49843	5.089	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.800%	
41) Toluene-d8		7.317	98	144487	4.635	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.600%	
43) trans-1,3-Dichloroprop...		7.625	79	17588	4.736	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.800%	
46) 2-Hexanone-d5		8.088	63	65777	48.142	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.280%	
56) 1,1,2,2-Tetrachloroeth...		10.217	84	33542	4.763	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.200%	
66) 1,2-Dichlorobenzene-d4		11.625	152	56941	5.718	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.400%	
Target Compounds							
13) Acetone		2.175	43	3278	3.815	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
Data File : VV023215.D
Acq On : 04 Nov 2021 20:16
Operator : SY/MD
Sample : M4445-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG391

Quant Time: Nov 09 01:32:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 08 13:19:52 2021
Response via : Initial Calibration

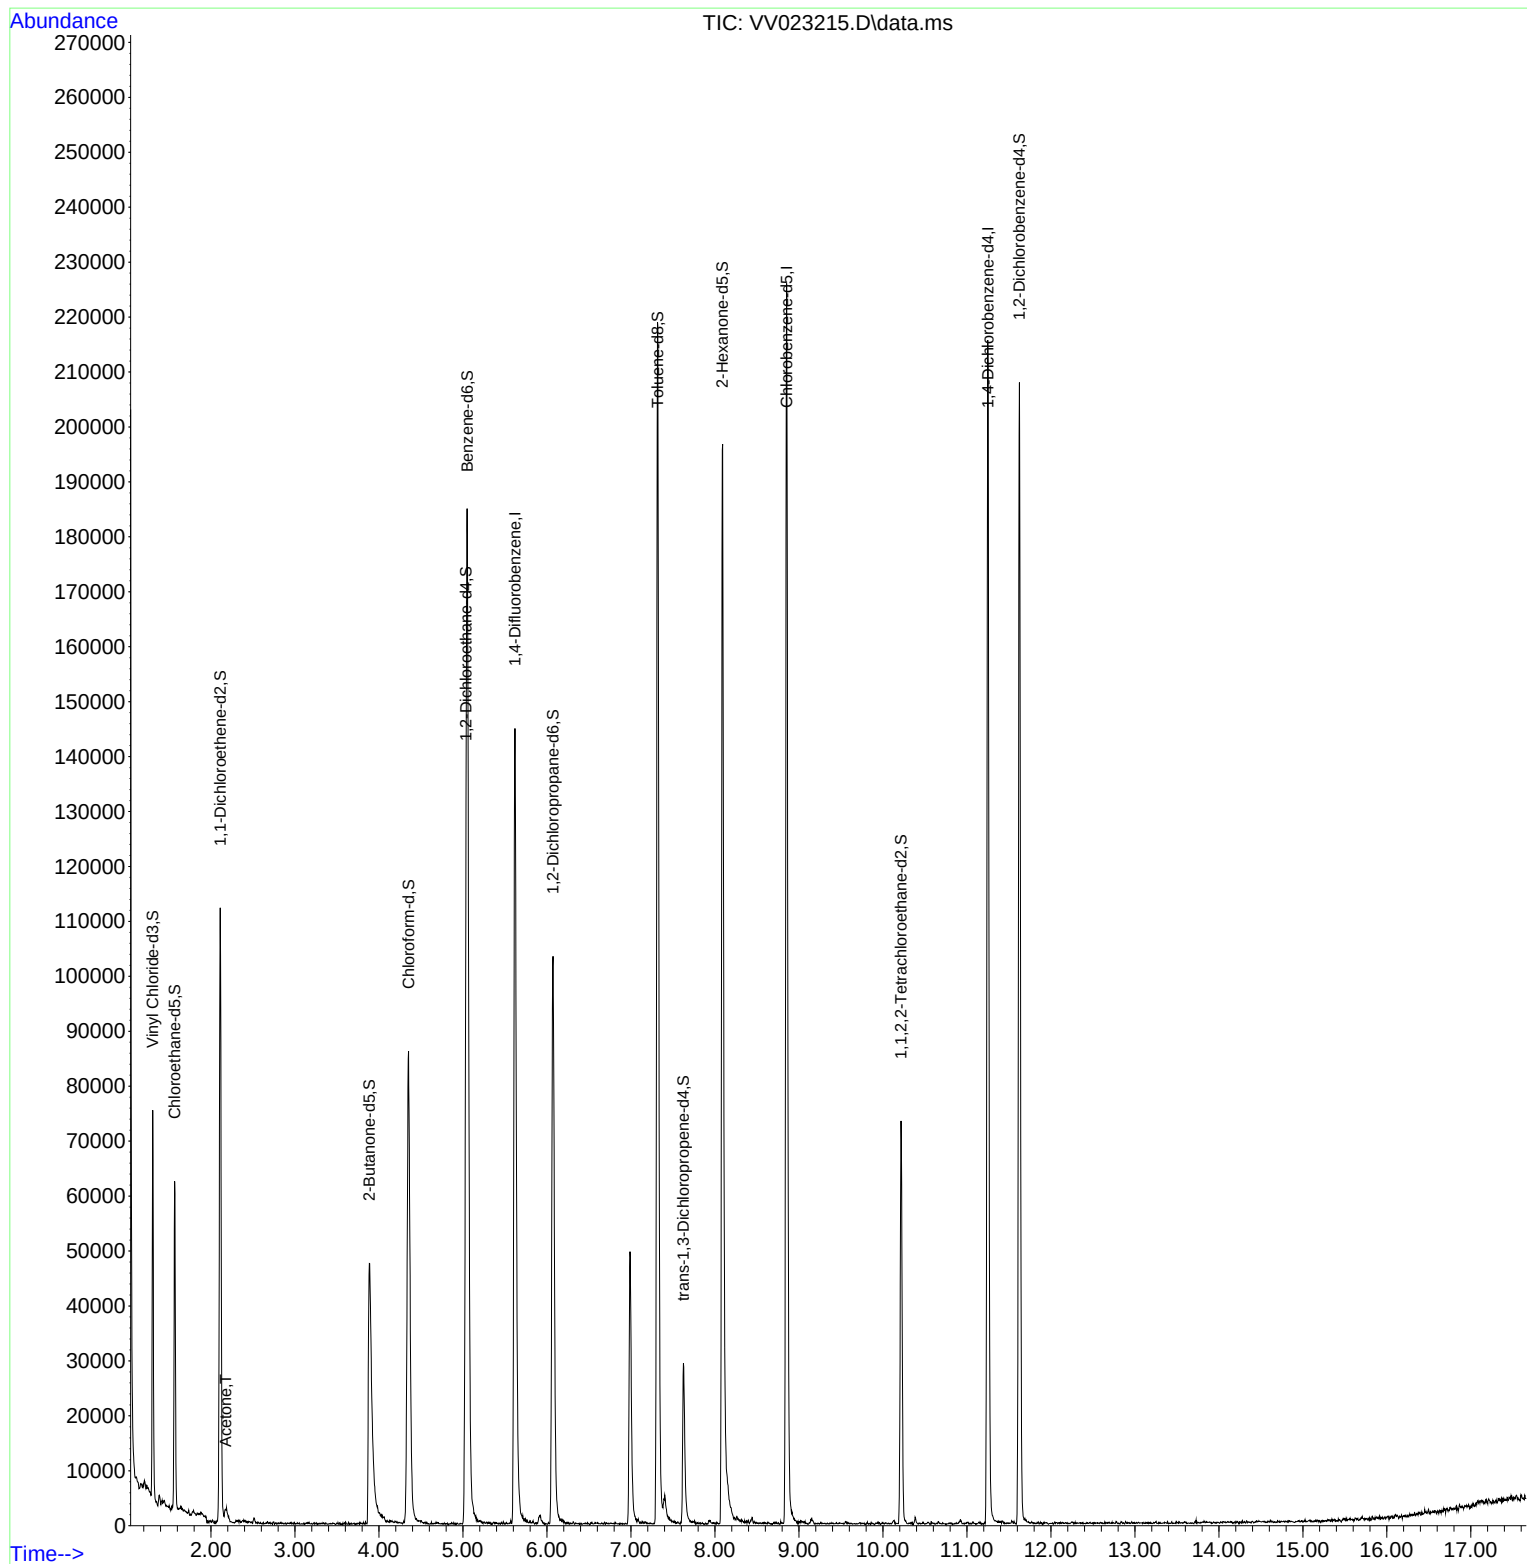

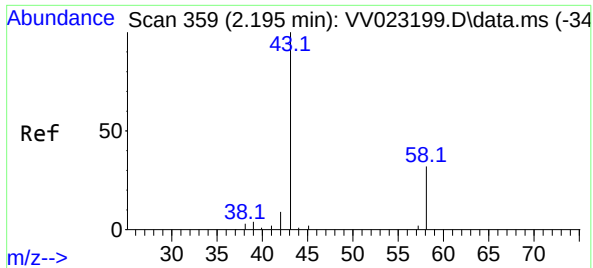

#13
Acetone
Concen: 3.815 ug/L
RT: 2.175 min Scan# 31
Delta R.T. -0.019 min
Lab File: VV023215.D
Acq: 04 Nov 2021 20:16

Instrument :
MSVOA_V
ClientSampleId :
BG391

Tgt Ion: 43 Resp: 3278
Ion Ratio Lower Upper
43 100
58 30.8 0.0 55.4

