
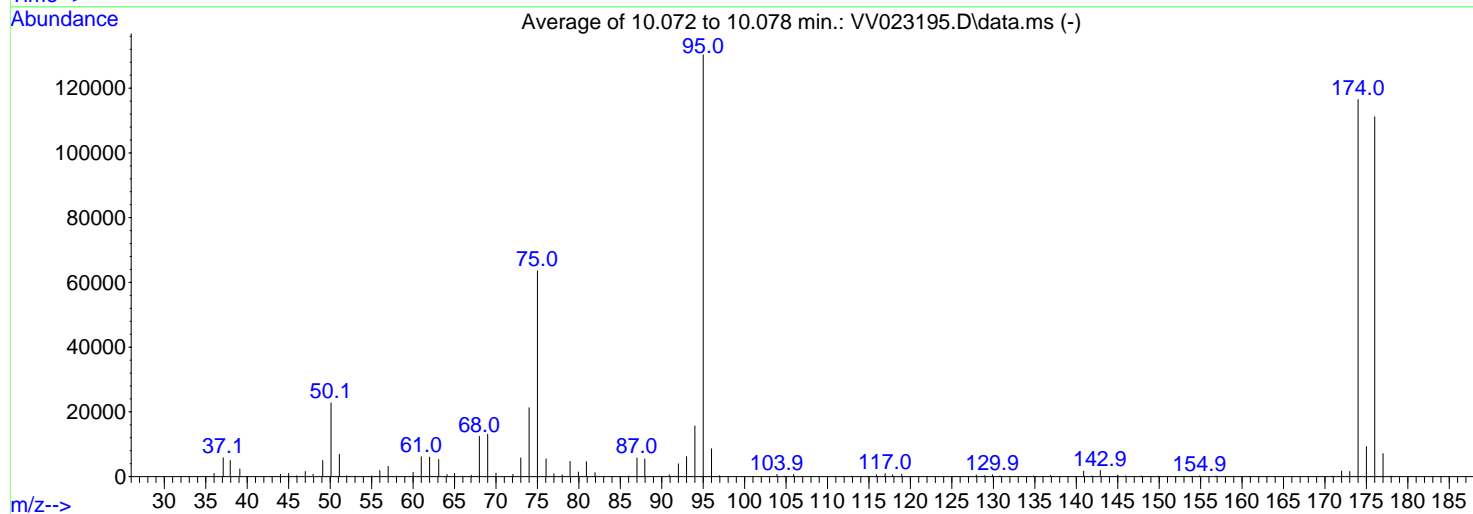


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110421\
 Data File : VV023195.D
 Acq On : 04 Nov 2021 11:14
 Operator : SY/MD
 Sample : BFB227
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB227

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Nov 11 08:19:32 2021

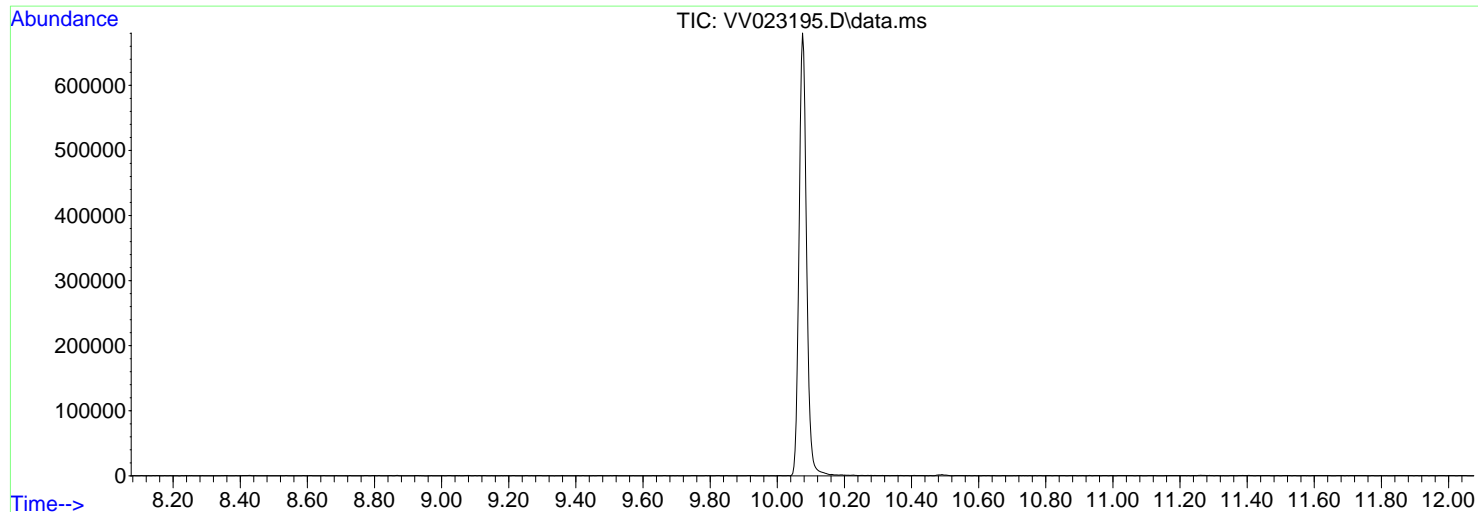

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	22797	PASS
75	95	30	80	48.8	63557	PASS
95	95	100	100	100.0	130288	PASS
96	95	5	9	6.6	8606	PASS
173	174	0.00	2	1.3	1568	PASS
174	95	50	120	89.4	116515	PASS
175	174	5	9	8.0	9277	PASS
176	174	95	105	95.4	111149	PASS
177	176	5	10	6.4	7143	PASS

m/z	Abundance
37.80	100.0
39.90	155.0
44.00	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	928.0
37.10	5532.0
38.00	5057.0
39.10	2329.0
39.90	282.0
42.80	118.0
44.00	954.0
45.00	1049.0
45.90	265.0
47.00	1579.0
48.00	729.0
49.10	4900.0
50.10	22512.0
51.10	7128.0
52.00	250.0
53.00	152.0
55.10	274.0
56.00	1834.0
57.00	3138.0
58.00	185.0
60.00	1309.0
61.00	6025.0
62.00	6035.0
63.10	5413.0
64.10	694.0
65.00	1085.0
65.90	160.0
67.00	317.0
68.00	12161.0
69.00	13165.0
70.00	1080.0
71.00	103.0
72.10	758.0
73.00	5552.0
74.00	20728.0
75.00	63000.0
76.00	5433.0
77.00	847.0
78.00	614.0
78.90	4494.0
80.00	1432.0
80.90	4466.0
81.90	1242.0
83.10	123.0
86.00	228.0
87.00	5730.0
88.00	5463.0
90.90	533.0
92.00	3900.0
93.00	6295.0
94.00	15570.0
95.00	126800.0
96.00	8618.0
97.00	327.0
103.90	645.0
104.80	177.0
105.90	625.0
106.90	171.0
110.00	104.0
110.90	170.0
112.00	135.0
112.90	146.0
114.80	166.0
115.90	489.0
117.00	896.0
117.90	602.0
119.00	827.0
127.90	497.0
128.90	326.0
129.90	521.0
130.80	214.0
134.90	269.0
136.90	337.0
140.10	125.0
140.90	1569.0
141.90	205.0
142.90	1886.0
144.00	160.0
145.00	556.0
145.90	324.0
147.10	138.0
147.80	201.0
150.00	138.0
152.00	101.0
153.10	132.0
154.90	325.0
156.90	178.0
159.00	159.0
161.00	156.0
170.80	174.0
171.20	221.0
172.00	1613.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

173.00	1593.0
174.00	110152.0
175.00	9087.0
176.00	105304.0
177.00	6985.0
177.90	202.0

Instrument :

MSVOA_V

ClientSampleId :

BFB227

m/z	Abundance
36.00	1028.0
37.10	6113.0
38.00	5274.0
39.10	2470.0
39.90	267.0
44.00	952.0
45.00	1033.0
45.90	274.0
47.00	1645.0
48.00	720.0
49.10	5175.0
50.10	23656.0
51.10	7131.0
52.00	248.0
53.10	181.0
55.00	275.0
56.00	1946.0
57.00	3211.0
58.00	201.0
60.00	1354.0
61.00	6343.0
62.00	6219.0
63.10	5487.0
64.10	629.0
65.00	1040.0
66.00	153.0
67.10	353.0
68.00	12906.0
69.00	13526.0
70.00	1143.0
72.10	756.0
73.00	5995.0
74.00	22024.0
75.00	65912.0
76.10	5644.0
77.00	900.0
78.00	540.0
78.90	4854.0
80.00	1512.0
80.90	4742.0
82.00	1286.0
83.00	152.0
86.00	234.0
87.00	6019.0
88.00	5749.0
90.90	601.0
92.00	3997.0
93.00	6447.0
94.00	16224.0
95.00	135360.0
96.00	8887.0
97.00	315.0
103.90	718.0
104.80	178.0
105.90	678.0
106.90	174.0
110.90	184.0
112.00	131.0
112.90	163.0
114.80	177.0
115.90	555.0
116.90	976.0
117.90	622.0
118.90	778.0
126.00	107.0
127.90	512.0
128.90	353.0
129.90	584.0
130.80	269.0
134.90	254.0
136.90	389.0
140.10	107.0
140.90	1781.0
141.90	266.0
142.90	1925.0
144.00	145.0
145.00	573.0
145.90	285.0
147.10	113.0
147.90	232.0
150.00	146.0
153.10	167.0
153.90	126.0
154.90	327.0
156.80	228.0
159.00	150.0
160.90	173.0
171.00	196.0
172.00	1812.0
173.00	1560.0
174.00	120864.0
175.00	9653.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

176.00	115008.0
177.00	7424.0
177.90	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	969.0
37.10	5888.0
38.00	5022.0
39.10	2328.0
39.90	245.0
44.00	889.0
45.00	955.0
46.00	259.0
47.00	1529.0
47.90	710.0
49.10	4970.0
50.10	22224.0
51.10	6505.0
52.00	244.0
53.10	193.0
54.90	288.0
56.00	1905.0
57.00	3130.0
58.00	239.0
60.00	1292.0
61.00	5996.0
62.00	5894.0
63.10	4961.0
64.10	559.0
65.00	929.0
66.00	142.0
67.10	323.0
68.00	12261.0
69.00	12607.0
70.00	1044.0
72.00	657.0
73.00	5888.0
74.00	21216.0
75.00	61760.0
76.10	5343.0
77.00	896.0
78.00	470.0
79.00	4736.0
79.90	1432.0
80.90	4581.0
81.90	1181.0
83.10	166.0
86.00	186.0
87.00	5665.0
87.90	5291.0
90.90	569.0
92.00	3914.0
93.00	5852.0
94.00	15174.0
95.00	128704.0
96.00	8313.0
96.90	282.0
103.90	712.0
104.80	144.0
105.10	147.0
105.90	622.0
106.90	160.0
110.90	172.0
111.80	113.0
112.90	156.0
114.90	171.0
115.90	566.0
116.90	979.0
117.80	593.0
118.90	711.0
128.00	488.0
128.90	361.0
129.90	583.0
130.80	279.0
134.80	236.0
136.90	365.0
140.00	106.0
140.90	1665.0
141.90	277.0
142.90	1775.0
145.00	536.0
146.00	211.0
147.90	247.0
149.90	112.0
153.00	178.0
153.90	137.0
154.90	287.0
156.90	251.0
158.90	149.0
160.80	176.0
170.90	209.0
172.00	1724.0
173.00	1551.0
174.00	118528.0
175.00	9092.0
176.00	113136.0
177.00	7021.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

178.00

215.0

Instrument :

MSVOA_V

ClientSampleId :

BFB227