

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
 Data File : VV032839.D
 Acq On : 03 Nov 2023 09:50
 Operator : SY/MD
 Sample : VV1104WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK210

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

Signal : TIC: VV032839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rBV	203041	213016	14.94%	1.908%
2	1.532	147	153	162	rVB	176535	197870	13.88%	1.772%
3	2.063	309	318	335	rVB	344335	500097	35.07%	4.479%
4	2.391	416	420	423	rBV5	1621	1371	0.10%	0.012%
5	2.506	451	456	459	rBV6	1875	1734	0.12%	0.016%
6	2.523	459	461	463	rBV3	2105	1269	0.09%	0.011%
7	2.613	488	489	493	rBV3	1183	881	0.06%	0.008%
8	2.670	504	507	511	rBV6	1570	1070	0.08%	0.010%
9	3.053	624	626	628	rBV3	1145	629	0.04%	0.006%
10	3.153	653	657	659	rBV4	1228	527	0.04%	0.005%
11	3.178	659	665	666	rBV5	1970	1683	0.12%	0.015%
12	3.195	668	670	671	rBV2	1234	456	0.03%	0.004%
13	3.220	676	678	681	rBV4	985	395	0.03%	0.004%
14	3.256	686	689	690	rBV3	872	462	0.03%	0.004%
15	3.359	715	721	723	rBV7	1569	1383	0.10%	0.012%
16	3.371	723	725	727	rBV3	1545	784	0.05%	0.007%
17	3.416	736	739	740	rBV3	1012	448	0.03%	0.004%
18	3.426	740	742	743	rBV2	765	348	0.02%	0.003%
19	3.449	747	749	750	rBV2	1439	384	0.03%	0.003%
20	3.516	768	770	772	rVV3	1214	472	0.03%	0.004%
21	3.532	772	775	778	rVB5	1199	814	0.06%	0.007%
22	3.574	785	788	790	rBV4	1631	974	0.07%	0.009%
23	3.596	793	795	799	rVV4	1090	693	0.05%	0.006%
24	3.638	806	808	809	rBV2	1077	569	0.04%	0.005%
25	3.690	822	824	826	rBV3	2304	1359	0.10%	0.012%
26	3.738	833	839	841	rBV6	1356	1151	0.08%	0.010%
27	3.786	845	854	882	rBV	85946	247178	17.33%	2.214%
28	4.092	947	949	950	rBV2	1906	919	0.06%	0.008%
29	4.252	985	999	1018	rBV	227996	577871	40.53%	5.176%
30	4.751	1153	1154	1155	rBV2	1466	497	0.03%	0.004%
31	4.776	1160	1162	1166	rVV3	2003	1311	0.09%	0.012%
32	4.825	1175	1177	1179	rBV3	1066	473	0.03%	0.004%
33	4.957	1197	1218	1236	rBV3	531822	1425927	100.00%	12.772%
34	5.304	1323	1326	1328	rBV4	2103	1273	0.09%	0.011%
35	5.535	1386	1398	1434	rBV	407060	913831	64.09%	8.185%
36	5.989	1528	1539	1573	rBV	314302	692161	48.54%	6.200%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
 Data File : VV032839.D
 Acq On : 03 Nov 2023 09:50
 Operator : SY/MD
 Sample : VV1104WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK210

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.500	1694	1698	1702	rBV7	2070	1649	0.12%	0.015%
38	6.532	1707	1708	1709	rBV	1096	278	0.02%	0.002%
39	6.561	1714	1717	1718	rBV3	1817	1023	0.07%	0.009%
40	6.657	1742	1747	1748	rBV5	1726	1357	0.10%	0.012%
41	6.915	1814	1827	1849	rBV	166105	332423	23.31%	2.977%
42	7.146	1897	1899	1900	rBV2	1548	564	0.04%	0.005%
43	7.246	1919	1930	1962	rBV	623727	1162977	81.56%	10.417%
44	7.554	2018	2026	2047	rBV	115697	210331	14.75%	1.884%
45	7.950	2147	2149	2153	rBV4	1551	913	0.06%	0.008%
46	7.995	2161	2163	2164	rBV2	1846	816	0.06%	0.007%
47	8.027	2164	2173	2213	rVV	280223	588390	41.26%	5.270%
48	8.365	2268	2278	2280	rBV9	4314	6331	0.44%	0.057%
49	8.786	2398	2409	2432	rBV	666859	1121883	78.68%	10.048%
50	9.194	2531	2536	2540	rBV8	1436	2031	0.14%	0.018%
51	9.281	2560	2563	2566	rBV4	1411	1214	0.09%	0.011%
52	9.345	2581	2583	2587	rVB5	1107	472	0.03%	0.004%
53	9.365	2587	2589	2592	rBV3	1731	1133	0.08%	0.010%
54	9.413	2601	2604	2605	rBV3	1532	907	0.06%	0.008%
55	9.734	2702	2704	2707	rVB4	2202	1305	0.09%	0.012%
56	9.754	2707	2710	2711	rBV3	1717	888	0.06%	0.008%
57	9.821	2726	2731	2733	rBV5	2012	1417	0.10%	0.013%
58	9.915	2758	2760	2761	rBV2	1406	569	0.04%	0.005%
59	9.943	2767	2769	2772	rBV4	1848	1036	0.07%	0.009%
60	10.001	2785	2787	2791	rBV4	1818	916	0.06%	0.008%
61	10.152	2823	2834	2851	rBV	447749	719400	50.45%	6.444%
62	10.522	2947	2949	2951	rBV3	1070	548	0.04%	0.005%
63	10.558	2958	2960	2961	rBV2	1040	399	0.03%	0.004%
64	10.599	2968	2973	2980	rBV10	2990	3498	0.25%	0.031%
65	10.641	2983	2986	2987	rBV3	1325	868	0.06%	0.008%
66	10.847	3048	3050	3052	rBV3	1903	1015	0.07%	0.009%
67	10.895	3063	3065	3068	rVB4	1485	718	0.05%	0.006%
68	10.969	3085	3088	3089	rBV3	1236	701	0.05%	0.006%
69	10.988	3091	3094	3095	rBV3	1565	921	0.06%	0.008%
70	11.027	3104	3106	3108	rVB3	1528	691	0.05%	0.006%
71	11.046	3108	3112	3117	rBV7	1380	1430	0.10%	0.013%
72	11.085	3121	3124	3126	rBV5	1949	1320	0.09%	0.012%
73	11.101	3126	3129	3131	rVB4	1530	731	0.05%	0.007%
74	11.188	3145	3156	3178	rBV	660512	1027127	72.03%	9.200%
75	11.561	3261	3272	3296	rBV	691968	1108463	77.74%	9.928%
76	11.918	3381	3383	3387	rBV5	1693	1566	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
 Data File : VV032839.D
 Acq On : 03 Nov 2023 09:50
 Operator : SY/MD
 Sample : VV1104WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK210

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.046	3420	3423	3424	rBV3	1093	682	0.05%	0.006%
78	12.175	3461	3463	3466	rBV4	1310	753	0.05%	0.007%
79	12.223	3477	3478	3480	rBV2	864	427	0.03%	0.004%
80	12.474	3553	3556	3558	rBV3	1615	606	0.04%	0.005%
81	12.487	3558	3560	3565	rVV5	997	896	0.06%	0.008%
82	12.586	3585	3591	3594	rBV7	4212	5028	0.35%	0.045%
83	12.644	3608	3609	3610	rBV	865	280	0.02%	0.003%
84	12.824	3663	3665	3667	rBV3	1543	763	0.05%	0.007%
85	13.037	3729	3731	3733	rBV3	1170	601	0.04%	0.005%
86	13.111	3752	3754	3756	rBV2	1625	686	0.05%	0.006%
87	13.207	3775	3784	3794	rBV2	7964	14433	1.01%	0.129%
88	13.348	3821	3828	3830	rBV6	1456	1481	0.10%	0.013%
89	13.377	3830	3837	3840	rBV10	1746	2140	0.15%	0.019%
90	13.445	3852	3858	3868	rVB2	13563	20812	1.46%	0.186%
91	13.574	3893	3898	3900	rBV4	1521	1453	0.10%	0.013%
92	13.738	3945	3949	3950	rBV4	1973	1374	0.10%	0.012%
93	13.786	3962	3964	3966	rBV2	1515	742	0.05%	0.007%
94	13.882	3992	3994	3996	rBV3	1373	598	0.04%	0.005%
95	14.020	4034	4037	4041	rBV6	1415	1274	0.09%	0.011%
96	14.236	4101	4104	4108	rBV5	1611	1047	0.07%	0.009%
97	14.339	4130	4136	4140	rBV9	2475	3026	0.21%	0.027%
98	14.381	4147	4149	4151	rBV3	2248	974	0.07%	0.009%
99	14.458	4171	4173	4175	rBV3	1152	502	0.04%	0.004%
100	15.239	4412	4416	4419	rBV6	2476	1652	0.12%	0.015%




Sum of corrected areas: 11164729

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032839.D
Acq On : 03 Nov 2023 09:50
Operator : SY/MD
Sample : VV1104WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

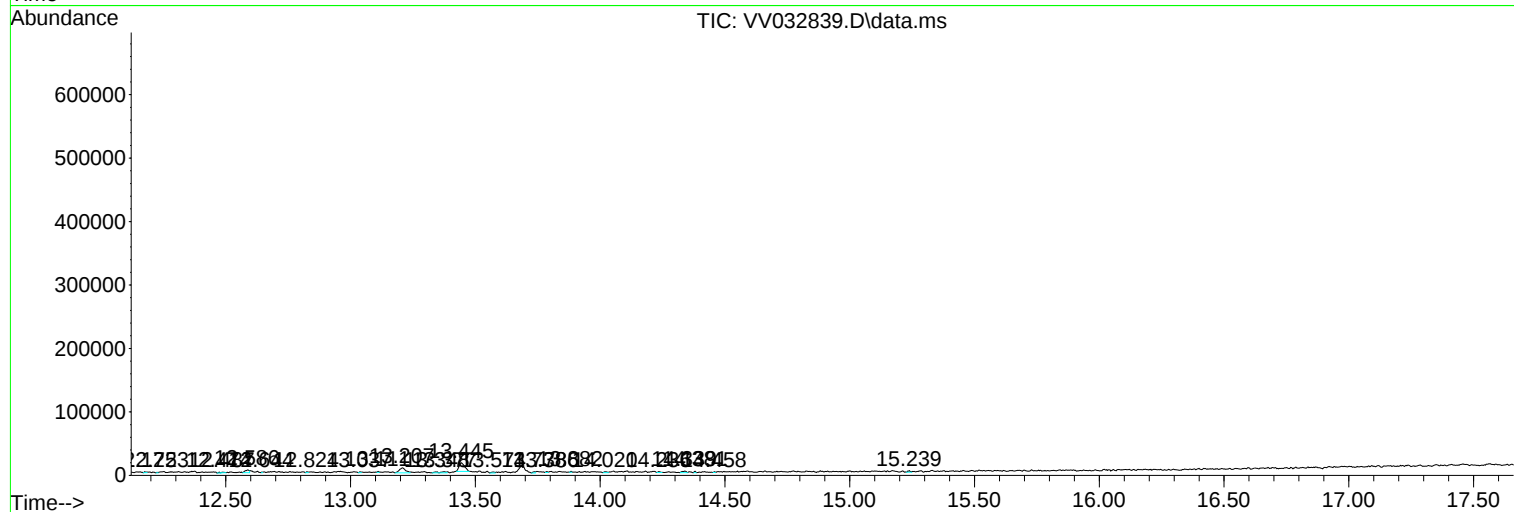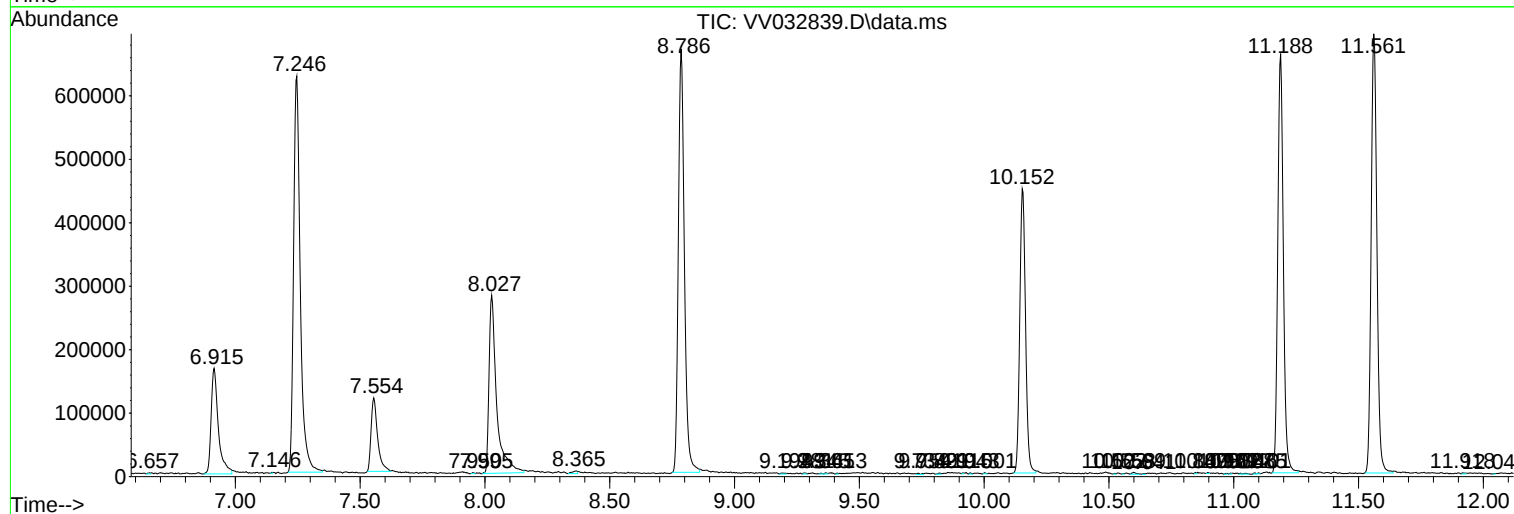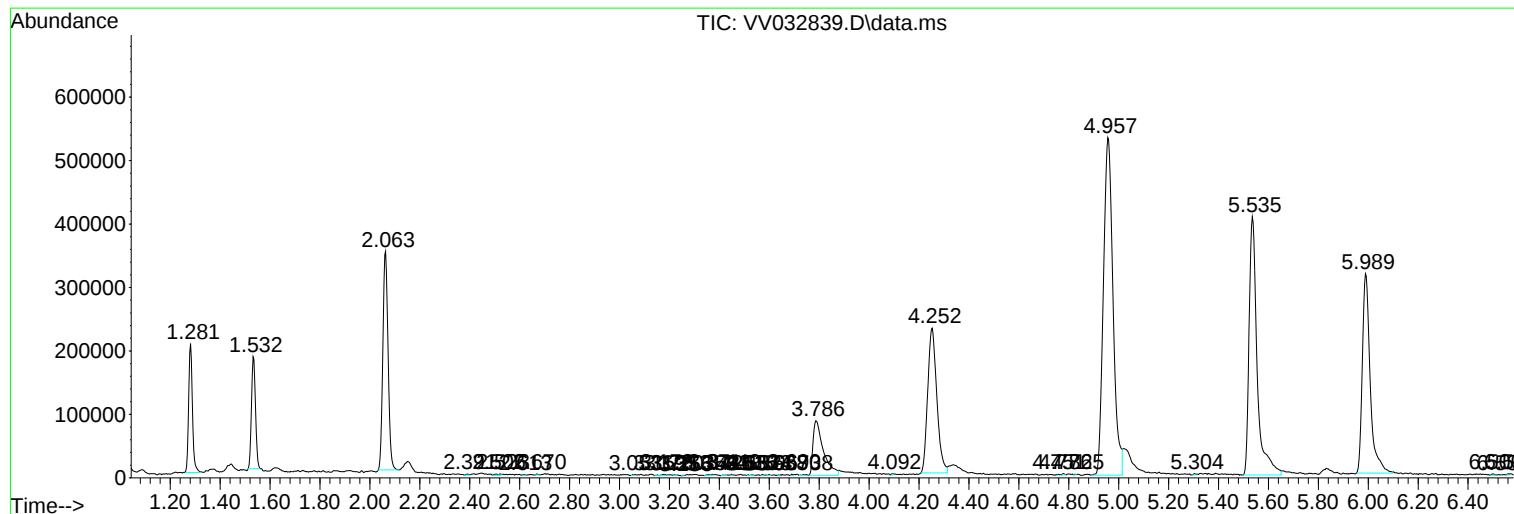

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032839.D
Acq On : 03 Nov 2023 09:50
Operator : SY/MD
Sample : VV1104WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032839.D
Acq On : 03 Nov 2023 09:50
Operator : SY/MD
Sample : VV1104WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------