

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
 Data File : VV032842.D
 Acq On : 03 Nov 2023 11:00
 Operator : SY/MD
 Sample : 05226-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	194613	203081	14.61%	1.827%
2	1.535	147	154	166	rVB	177536	204744	14.73%	1.842%
3	2.063	310	318	328	rBV	334011	473003	34.04%	4.255%
4	2.664	502	505	508	rBV5	1904	1453	0.10%	0.013%
5	2.687	508	512	513	rBV4	1437	936	0.07%	0.008%
6	2.757	530	534	535	rBV2	1509	889	0.06%	0.008%
7	2.802	545	548	550	rBV4	1473	966	0.07%	0.009%
8	2.851	559	563	567	rVB7	1897	1619	0.12%	0.015%
9	2.870	567	569	572	rBV4	1812	1088	0.08%	0.010%
10	2.973	598	601	603	rBV4	1689	1146	0.08%	0.010%
11	3.021	612	616	620	rBV6	2151	1929	0.14%	0.017%
12	3.066	627	630	633	rVB4	1373	815	0.06%	0.007%
13	3.082	633	635	637	rBV3	1744	819	0.06%	0.007%
14	3.111	641	644	646	rBV3	1209	886	0.06%	0.008%
15	3.214	672	676	680	rVB7	1821	1680	0.12%	0.015%
16	3.269	690	693	698	rBV7	1540	1438	0.10%	0.013%
17	3.294	698	701	705	rVB6	1087	890	0.06%	0.008%
18	3.317	706	708	713	rVB5	1895	1024	0.07%	0.009%
19	3.436	744	745	749	rVB4	1345	660	0.05%	0.006%
20	3.461	749	753	756	rVB6	1423	851	0.06%	0.008%
21	3.481	756	759	761	rBV3	1446	861	0.06%	0.008%
22	3.603	793	797	799	rBV5	1187	737	0.05%	0.007%
23	3.641	806	809	812	rVB5	1444	823	0.06%	0.007%
24	3.654	812	813	816	rVB3	1331	547	0.04%	0.005%
25	3.725	829	835	839	rVB9	1806	1806	0.13%	0.016%
26	3.789	841	855	884	rBV2	101857	313883	22.59%	2.823%
27	4.252	985	999	1020	rBV	222388	578685	41.64%	5.205%
28	4.532	1084	1086	1088	rBV3	1442	796	0.06%	0.007%
29	4.622	1113	1114	1118	rBV3	1376	1092	0.08%	0.010%
30	4.960	1202	1219	1237	rBV2	524048	1389686	100.00%	12.501%
31	5.535	1387	1398	1414	rBV	408147	833880	60.00%	7.501%
32	5.928	1519	1520	1523	rBV3	1932	1225	0.09%	0.011%
33	5.992	1528	1540	1570	rVV	308266	686827	49.42%	6.178%
34	6.320	1641	1642	1647	rBV5	1670	1308	0.09%	0.012%
35	6.403	1663	1668	1672	rBV8	2348	2876	0.21%	0.026%
36	6.915	1814	1827	1850	rBV	161244	326764	23.51%	2.939%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
 Data File : VV032842.D
 Acq On : 03 Nov 2023 11:00
 Operator : SY/MD
 Sample : 05226-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	7.246	1919	1930	1963	rBV	615110	1161038	83.55%	10.444%
38	7.555	2017	2026	2050	rBV2	117431	221087	15.91%	1.989%
39	8.027	2164	2173	2211	rBV	275589	585363	42.12%	5.265%
40	8.461	2305	2308	2311	rBV5	1882	996	0.07%	0.009%
41	8.542	2329	2333	2335	rBV5	2485	1711	0.12%	0.015%
42	8.567	2335	2341	2342	rVV6	1599	1311	0.09%	0.012%
43	8.786	2398	2409	2428	rBV	678925	1152508	82.93%	10.367%
44	9.323	2573	2576	2577	rBV3	1057	566	0.04%	0.005%
45	9.419	2603	2606	2607	rBV3	1565	846	0.06%	0.008%
46	9.484	2624	2626	2631	rBV6	1889	1394	0.10%	0.013%
47	9.535	2639	2642	2646	rBV5	1872	1441	0.10%	0.013%
48	9.686	2686	2689	2693	rBV5	1152	898	0.06%	0.008%
49	9.706	2693	2695	2699	rVB4	1803	779	0.06%	0.007%
50	9.934	2764	2766	2770	rVB5	1452	639	0.05%	0.006%
51	10.152	2824	2834	2852	rVV	439583	700767	50.43%	6.304%
52	10.329	2879	2889	2898	rVB2	14204	27061	1.95%	0.243%
53	10.426	2918	2919	2922	rBV3	1231	601	0.04%	0.005%
54	10.442	2922	2924	2926	rBV3	1503	823	0.06%	0.007%
55	10.480	2933	2936	2941	rBV5	1748	1424	0.10%	0.013%
56	10.548	2954	2957	2961	rBV5	1318	1038	0.07%	0.009%
57	10.567	2961	2963	2967	rVV5	1183	830	0.06%	0.007%
58	10.590	2967	2970	2974	rBV5	1464	1272	0.09%	0.011%
59	10.667	2988	2994	2997	rBV7	2661	2925	0.21%	0.026%
60	10.767	3022	3025	3027	rBV4	1653	1176	0.08%	0.011%
61	10.924	3070	3074	3076	rBV5	1716	1022	0.07%	0.009%
62	10.966	3083	3087	3089	rBV4	1351	1059	0.08%	0.010%
63	11.024	3100	3105	3107	rBV5	2295	2046	0.15%	0.018%
64	11.053	3112	3114	3117	rVB4	2057	1119	0.08%	0.010%
65	11.072	3117	3120	3121	rBV2	1707	760	0.05%	0.007%
66	11.133	3137	3139	3142	rBV3	1765	866	0.06%	0.008%
67	11.188	3146	3156	3178	rVV	669956	1041263	74.93%	9.366%
68	11.461	3237	3241	3244	rBV6	2550	1743	0.13%	0.016%
69	11.561	3260	3272	3292	rBV	700377	1119177	80.53%	10.067%
70	11.738	3324	3327	3330	rBV5	1951	1365	0.10%	0.012%
71	11.914	3379	3382	3385	rBV4	2302	1463	0.11%	0.013%
72	12.011	3409	3412	3413	rBV3	1436	670	0.05%	0.006%
73	12.046	3420	3423	3427	rVB6	2059	1545	0.11%	0.014%
74	12.066	3427	3429	3430	rBV2	2114	850	0.06%	0.008%
75	12.178	3458	3464	3466	rBV6	2605	2625	0.19%	0.024%
76	12.242	3482	3484	3489	rVB5	2442	1665	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
 Data File : VV032842.D
 Acq On : 03 Nov 2023 11:00
 Operator : SY/MD
 Sample : 05226-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.268	3489	3492	3493	rBV3	1617	944	0.07%	0.008%
78	12.432	3542	3543	3549	rVB6	1983	1435	0.10%	0.013%
79	12.480	3556	3558	3560	rBV3	1038	649	0.05%	0.006%
80	12.532	3572	3574	3578	rBV5	1601	1264	0.09%	0.011%
81	12.654	3610	3612	3616	rVB5	1267	634	0.05%	0.006%
82	12.709	3626	3629	3631	rBV4	1691	785	0.06%	0.007%
83	13.062	3737	3739	3740	rBV2	1579	804	0.06%	0.007%
84	13.104	3750	3752	3755	rBV4	1732	792	0.06%	0.007%
85	13.185	3773	3777	3781	rBV6	2885	2605	0.19%	0.023%
86	13.210	3781	3785	3788	rBV5	2436	2332	0.17%	0.021%
87	13.313	3813	3817	3822	rVB7	1822	1898	0.14%	0.017%
88	13.342	3822	3826	3828	rBV5	1844	1176	0.08%	0.011%
89	13.365	3828	3833	3836	rVB5	1413	1108	0.08%	0.010%
90	13.393	3840	3842	3844	rBV3	920	579	0.04%	0.005%
91	13.426	3850	3852	3855	rBV4	1755	1246	0.09%	0.011%
92	13.551	3887	3891	3892	rBV4	1922	1354	0.10%	0.012%
93	13.615	3909	3911	3915	rBV5	1690	1014	0.07%	0.009%
94	13.770	3957	3959	3963	rBV5	1903	1491	0.11%	0.013%
95	13.863	3986	3988	3990	rBV3	1091	570	0.04%	0.005%
96	13.892	3995	3997	3999	rBV3	1841	725	0.05%	0.007%
97	14.326	4129	4132	4135	rBV5	1709	1432	0.10%	0.013%
98	14.355	4137	4141	4143	rBV4	1663	1229	0.09%	0.011%
99	14.551	4200	4202	4203	rBV2	1801	669	0.05%	0.006%
100	14.577	4207	4210	4211	rBV3	1633	858	0.06%	0.008%


Sum of corrected areas: 11117038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032842.D
Acq On : 03 Nov 2023 11:00
Operator : SY/MD
Sample : 05226-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

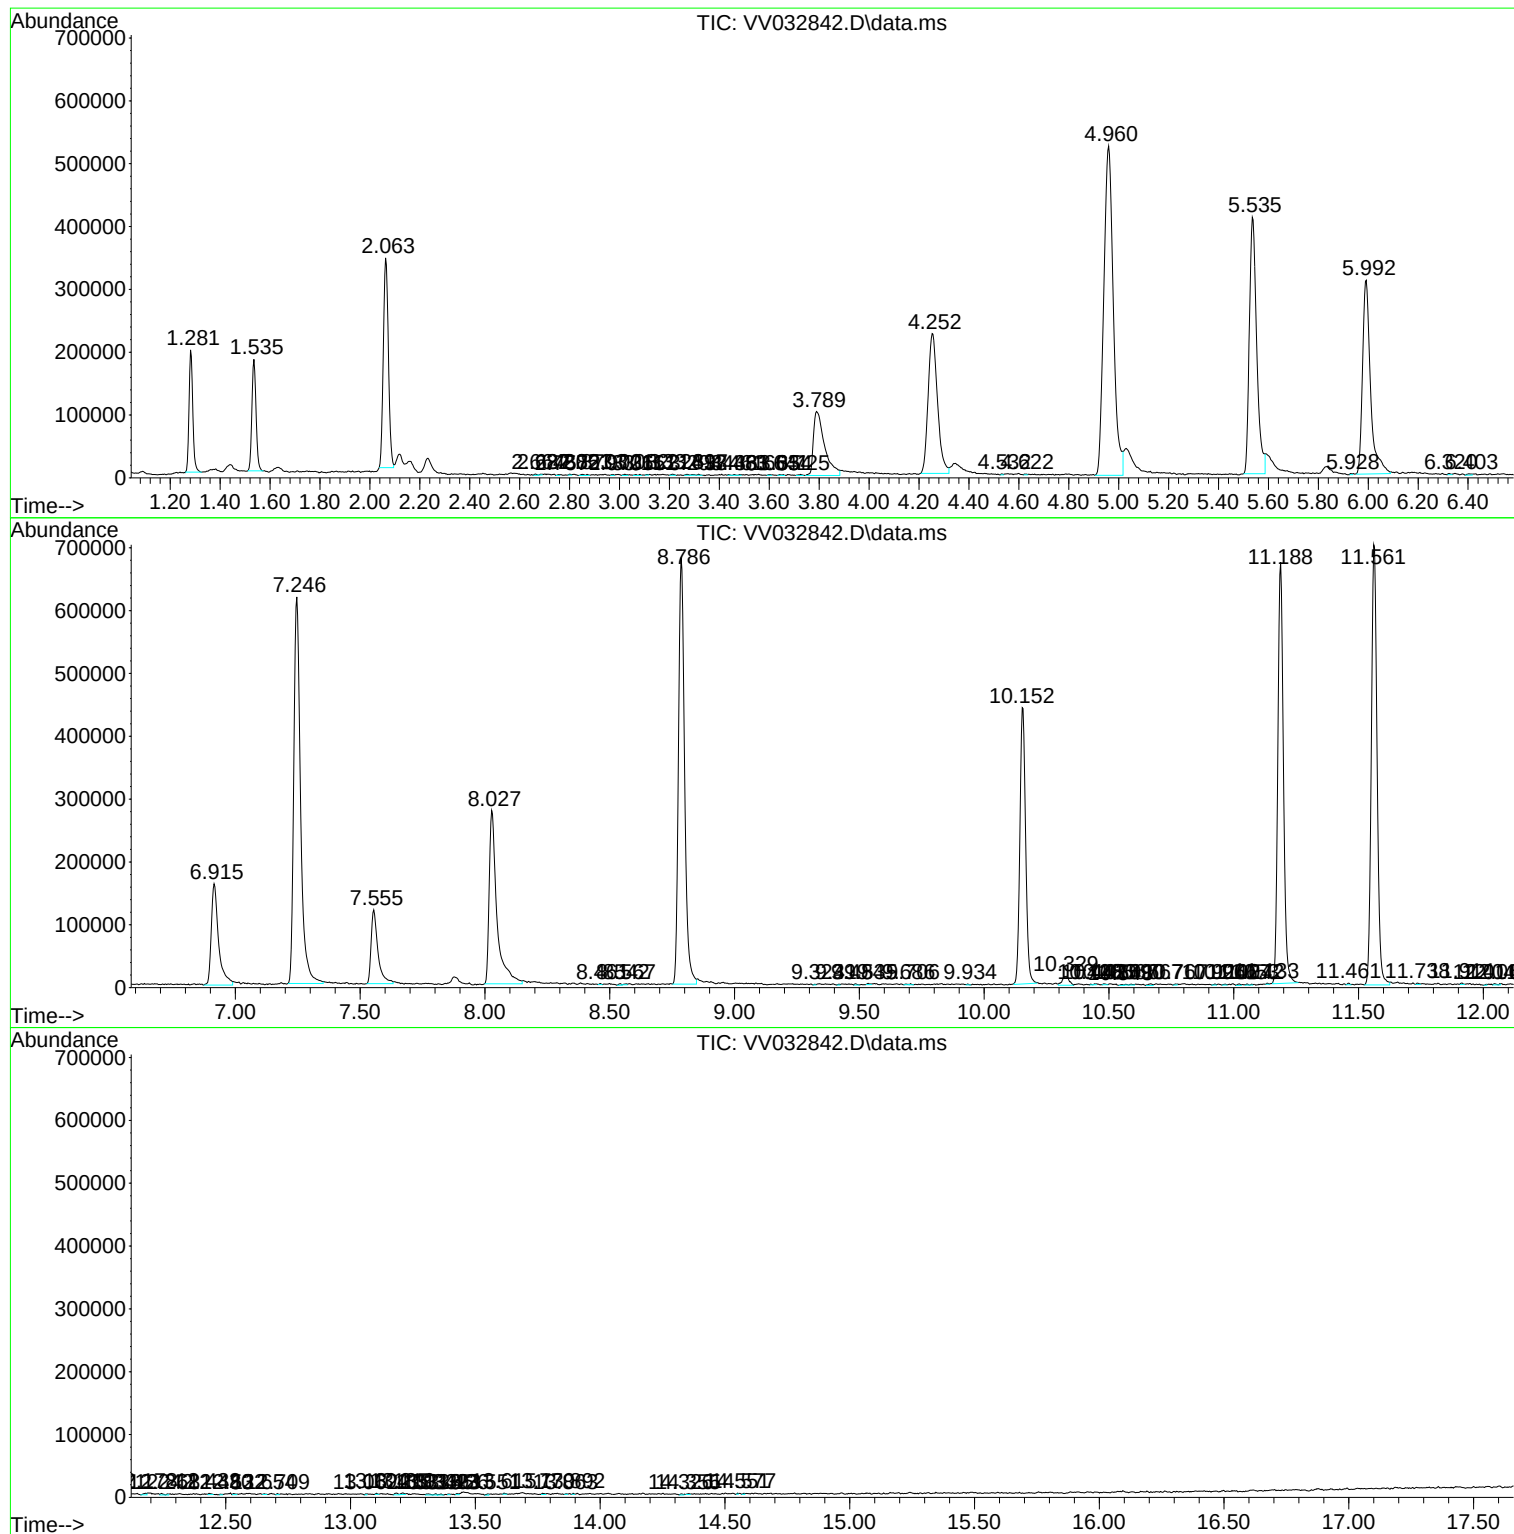

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032842.D
Acq On : 03 Nov 2023 11:00
Operator : SY/MD
Sample : 05226-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032842.D
Acq On : 03 Nov 2023 11:00
Operator : SY/MD
Sample : 05226-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------