

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
 Data File : VV032844.D
 Acq On : 03 Nov 2023 11:46
 Operator : SY/MD
 Sample : 05226-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

Signal : TIC: VV032844.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.147	31	33	34	rBV2	1706	807	0.06%	0.008%
2	1.282	69	75	84	rBV	195465	188631	13.92%	1.769%
3	1.532	147	153	166	rVB	172530	197446	14.57%	1.852%
4	2.063	309	318	332	rVB	318952	462911	34.15%	4.342%
5	2.323	394	399	401	rBV5	2329	2204	0.16%	0.021%
6	2.426	428	431	432	rBV3	1648	777	0.06%	0.007%
7	2.491	449	451	456	rVB6	2190	1584	0.12%	0.015%
8	2.516	456	459	463	rBV5	1446	1229	0.09%	0.012%
9	2.674	503	508	510	rBV6	1771	1758	0.13%	0.016%
10	2.745	527	530	531	rVB3	1609	787	0.06%	0.007%
11	2.806	547	549	553	rBV5	1046	816	0.06%	0.008%
12	2.912	580	582	585	rVB3	1830	914	0.07%	0.009%
13	2.954	592	595	596	rBV3	1593	748	0.06%	0.007%
14	3.118	644	646	651	rVB5	1558	1215	0.09%	0.011%
15	3.143	651	654	658	rBV6	1208	902	0.07%	0.008%
16	3.169	658	662	664	rBV4	913	793	0.06%	0.007%
17	3.220	675	678	682	rVB6	1257	833	0.06%	0.008%
18	3.249	682	687	691	rVB7	1879	1719	0.13%	0.016%
19	3.278	691	696	701	rBV9	1980	2413	0.18%	0.023%
20	3.320	705	709	712	rVB5	1404	890	0.07%	0.008%
21	3.339	712	715	718	rBV4	1453	1094	0.08%	0.010%
22	3.378	722	727	729	rBV5	1487	1053	0.08%	0.010%
23	3.536	774	776	778	rBV3	1655	822	0.06%	0.008%
24	3.574	785	788	790	rBV4	1405	708	0.05%	0.007%
25	3.626	801	804	808	rBV6	1308	1041	0.08%	0.010%
26	3.786	843	854	879	rBV	81893	225941	16.67%	2.119%
27	4.253	984	999	1017	rBV	215271	556957	41.09%	5.224%
28	4.597	1103	1106	1107	rBV2	1344	816	0.06%	0.008%
29	4.761	1155	1157	1159	rBV3	1813	1116	0.08%	0.010%
30	4.863	1186	1189	1191	rBV4	1656	1012	0.07%	0.009%
31	4.957	1201	1218	1236	rBV2	504267	1355436	100.00%	12.713%
32	5.535	1386	1398	1414	rBV	391825	819093	60.43%	7.683%
33	5.989	1528	1539	1570	rBV	296672	652581	48.15%	6.121%
34	6.523	1703	1705	1709	rBV5	1855	879	0.06%	0.008%
35	6.561	1715	1717	1719	rBV2	1329	673	0.05%	0.006%
36	6.629	1735	1738	1744	rVB8	2301	2060	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
 Data File : VV032844.D
 Acq On : 03 Nov 2023 11:46
 Operator : SY/MD
 Sample : 05226-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.654	1744	1746	1748	rBV2	1431	861	0.06%	0.008%
38	6.828	1797	1800	1805	rBV7	1582	1111	0.08%	0.010%
39	6.915	1817	1827	1850	rBV	152844	303196	22.37%	2.844%
40	7.153	1897	1901	1904	rBV5	1804	1603	0.12%	0.015%
41	7.246	1918	1930	1958	rBV	588368	1124679	82.98%	10.549%
42	7.555	2018	2026	2047	rBV	109609	205924	15.19%	1.931%
43	7.873	2121	2125	2126	rBV3	5843	4215	0.31%	0.040%
44	7.979	2155	2158	2161	rBV5	1863	1663	0.12%	0.016%
45	8.027	2164	2173	2207	rVV	269471	554811	40.93%	5.204%
46	8.619	2353	2357	2360	rBV5	2012	1722	0.13%	0.016%
47	8.786	2398	2409	2428	rBV	672696	1130868	83.43%	10.607%
48	9.352	2584	2585	2591	rVB5	1731	1165	0.09%	0.011%
49	9.436	2607	2611	2616	rVB7	2356	2394	0.18%	0.022%
50	9.548	2643	2646	2647	rBV3	1559	836	0.06%	0.008%
51	9.645	2673	2676	2679	rBV5	1934	1396	0.10%	0.013%
52	9.744	2703	2707	2711	rVB6	1328	870	0.06%	0.008%
53	9.805	2723	2726	2728	rBV4	943	643	0.05%	0.006%
54	9.995	2783	2785	2788	rVB4	1443	700	0.05%	0.007%
55	10.156	2822	2835	2852	rBV	424643	696267	51.37%	6.531%
56	10.329	2880	2889	2898	rBV6	8469	13693	1.01%	0.128%
57	10.490	2936	2939	2943	rVB5	1925	1263	0.09%	0.012%
58	10.535	2950	2953	2955	rBV4	2741	1630	0.12%	0.015%
59	10.783	3028	3030	3031	rBV2	1607	746	0.06%	0.007%
60	10.828	3042	3044	3047	rBV4	1617	875	0.06%	0.008%
61	10.860	3051	3054	3059	rVB5	2762	2485	0.18%	0.023%
62	10.883	3059	3061	3062	rBV2	1569	797	0.06%	0.007%
63	10.956	3082	3084	3086	rBV3	1491	726	0.05%	0.007%
64	11.188	3145	3156	3175	rBV	652022	1011776	74.65%	9.490%
65	11.448	3234	3237	3238	rBV3	1266	822	0.06%	0.008%
66	11.493	3246	3251	3253	rBV4	1949	1887	0.14%	0.018%
67	11.561	3261	3272	3292	rBV	681814	1061195	78.29%	9.953%
68	11.770	3333	3337	3340	rBV6	1728	1281	0.09%	0.012%
69	11.847	3358	3361	3366	rBV6	1355	1239	0.09%	0.012%
70	11.924	3382	3385	3387	rBV3	1662	1109	0.08%	0.010%
71	12.034	3415	3419	3420	rBV3	1789	1206	0.09%	0.011%
72	12.075	3429	3432	3434	rBV4	1639	943	0.07%	0.009%
73	12.117	3443	3445	3447	rVB2	1840	803	0.06%	0.008%
74	12.133	3447	3450	3451	rBV3	1688	980	0.07%	0.009%
75	12.378	3521	3526	3531	rBV7	2716	2546	0.19%	0.024%
76	12.439	3541	3545	3547	rBV5	1465	1217	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
 Data File : VV032844.D
 Acq On : 03 Nov 2023 11:46
 Operator : SY/MD
 Sample : 05226-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.503	3561	3565	3566	rBV4	1342	961	0.07%	0.009%
78	12.545	3576	3578	3581	rBV4	1576	852	0.06%	0.008%
79	12.574	3584	3587	3588	rBV2	1385	758	0.06%	0.007%
80	12.635	3602	3606	3608	rVB4	1730	1085	0.08%	0.010%
81	12.741	3636	3639	3643	rBV6	1071	1007	0.07%	0.009%
82	12.786	3651	3653	3658	rVB6	1866	1052	0.08%	0.010%
83	12.818	3661	3663	3666	rBV3	965	696	0.05%	0.007%
84	12.863	3675	3677	3683	rVB7	1282	1134	0.08%	0.011%
85	13.288	3805	3809	3813	rVV6	1509	1429	0.11%	0.013%
86	13.387	3838	3840	3844	rBV5	2196	1752	0.13%	0.016%
87	13.590	3902	3903	3906	rBV3	1499	796	0.06%	0.007%
88	13.628	3910	3915	3916	rBV5	2025	1826	0.13%	0.017%
89	13.667	3925	3927	3930	rBV3	1237	650	0.05%	0.006%
90	13.683	3930	3932	3933	rBV2	1894	709	0.05%	0.007%
91	13.738	3945	3949	3950	rBV4	2089	1423	0.10%	0.013%
92	13.902	3997	4000	4005	rBV6	1412	1275	0.09%	0.012%
93	13.966	4018	4020	4023	rBV5	2001	834	0.06%	0.008%
94	14.095	4057	4060	4061	rBV3	1862	895	0.07%	0.008%
95	14.130	4068	4071	4073	rBV3	1687	1331	0.10%	0.012%
96	14.159	4077	4080	4083	rVB5	2571	1620	0.12%	0.015%
97	14.178	4083	4086	4087	rBV3	2269	1238	0.09%	0.012%
98	14.310	4123	4127	4128	rBV4	1761	1064	0.08%	0.010%
99	15.050	4355	4357	4361	rBV5	2196	1257	0.09%	0.012%
100	15.339	4444	4447	4449	rBV4	2362	1207	0.09%	0.011%




Sum of corrected areas: 10661653

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032844.D
Acq On : 03 Nov 2023 11:46
Operator : SY/MD
Sample : 05226-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

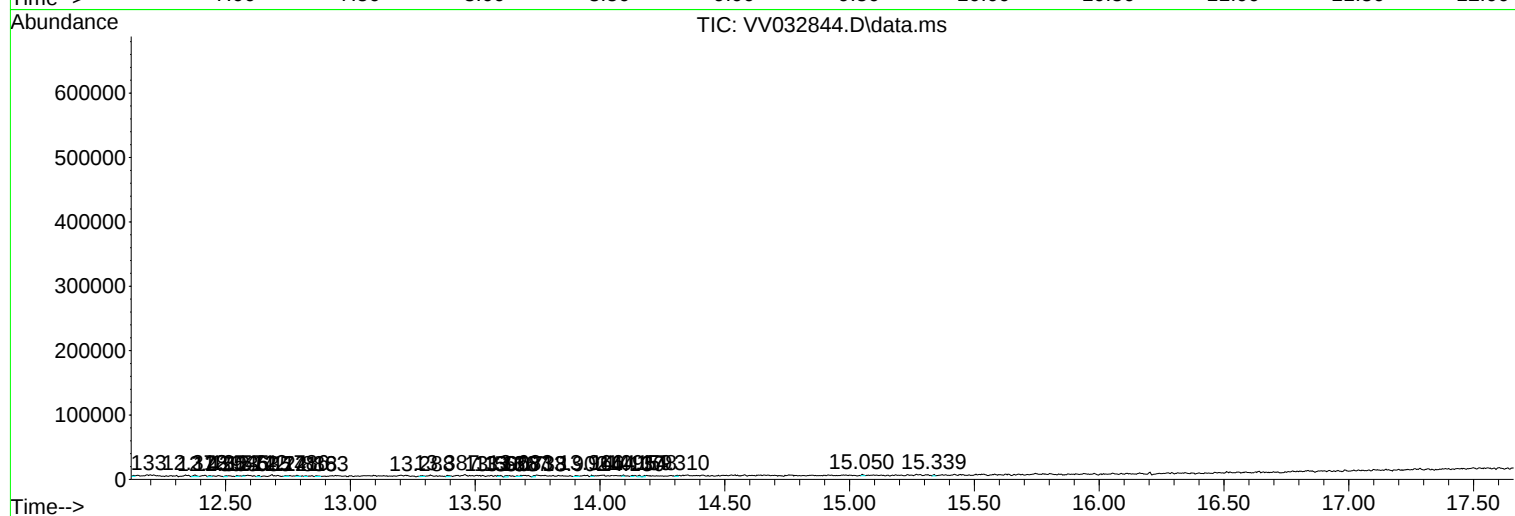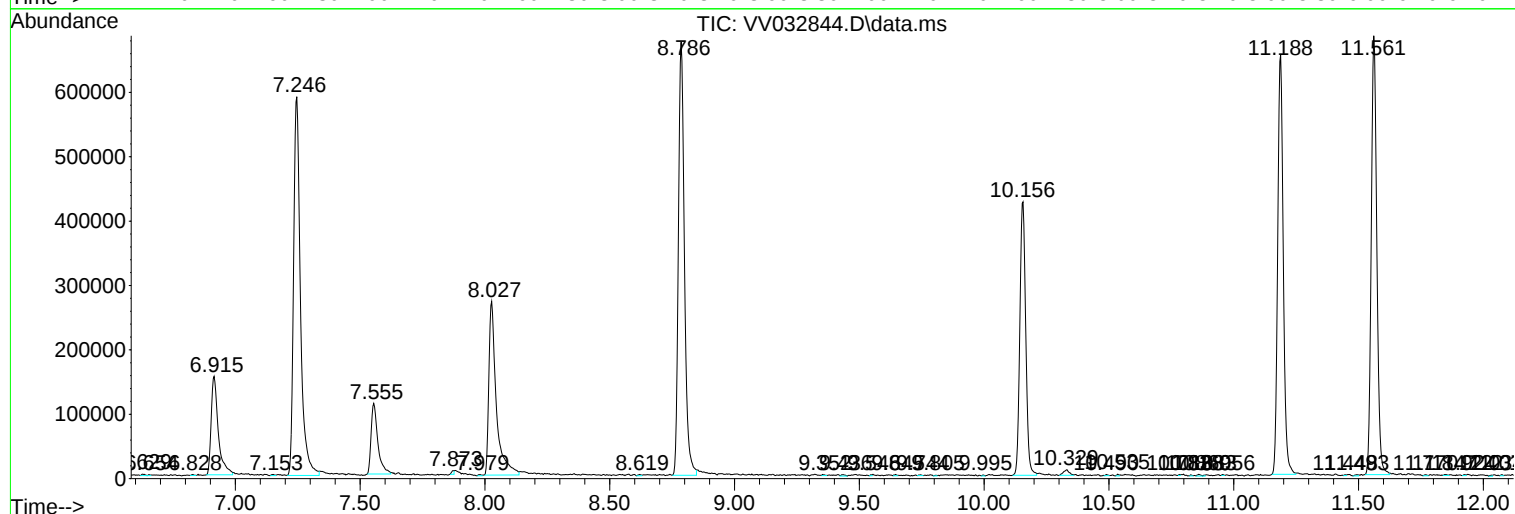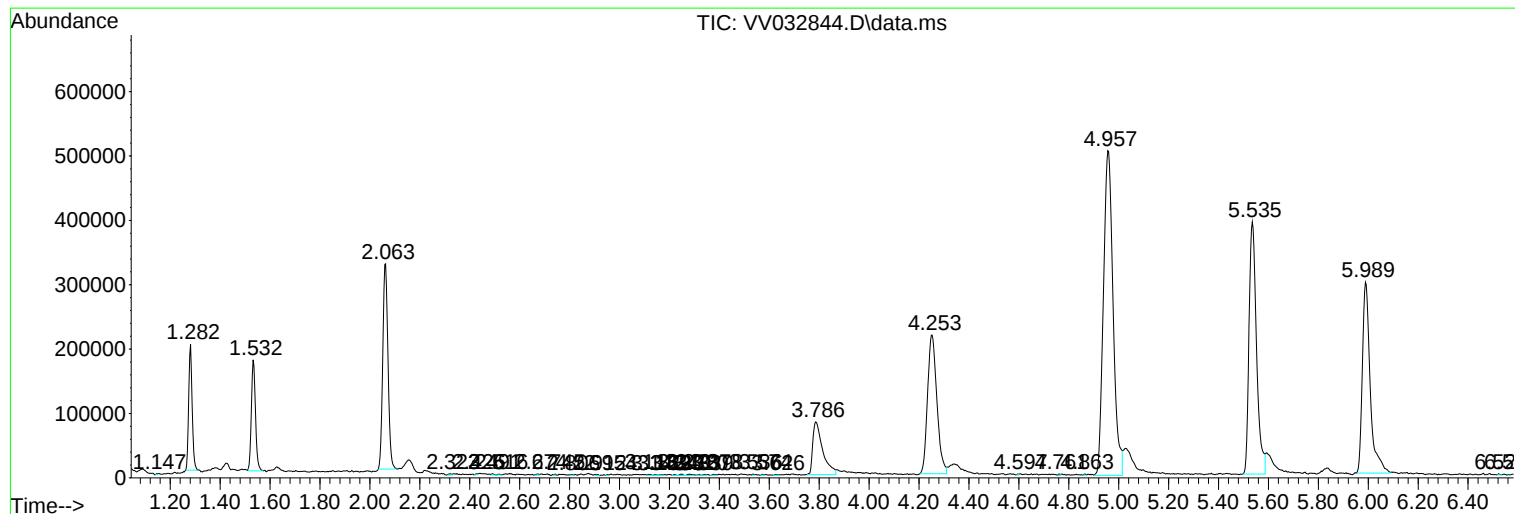

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032844.D
Acq On : 03 Nov 2023 11:46
Operator : SY/MD
Sample : 05226-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032844.D
Acq On : 03 Nov 2023 11:46
Operator : SY/MD
Sample : 05226-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc