


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110423\
Data File : VV032836.D
Acq On : 03 Nov 2023 08:07
Operator : SY/MD
Sample : BFB227
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB227

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Title : VOC Analysis
Last Update : Sat Nov 04 00:57:36 2023

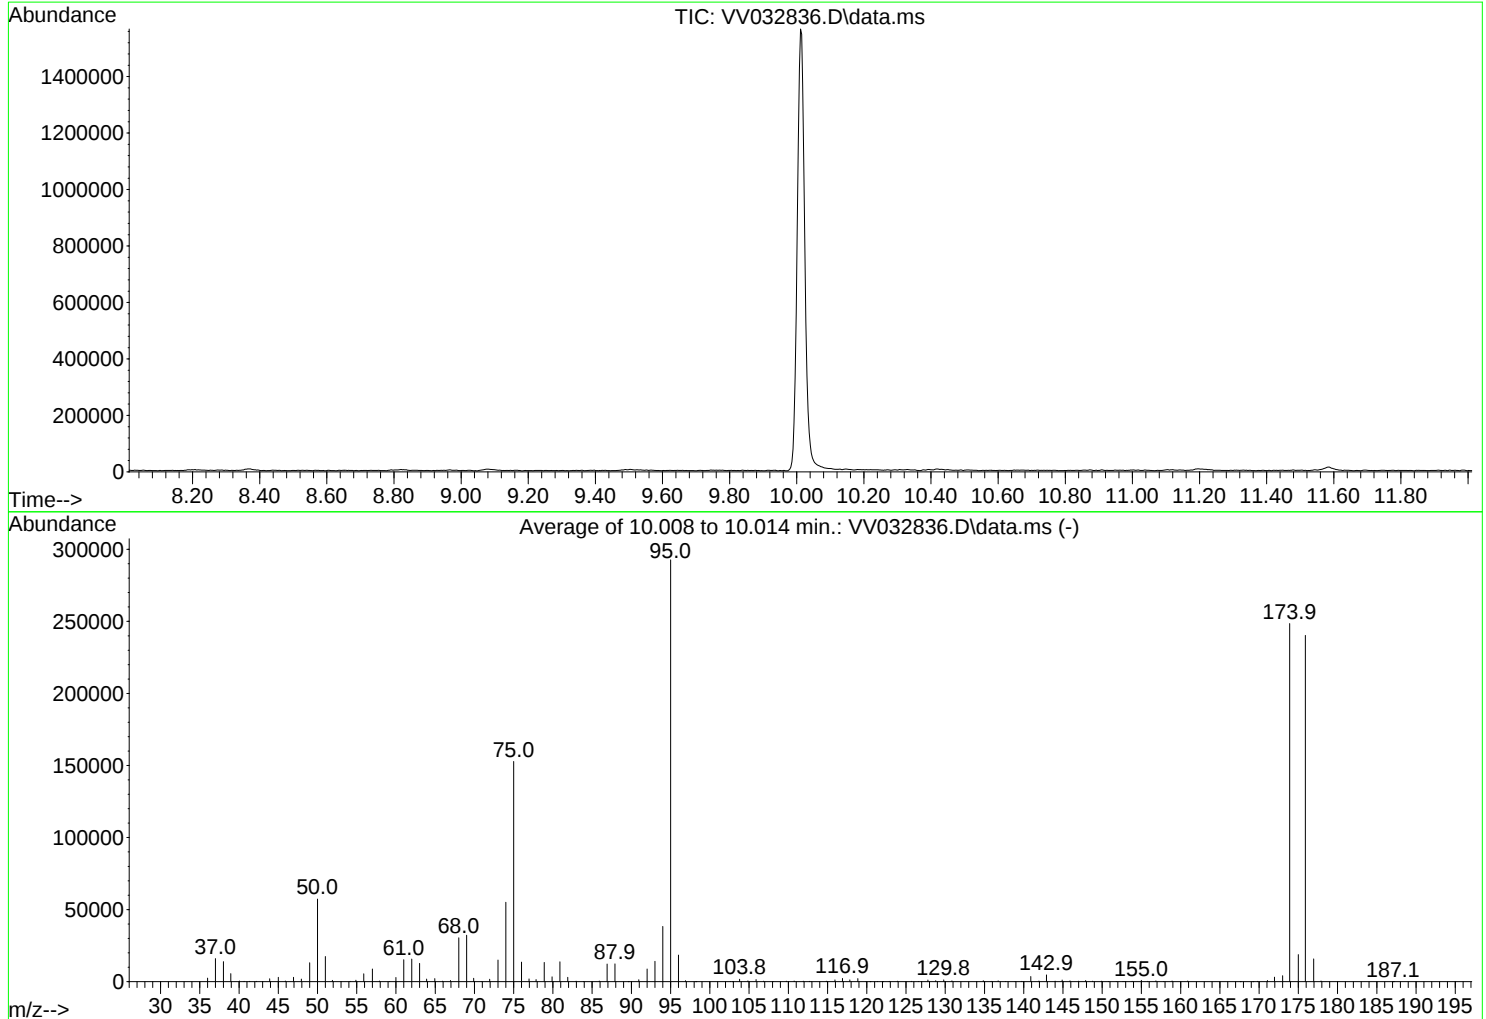

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	57325	PASS
75	95	30	80	52.2	152832	PASS
95	95	100	100	100.0	292715	PASS
96	95	5	9	6.3	18392	PASS
173	174	0.00	2	1.7	4133	PASS
174	95	50	120	84.9	248555	PASS
175	174	5	9	7.5	18736	PASS
176	174	95	105	96.7	240256	PASS
177	176	5	10	6.6	15747	PASS

m/z	Abundance
36.00	239.0
37.50	130.0
38.90	200.0
39.80	234.0
41.10	104.0
41.60	122.0
43.00	169.0
43.90	437.0
44.70	112.0
46.30	125.0
50.30	111.0
51.20	159.0
51.80	125.0
53.00	136.0
53.50	134.0
56.30	114.0
57.10	125.0
61.40	127.0
64.60	128.0
66.90	140.0
69.90	116.0
70.90	101.0
76.20	105.0
83.60	119.0
87.90	107.0
92.00	129.0
94.50	102.0
168.50	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	2721.0
37.00	15434.0
38.00	13150.0
39.00	5369.0
40.00	535.0
40.70	301.0
41.40	196.0
42.20	216.0
43.10	316.0
44.00	2296.0
45.00	2790.0
45.90	411.0
46.90	3074.0
48.00	1743.0
49.00	12735.0
50.00	55120.0
51.00	17072.0
52.00	1138.0
53.00	353.0
54.10	261.0
54.90	1006.0
55.90	5262.0
57.00	8781.0
57.90	379.0
60.00	2824.0
61.00	14869.0
62.00	15486.0
63.00	12460.0
63.90	1950.0
65.00	2194.0
65.90	344.0
67.00	1026.0
68.00	28632.0
69.00	31136.0
69.90	2361.0
70.90	177.0
72.00	1576.0
73.00	14328.0
74.00	52800.0
75.00	145088.0
76.00	13360.0
76.90	1835.0
77.90	1334.0
78.90	12632.0
79.90	3256.0
80.90	12903.0
81.90	3006.0
82.90	333.0
83.90	151.0
85.90	368.0
86.90	11354.0
87.90	11968.0
90.00	138.0
90.90	1287.0
92.00	8653.0
93.00	13573.0
94.00	35928.0
95.00	276736.0
96.00	17240.0
96.90	707.0
98.20	138.0
102.60	149.0
102.90	137.0
103.80	1523.0
104.80	574.0
105.90	1317.0
106.90	352.0
108.00	131.0
109.80	301.0
110.80	431.0
111.90	310.0
112.70	344.0
114.90	381.0
116.00	1060.0
116.90	2158.0
117.80	1112.0
118.80	2149.0
120.00	100.0
120.40	103.0
121.40	130.0
122.90	185.0
123.80	293.0
125.70	175.0
127.00	131.0
127.80	1194.0
128.80	643.0
129.80	1258.0
130.90	469.0
134.00	131.0
134.80	647.0
135.90	170.0
136.70	558.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

138.90	161.0
139.80	220.0
140.90	3296.0
142.00	405.0
142.90	4459.0
144.00	325.0
144.90	1314.0
145.90	604.0
147.00	288.0
147.90	644.0
148.80	253.0
150.00	332.0
152.60	199.0
153.00	202.0
153.80	184.0
155.00	783.0
155.80	206.0
156.80	627.0
157.80	127.0
158.90	378.0
161.00	354.0
167.60	117.0
169.80	127.0
171.00	772.0
172.00	2913.0
173.00	3727.0
173.90	229888.0
175.00	17664.0
175.90	220672.0
176.90	14924.0
177.90	401.0
187.10	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	2736.0
37.00	16632.0
38.00	14472.0
39.00	5958.0
40.00	445.0
40.70	269.0
41.30	226.0
42.20	223.0
43.00	310.0
43.90	2510.0
45.00	3138.0
45.90	431.0
46.90	3157.0
48.00	1846.0
49.00	13698.0
50.00	59240.0
51.00	18200.0
51.90	1007.0
53.10	291.0
54.20	304.0
54.90	1003.0
55.90	5569.0
57.00	9148.0
57.90	429.0
60.00	3068.0
61.00	15807.0
62.00	16193.0
63.00	13073.0
63.90	1845.0
65.00	2165.0
66.00	344.0
67.00	984.0
68.00	31544.0
69.00	33544.0
69.90	2558.0
70.80	197.0
72.00	1749.0
73.00	15527.0
74.00	57256.0
75.00	158016.0
76.00	14237.0
76.90	1904.0
77.90	1463.0
78.90	13808.0
79.90	3529.0
80.90	14287.0
81.90	3137.0
82.90	363.0
83.90	144.0
85.90	282.0
86.90	12508.0
87.90	12897.0
90.00	150.0
91.00	1308.0
92.00	9132.0
93.00	14513.0
94.00	39544.0
95.00	302720.0
96.00	19040.0
96.90	737.0
102.70	159.0
103.80	1790.0
104.80	535.0
105.90	1553.0
106.90	341.0
108.00	149.0
109.80	331.0
110.80	431.0
111.90	362.0
112.70	348.0
114.90	364.0
116.00	1220.0
116.90	2339.0
117.90	1226.0
118.90	2211.0
121.30	117.0
122.80	203.0
123.90	329.0
125.70	191.0
126.60	132.0
127.00	138.0
127.80	1190.0
128.80	693.0
129.80	1334.0
130.80	524.0
134.00	164.0
134.90	705.0
135.90	190.0
136.70	600.0
137.70	113.0
138.90	171.0
139.70	249.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

140.90	3602.0
142.00	428.0
142.90	4948.0
144.00	322.0
144.90	1189.0
145.90	634.0
147.00	321.0
147.90	788.0
148.80	325.0
149.90	371.0
150.80	119.0
151.80	137.0
152.70	220.0
153.80	169.0
155.00	912.0
155.80	211.0
156.90	569.0
157.90	149.0
158.90	495.0
160.90	401.0
169.80	217.0
171.10	765.0
171.90	3268.0
173.00	4226.0
173.90	257216.0
175.00	19520.0
175.90	248768.0
176.90	16408.0
177.90	470.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	2577.0
37.00	15957.0
38.00	14008.0
39.00	5899.0
40.10	389.0
40.60	236.0
41.30	218.0
42.20	231.0
42.90	277.0
43.90	2427.0
45.00	3057.0
45.90	472.0
47.00	2871.0
47.90	1917.0
49.00	12967.0
50.00	57616.0
51.00	17464.0
51.90	822.0
53.00	270.0
54.10	297.0
54.90	883.0
55.90	5401.0
57.00	8756.0
57.90	488.0
59.20	267.0
60.00	2899.0
61.00	15133.0
62.00	15457.0
63.00	12584.0
63.90	1630.0
64.90	1986.0
66.00	326.0
67.00	928.0
68.00	31144.0
69.00	31976.0
70.00	2407.0
70.80	236.0
71.90	1645.0
73.00	15169.0
74.00	55224.0
75.00	155392.0
76.00	13551.0
77.00	1788.0
77.80	1494.0
78.90	13643.0
79.90	3373.0
80.90	14135.0
81.90	2961.0
83.00	388.0
85.70	272.0
86.00	299.0
86.90	12673.0
87.90	12338.0
89.60	149.0
90.00	127.0
91.00	1293.0
92.00	9035.0
93.00	14140.0
94.00	39576.0
95.00	298688.0
96.00	18896.0
96.90	673.0
102.70	182.0
103.80	1847.0
104.90	495.0
105.90	1615.0
106.80	344.0
108.10	145.0
109.70	305.0
110.70	402.0
111.90	360.0
112.90	337.0
114.80	355.0
115.90	1279.0
116.90	2311.0
117.90	1293.0
118.90	2161.0
119.80	117.0
122.00	129.0
122.80	177.0
124.00	307.0
125.70	169.0
126.60	153.0
127.80	1130.0
128.80	674.0
129.80	1281.0
130.90	570.0
134.00	156.0
134.90	696.0
135.80	226.0
136.80	545.0
137.70	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

138.90	176.0
139.70	265.0
140.90	3638.0
141.90	408.0
142.90	4728.0
144.00	263.0
144.90	963.0
145.90	577.0
147.00	302.0
147.90	823.0
148.80	330.0
149.80	359.0
150.80	107.0
151.80	184.0
152.80	234.0
153.80	186.0
155.00	865.0
155.80	201.0
156.90	516.0
157.90	166.0
158.90	492.0
160.80	481.0
169.20	115.0
169.80	222.0
171.10	704.0
171.90	3221.0
173.00	4445.0
173.90	258560.0
175.00	19024.0
175.90	251328.0
177.00	15910.0
177.90	478.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227