
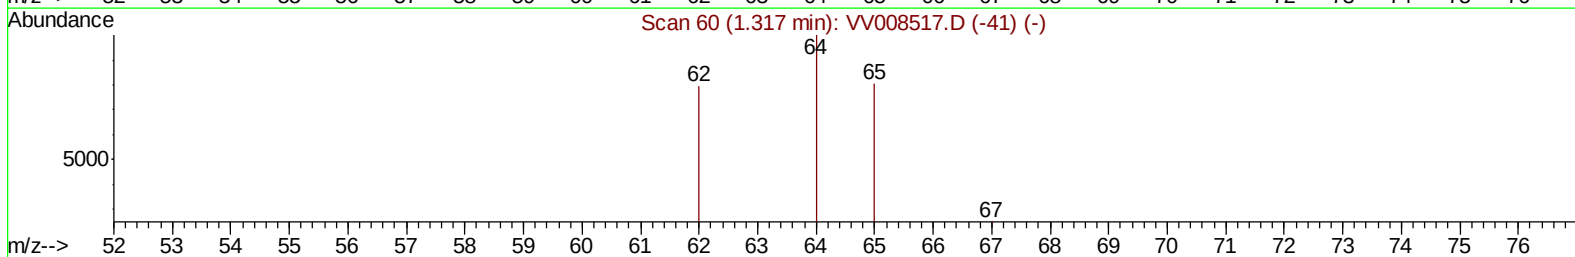
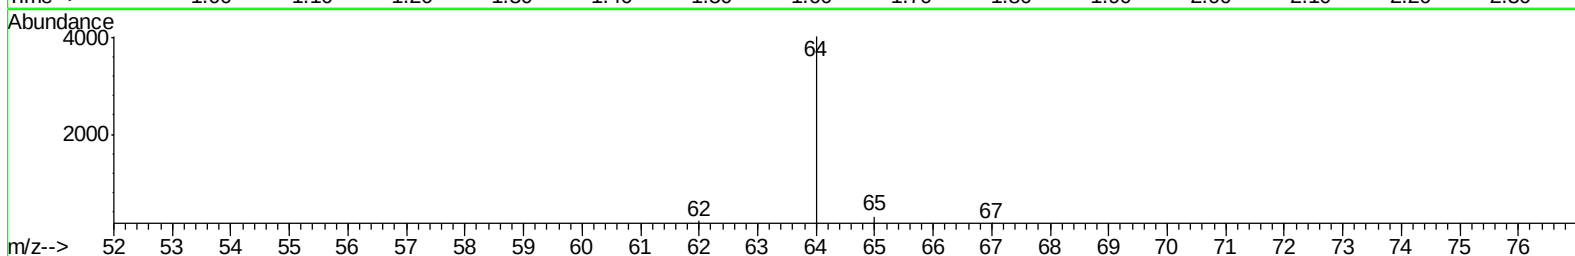


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008515.D
Acq On : 05 Nov 2018 12:28
Operator : SY/MD
Sample : VSTD0.0540
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 06 10:34:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:32:16 2018
Response via : Initial Calibration

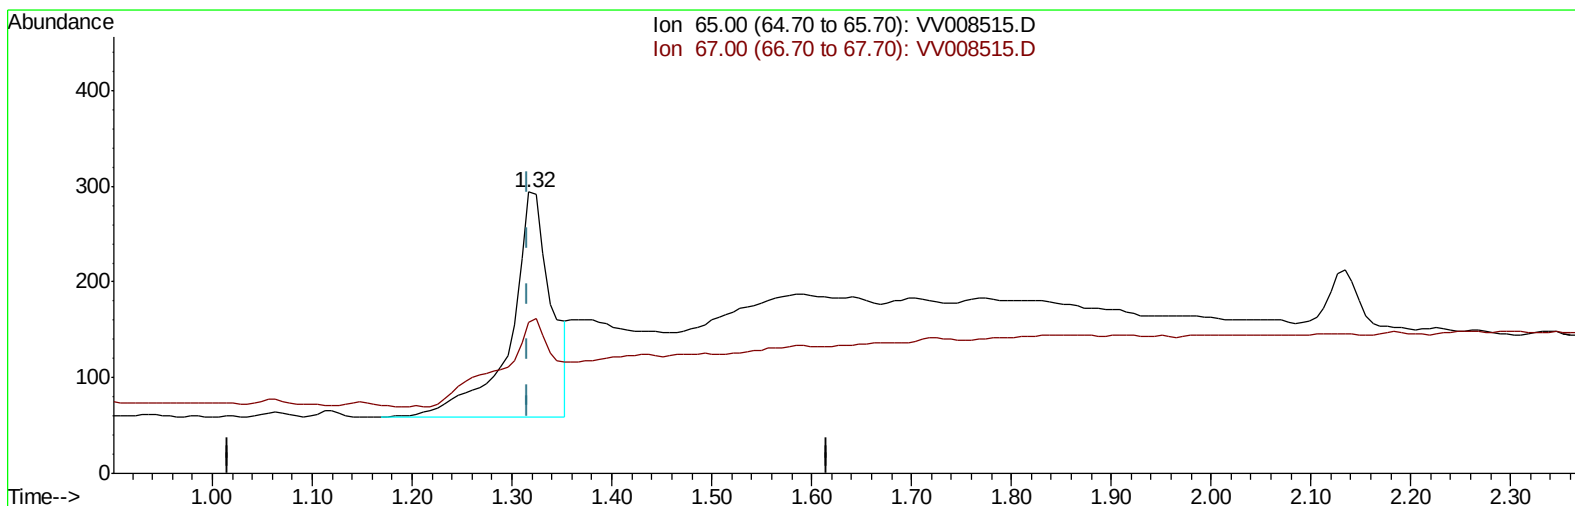

TIC: VV008515.D

(2) Vinyl Chloride-d3 (S)




1.317min (+0.001) 0.12ug/L

response 666

Ion	Exp%	Act%
65.00	100	100
67.00	35.50	53.90#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008515.D
Acq On : 05 Nov 2018 12:28
Operator : SY/MD
Sample : VSTD0.0540
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 06 10:34:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:32:16 2018
Response via : Initial Calibration

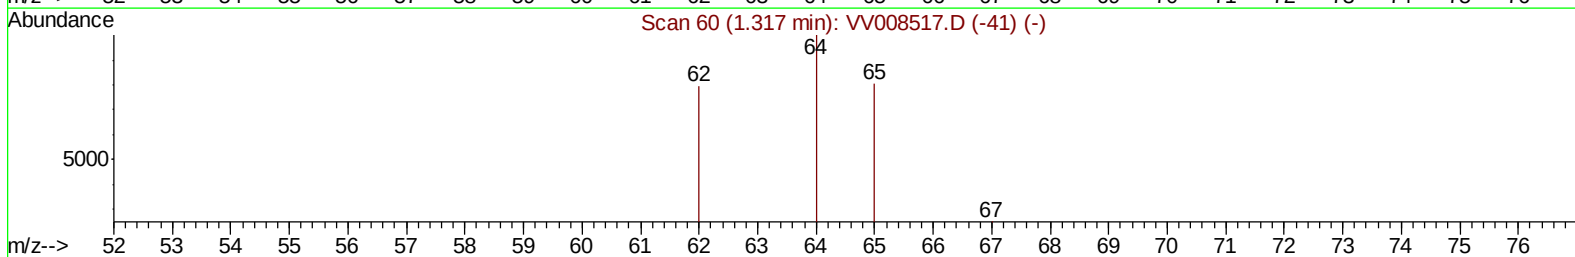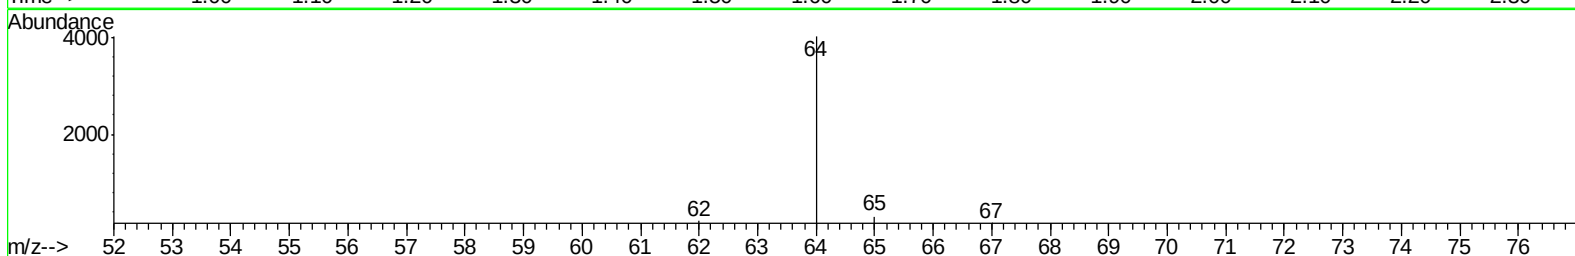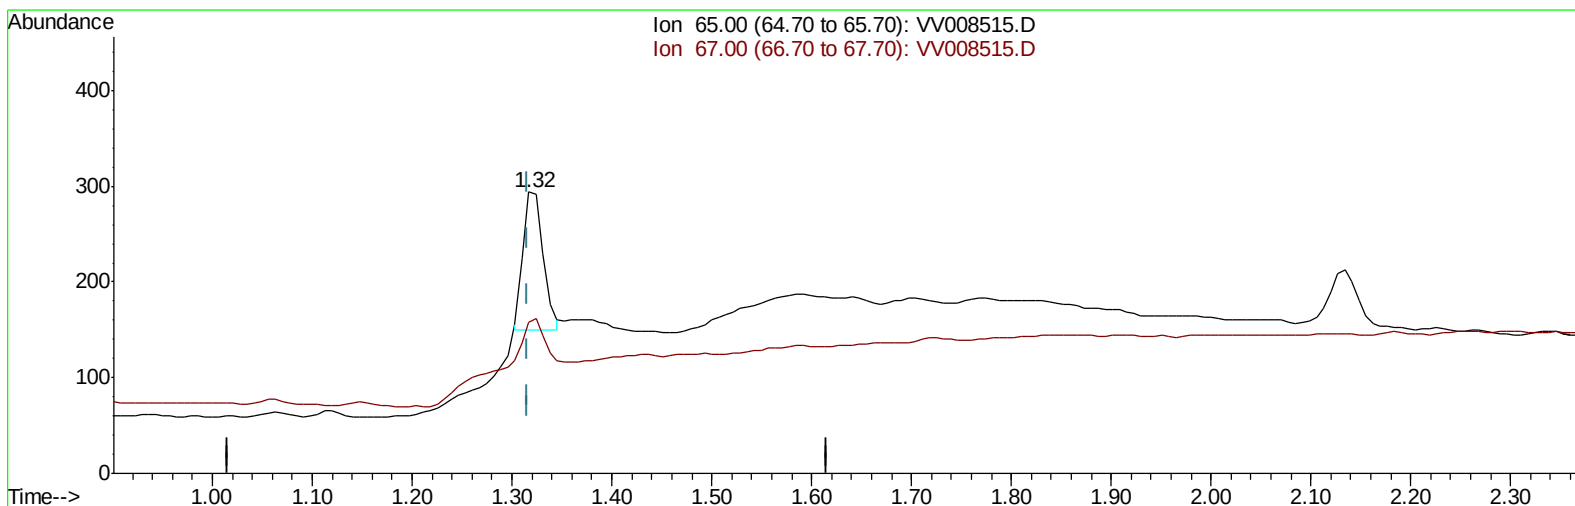

TIC: VV008515.D

(2) Vinyl Chloride-d3 (S)




1.317min (+0.001) 0.04ug/L m

response 202

Ion	Exp%	Act%
65.00	100	100
67.00	35.50	177.72#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008515.D
Acq On : 05 Nov 2018 12:28
Operator : SY/MD
Sample : VSTD0.0540
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 06 10:34:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:32:16 2018
Response via : Initial Calibration

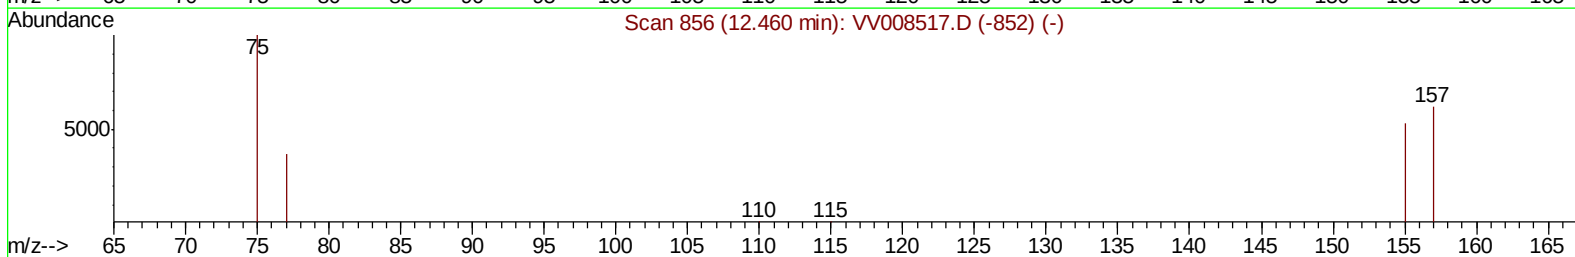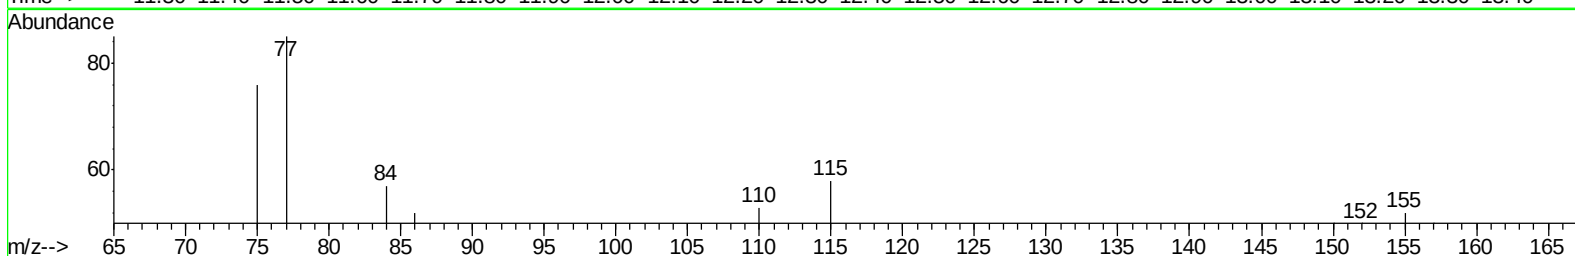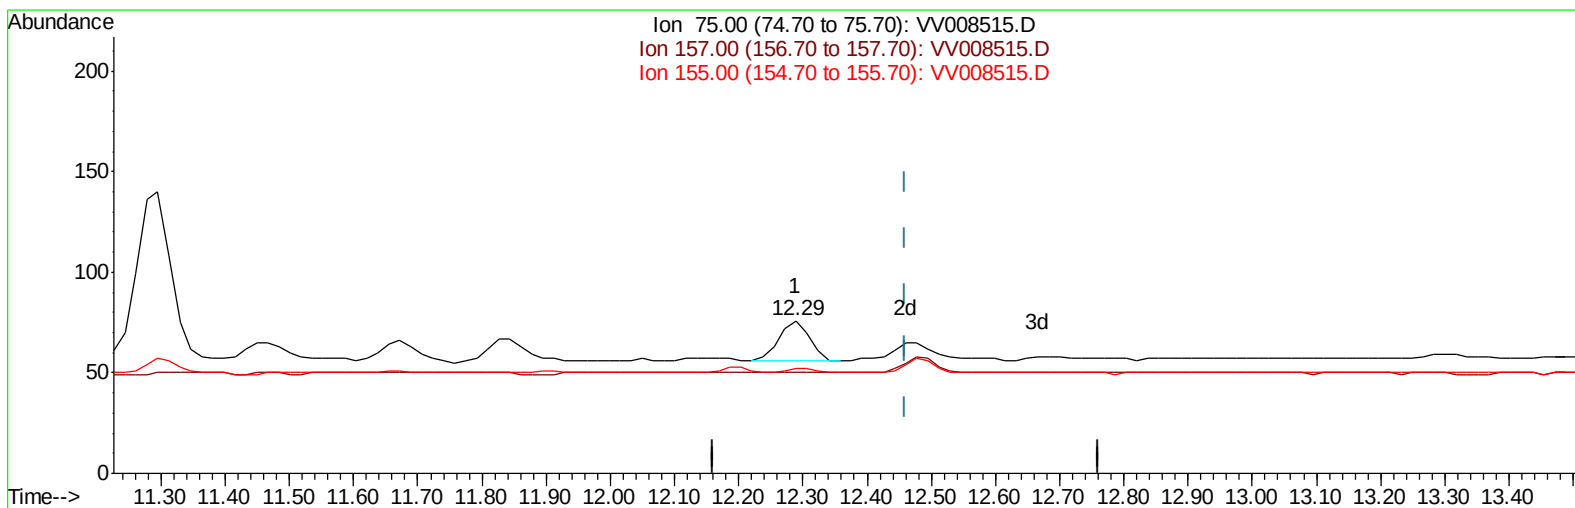

TIC: VV008515.D

(13) 1,2-Dibromo-3-chloropropane (T)




12.289min (-0.171) 0.11ug/L

response 66

Ion	Exp%	Act%
75.00	100	100
157.00	71.10	65.79
155.00	65.40	68.42
0.00	0.00	0.00

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008515.D
Acq On : 05 Nov 2018 12:28
Operator : SY/MD
Sample : VSTD0.0540
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 06 10:34:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:32:16 2018
Response via : Initial Calibration

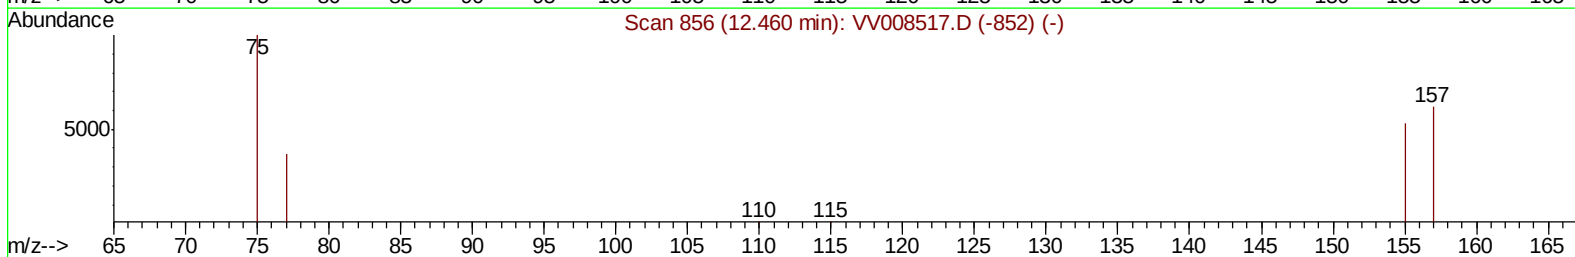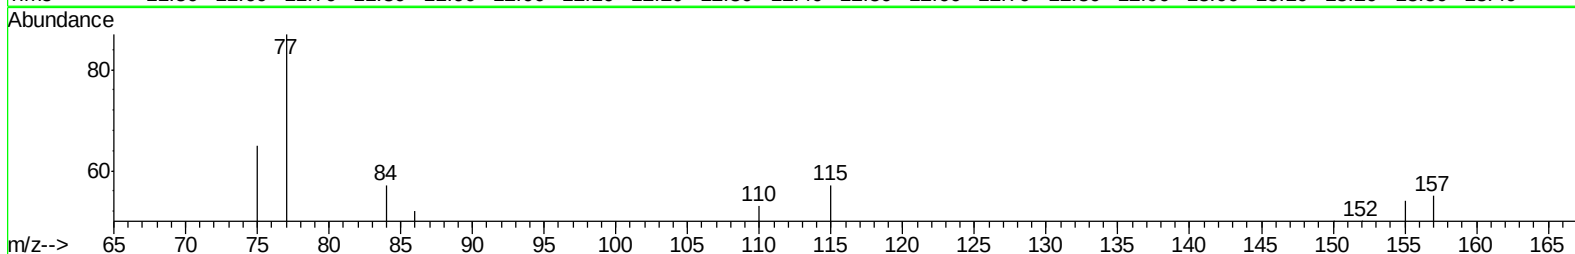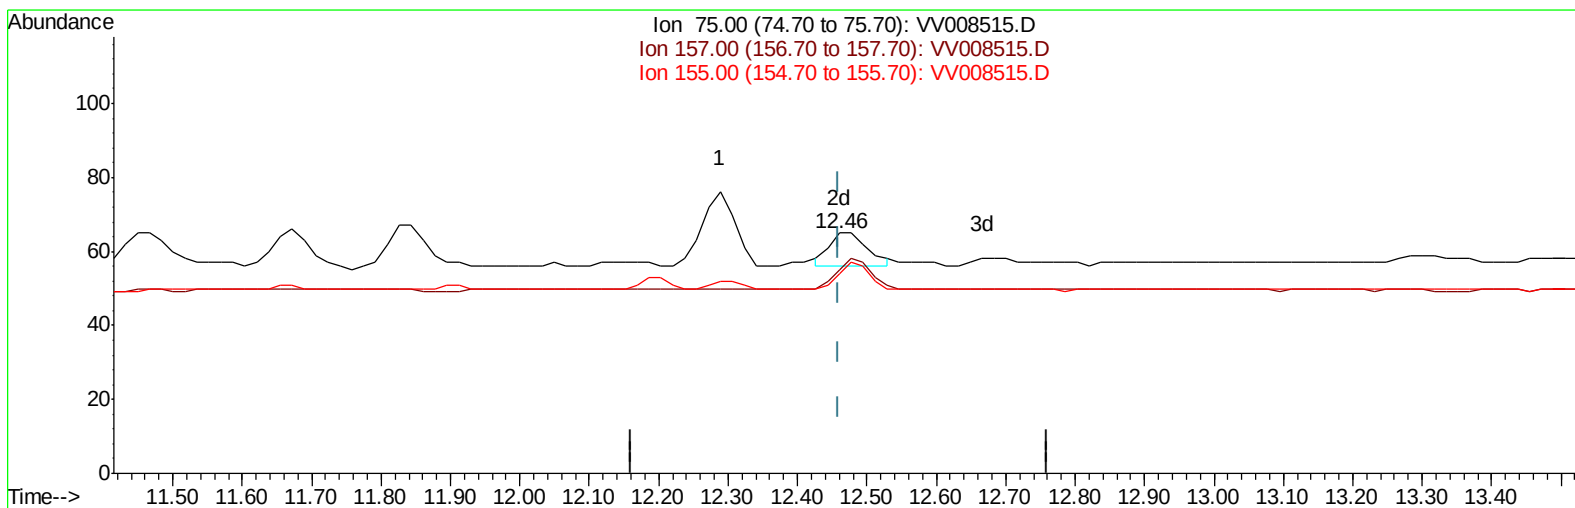

TIC: VV008515.D

(13) 1,2-Dibromo-3-chloropropane (T)

12.460min (-0.000) 0.06ug/L m

response 35

Ion	Exp%	Act%
75.00	100	100
157.00	71.10	84.62
155.00	65.40	83.08#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
 Data File : VV008515.D
 Acq On : 05 Nov 2018 12:28
 Operator : SY/MD
 Sample : VSTD0.0540
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 06 10:44:10 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 06 10:32:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	6259	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.89	117	5489	0.50	ug/L	0.00
10) 1,4-Dichlorobenzene-d4	11.29	152	2325	0.50	ug/L	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) Vinyl Chloride-d3	1.32	65	202m	0.04	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.09	65	231	0.05	ug/L	0.00
7) Toluene-d8	7.36	98	692	0.05	ug/L	0.02
9) 1,1,2,2-Tetrachloroethane-	10.25	84	193	0.05	ug/L	0.00
11) 1-2-dichlorobenzene-d4	11.67	152	265	0.06	ug/L	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Vinyl chloride	1.32	62	300	0.058	ug/L #	1
6) Trichloroethene	5.96	95	347	0.064	ug/L	94
8) 1,2-Dibromoethane	8.40	107	150	0.048	ug/L #	88
12) 1,2,3-Trichloropropane	10.32	75	129	0.045	ug/L	97
13) 1,2-Dibromo-3-chloropropan	12.46	75	35m	0.059	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008515.D
Acq On : 05 Nov 2018 12:28
Operator : SY/MD
Sample : VSTD0.0540
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 06 10:44:10 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:32:16 2018
Response via : Initial Calibration

