
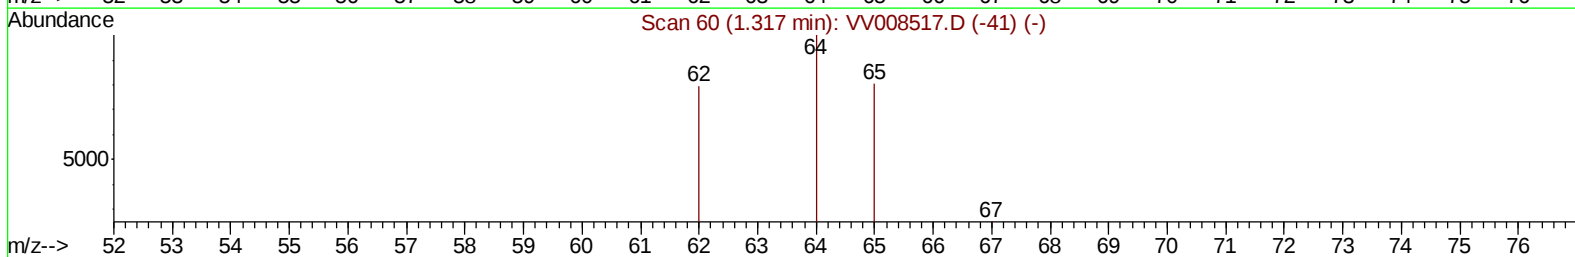
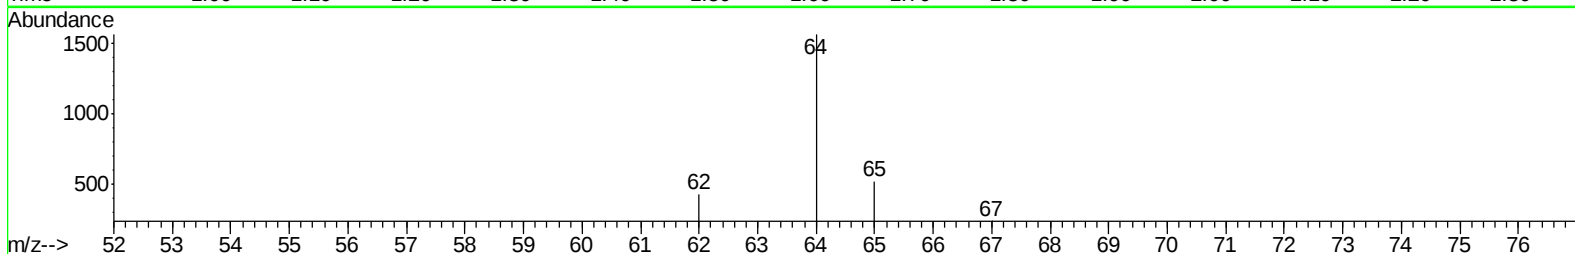


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008516.D
Acq On : 05 Nov 2018 13:06
Operator : SY/MD
Sample : VSTD0.141
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Nov 06 10:40:04 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:32:16 2018
Response via : Initial Calibration

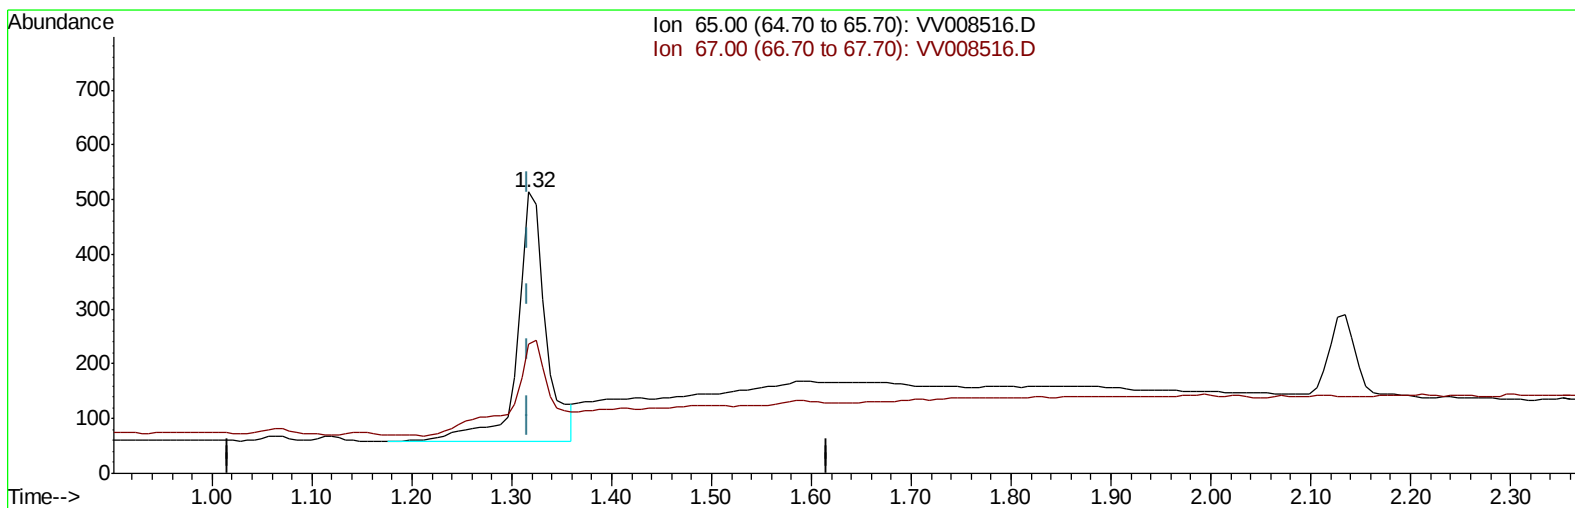

TIC: VV008516.D

(2) Vinyl Chloride-d3 (S)




1.317min (+0.001) 0.13ug/L

response 915

Ion	Exp%	Act%
65.00	100	100
67.00	35.50	51.91#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008516.D
Acq On : 05 Nov 2018 13:06
Operator : SY/MD
Sample : VSTD0.141
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Nov 06 10:40:04 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:32:16 2018
Response via : Initial Calibration

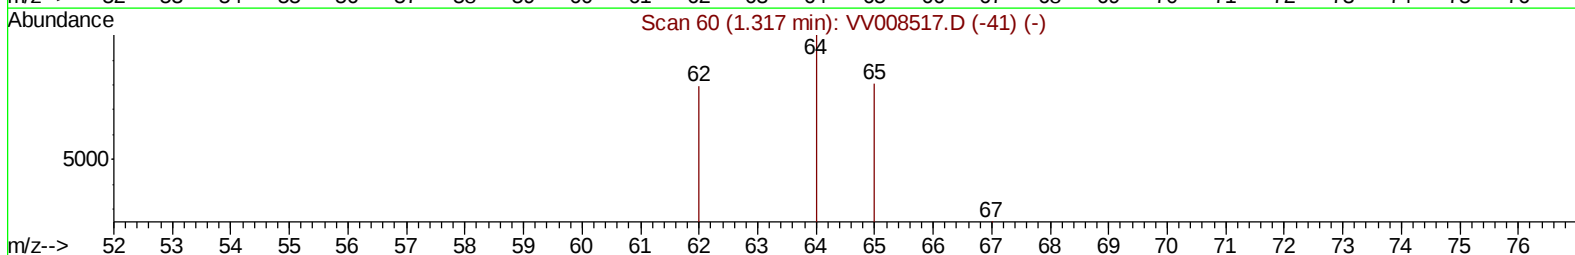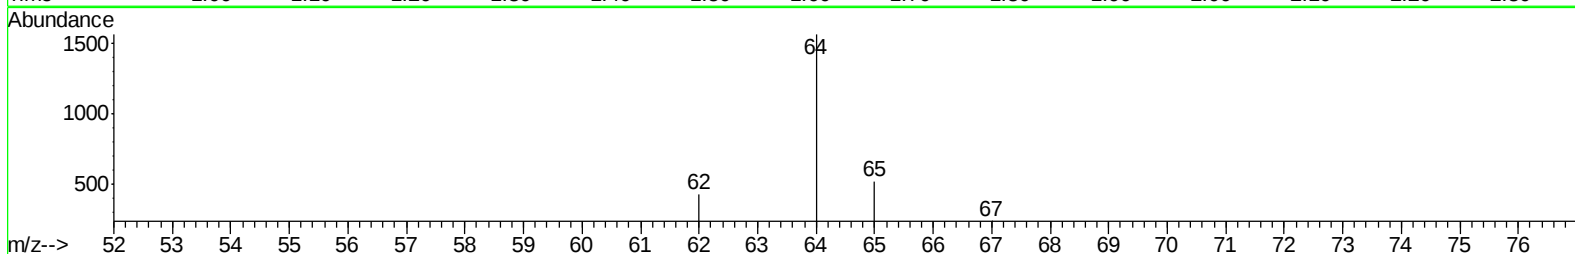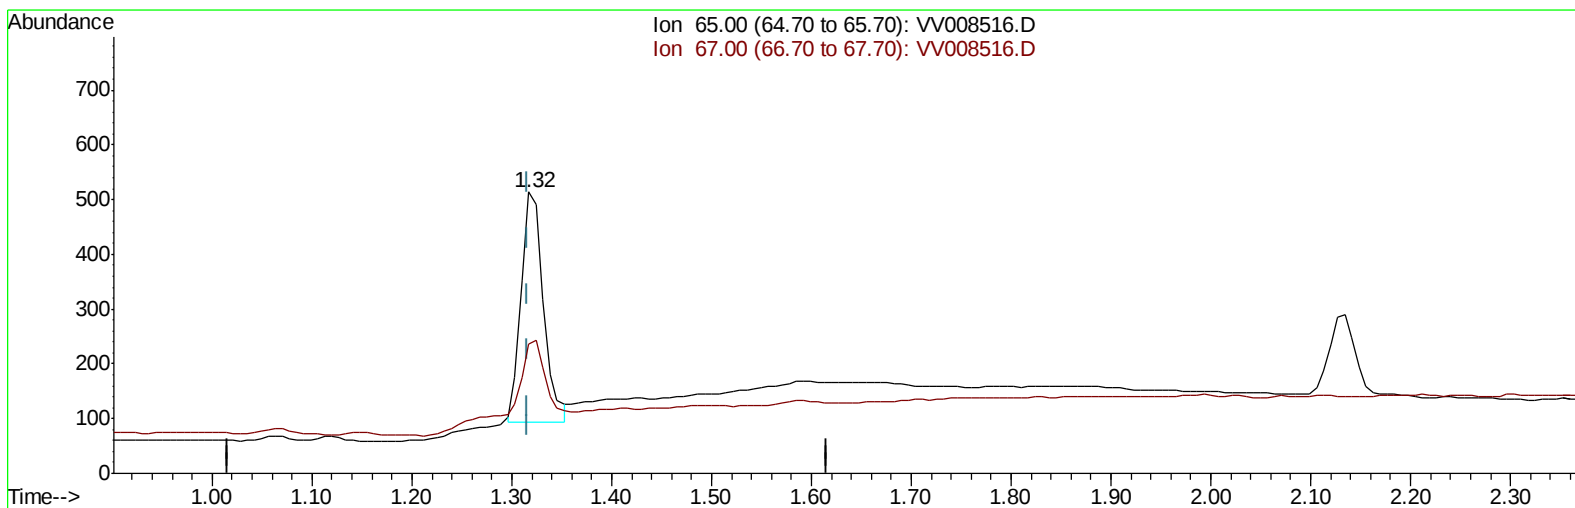

TIC: VV008516.D

(2) Vinyl Chloride-d3 (S)

1.317min (+0.001) 0.09ug/L m

response 649

Ion	Exp%	Act%
65.00	100	100
67.00	35.50	73.19#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
 Data File : VV008516.D
 Acq On : 05 Nov 2018 13:06
 Operator : SY/MD
 Sample : VSTD0.141
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Nov 06 10:45:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 06 10:32:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	8002	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.89	117	7015	0.50	ug/L	0.00
10) 1,4-Dichlorobenzene-d4	11.30	152	2976	0.50	ug/L	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) Vinyl Chloride-d3	1.32	65	649m	0.09	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.09	65	584	0.10	ug/L	0.00
7) Toluene-d8	7.35	98	1784	0.10	ug/L	0.00
9) 1,1,2,2-Tetrachloroethane-	10.25	84	485	0.10	ug/L	0.00
11) 1-2-dichlorobenzene-d4	11.67	152	646	0.11	ug/L	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Vinyl chloride	1.32	62	625	0.094	ug/L #	1
6) Trichloroethene	5.96	95	707	0.103	ug/L	97
8) 1,2-Dibromoethane	8.40	107	348	0.088	ug/L #	94
12) 1,2,3-Trichloropropane	10.32	75	318	0.087	ug/L	94
13) 1,2-Dibromo-3-chloropropan	12.46	75	83	0.110	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008516.D
Acq On : 05 Nov 2018 13:06
Operator : SY/MD
Sample : VSTD0.141
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Nov 06 10:45:45 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:32:16 2018
Response via : Initial Calibration

