
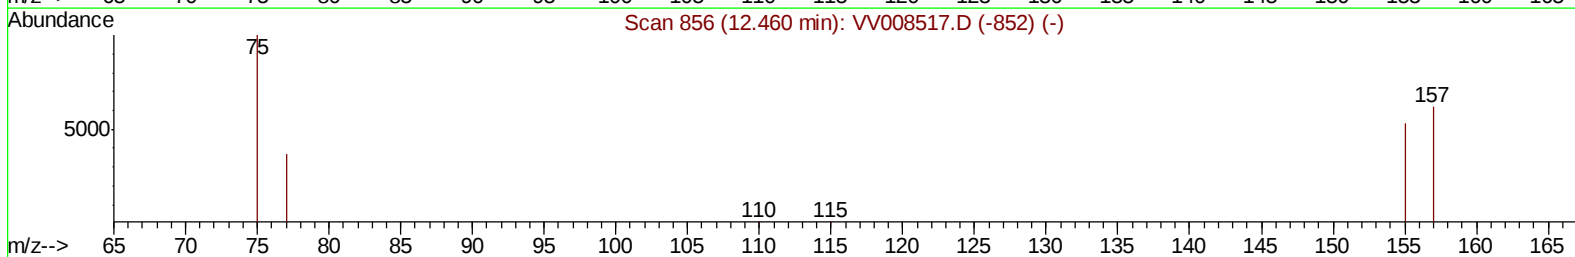
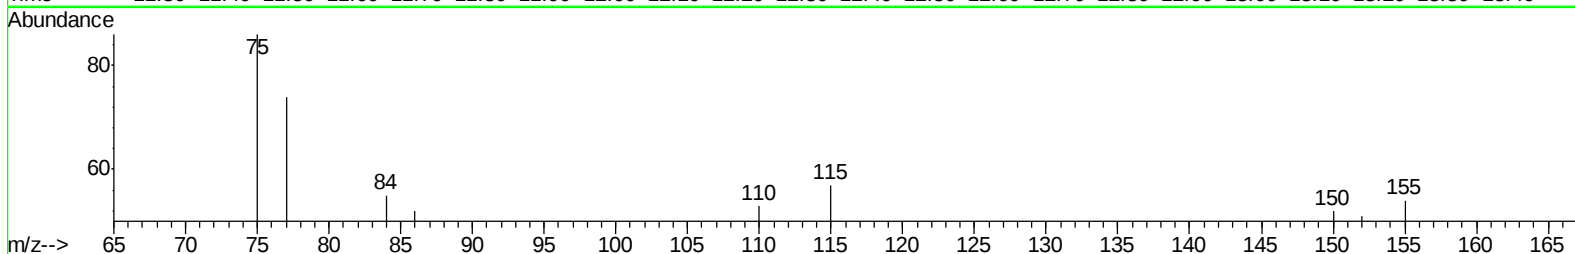


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008527.D
Acq On : 05 Nov 2018 19:19
Operator : SY/MD
Sample : MDL06
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 06 11:01:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:52:01 2018
Response via : Initial Calibration

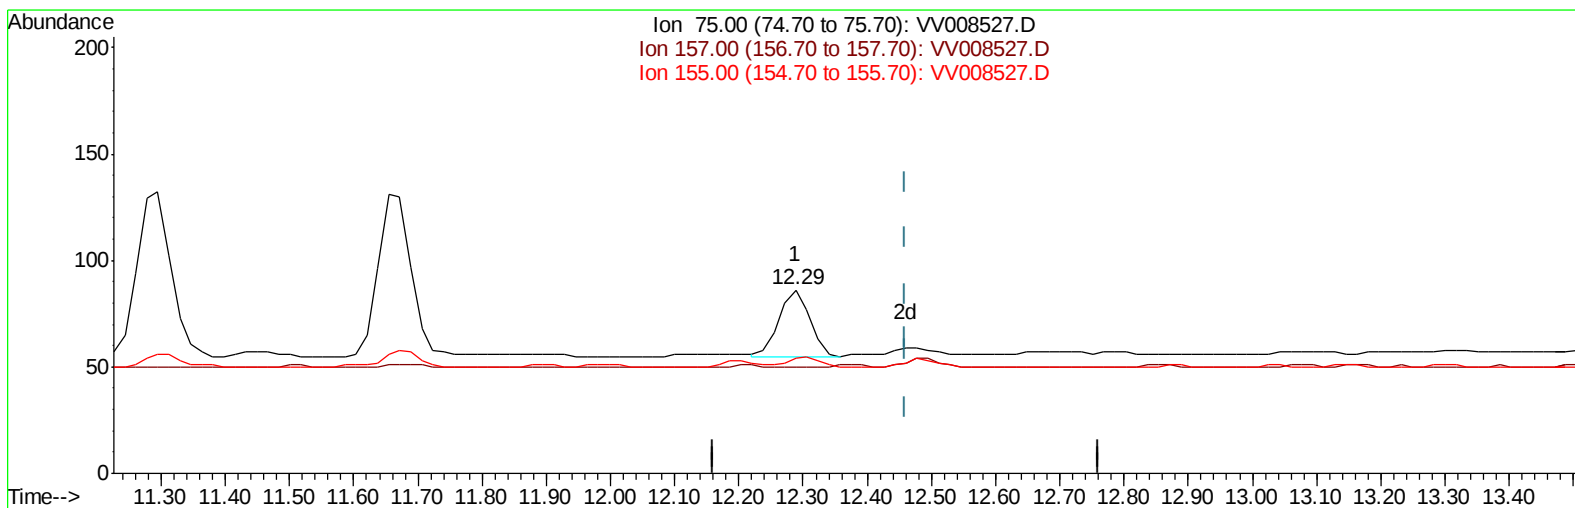

TIC: VV008527.D

(13) 1,2-Dibromo-3-chloropropane (T)




12.289min (-0.172) 0.18ug/L

response 104

Ion	Exp%	Act%
75.00	100	100
157.00	71.10	58.14
155.00	65.40	62.79
0.00	0.00	0.00

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008527.D
Acq On : 05 Nov 2018 19:19
Operator : SY/MD
Sample : MDL06
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 06 11:01:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:52:01 2018
Response via : Initial Calibration

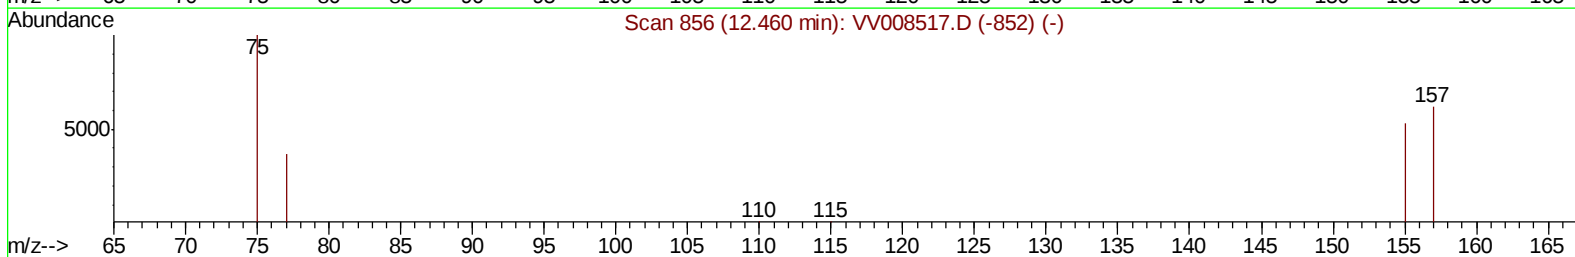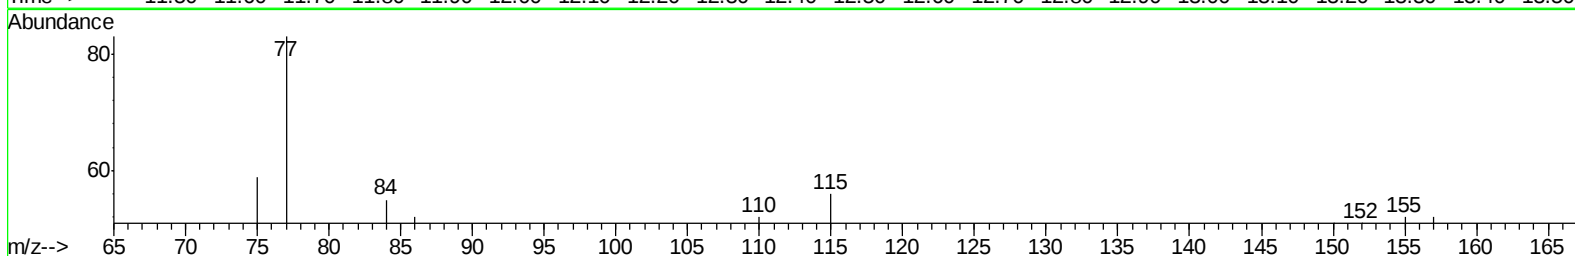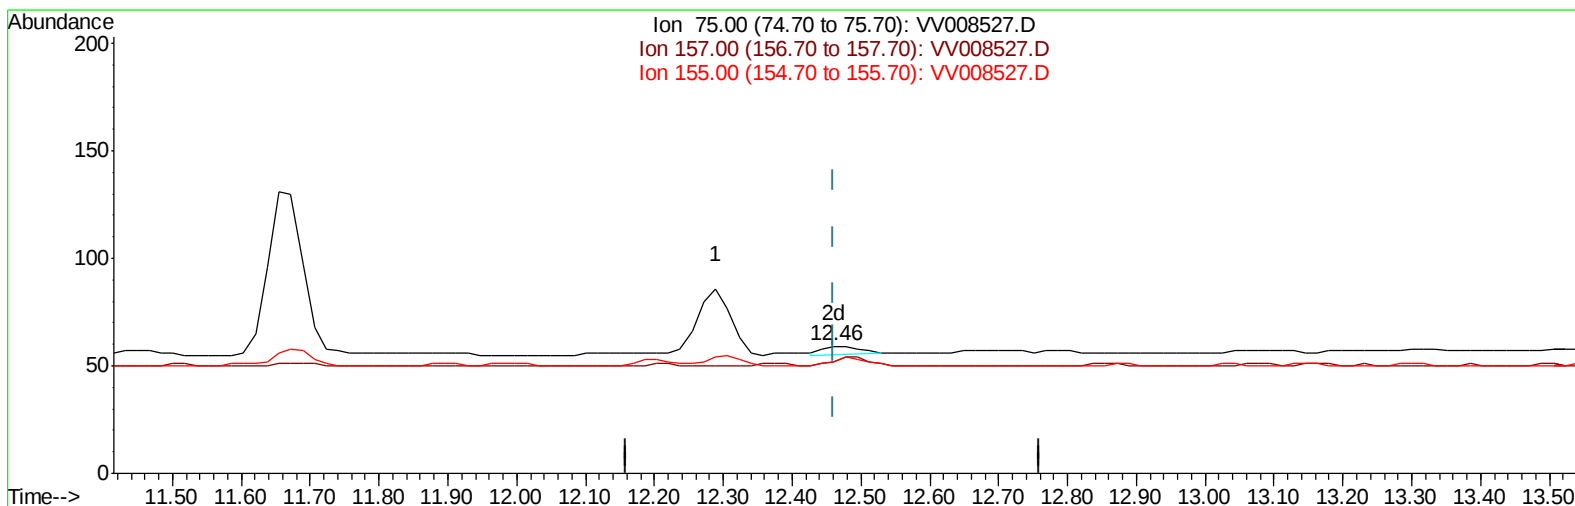

TIC: VV008527.D

(13) 1,2-Dibromo-3-chloropropane (T)

12.460min (-0.000) 0.03ug/L m

response 17

Ion	Exp%	Act%
75.00	100	100
157.00	71.10	88.14#
155.00	65.40	88.14#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
 Data File : VV008527.D
 Acq On : 05 Nov 2018 19:19
 Operator : SY/MD
 Sample : MDL06
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 06 11:11:19 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 06 10:52:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	6090	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.89	117	5318	0.50	ug/L	0.00
10) 1,4-Dichlorobenzene-d4	11.29	152	2229	0.50	ug/L	0.00

System Monitoring Compounds

2) Vinyl Chloride-d3	1.32	65	2574	0.53	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	106.00%
4) 1,2-Dichloroethane-d4	5.09	65	2344	0.52	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.00%
7) Toluene-d8	7.36	98	6778	0.50	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.00%
9) 1,1,2,2-Tetrachloroethane-	10.25	84	1949	0.53	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	106.00%
11) 1-2-dichlorobenzene-d4	11.67	152	2350	0.50	ug/L	0.00
Spiked Amount	0.500		Recovery	=	100.00%	

Target Compounds

					Qvalue
3) Vinyl chloride	1.32	62	207	0.041 ug/L #	1
6) Trichloroethene	5.96	95	206	0.038 ug/L	93
8) 1,2-Dibromoethane	8.40	107	75	0.026 ug/L #	82
12) 1,2,3-Trichloropropane	10.30	75	68	0.026 ug/L #	88
13) 1,2-Dibromo-3-chloropropan	12.46	75	17m	0.029 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110518\
Data File : VV008527.D
Acq On : 05 Nov 2018 19:19
Operator : SY/MD
Sample : MDL06
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 06 11:11:19 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 06 10:52:01 2018
Response via : Initial Calibration

