


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110518\
Data File : VV008514.D
Acq On : 05 Nov 2018 11:27
Operator : SY/MD
Sample : BFB40
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110518SIM.M
Title : TRACE VOA SOM01.0
Last Update : Tue Nov 06 10:52:01 2018

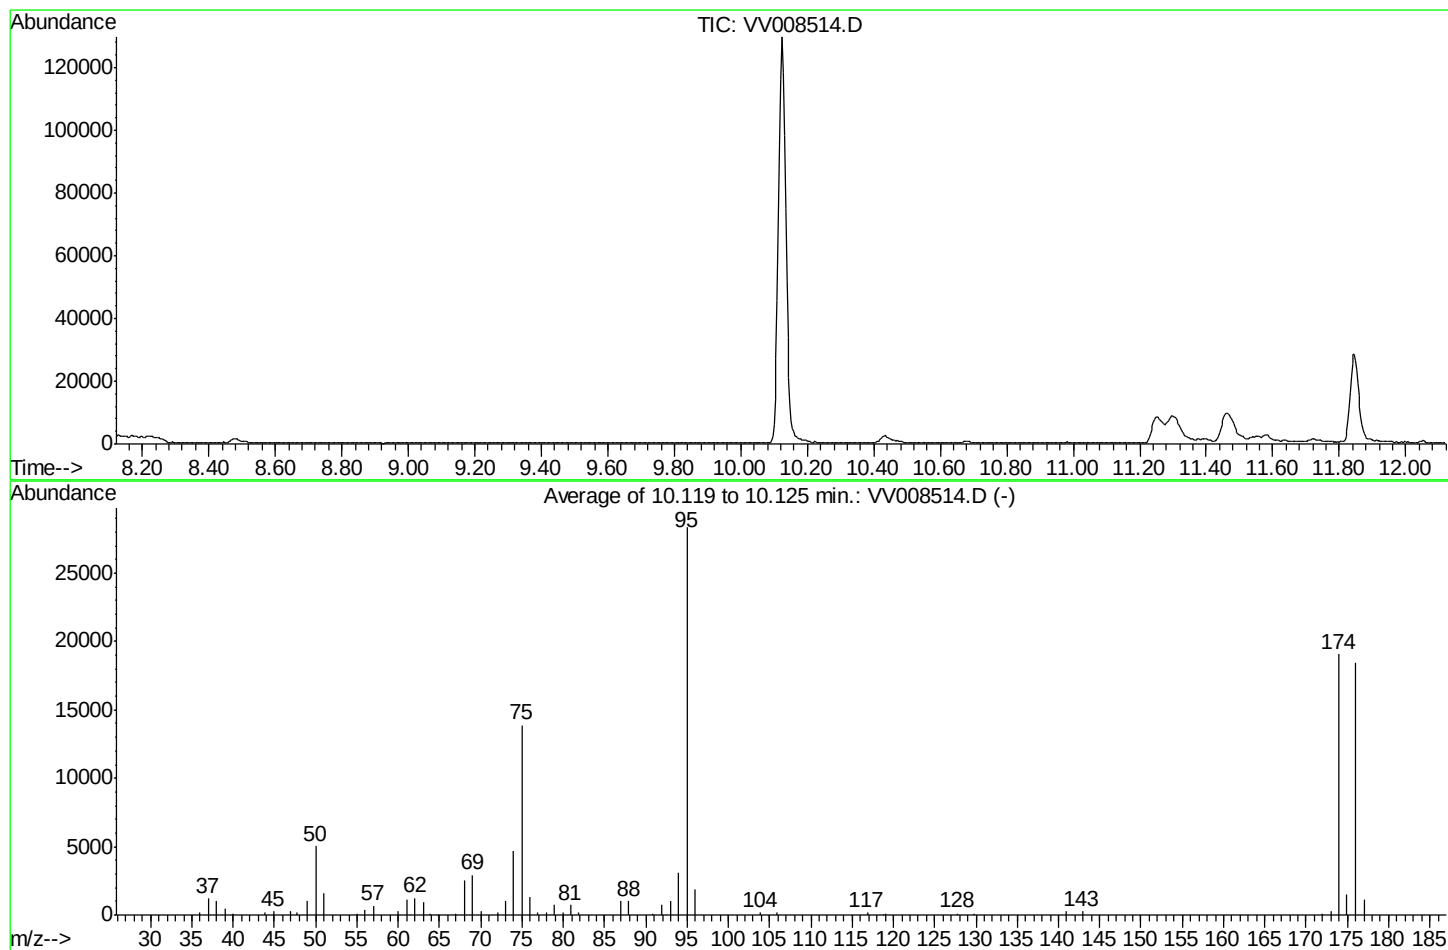

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	5013	PASS
75	95	30	80	48.9	13873	PASS
95	95	100	100	100.0	28349	PASS
96	95	5	9	6.5	1830	PASS
173	174	0.00	2	1.3	245	PASS
174	95	50	120	67.3	19082	PASS
175	174	5	9	8.0	1521	PASS
176	174	95	101	96.8	18469	PASS
177	176	5	9	6.3	1157	PASS

m/z	Abundance
44.00	379.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
35.90	199.0
37.00	1108.0
38.00	1092.0
39.00	473.0
39.90	112.0
43.90	485.0
44.90	217.0
47.00	274.0
47.70	157.0
48.90	1040.0
50.00	4740.0
51.00	1487.0
55.00	116.0
55.90	304.0
57.00	651.0
59.90	219.0
61.00	1035.0
62.00	1071.0
63.00	930.0
67.00	105.0
68.00	2449.0
69.00	2674.0
70.00	276.0
72.10	116.0
73.00	993.0
74.00	4383.0
75.00	13038.0
76.00	1272.0
77.00	215.0
77.90	188.0
78.90	717.0
80.00	202.0
80.90	682.0
81.90	172.0
86.90	956.0
87.90	976.0
91.90	792.0
93.00	1073.0
94.00	2873.0
95.00	26720.0
96.00	1773.0
103.90	147.0
105.80	160.0
116.80	167.0
119.10	129.0
127.80	125.0
140.90	191.0
142.90	216.0
172.00	146.0
173.10	233.0
174.00	17424.0
174.90	1378.0
176.00	16688.0
177.00	1078.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
35.90	248.0
37.00	1229.0
38.00	1083.0
39.00	502.0
40.00	108.0
43.90	563.0
44.90	241.0
47.00	295.0
47.70	172.0
48.90	1094.0
50.00	5192.0
51.00	1628.0
54.90	131.0
55.90	352.0
57.00	686.0
59.90	253.0
61.00	1181.0
62.00	1298.0
63.00	982.0
63.90	105.0
67.00	110.0
68.00	2619.0
69.00	3068.0
70.00	287.0
72.00	143.0
73.00	1083.0
74.00	4787.0
75.00	14327.0
76.00	1326.0
76.90	238.0
77.90	185.0
78.90	726.0
79.90	221.0
80.90	753.0
81.90	214.0
86.90	1035.0
88.00	1048.0
90.80	113.0
91.90	823.0
93.00	1094.0
94.00	3131.0
95.00	29272.0
96.00	1899.0
103.90	153.0
105.80	151.0
116.80	187.0
119.10	135.0
127.80	128.0
129.80	107.0
140.90	244.0
142.90	260.0
172.00	131.0
173.00	255.0
174.00	19752.0
174.90	1583.0
176.00	19112.0
177.00	1174.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
35.00	261.0
37.00	1232.0
38.00	1027.0
39.00	475.0
40.00	109.0
43.90	575.0
44.90	260.0
46.90	311.0
47.70	179.0
49.00	1057.0
50.00	5107.0
51.00	1619.0
54.90	133.0
55.90	358.0
57.00	695.0
60.00	248.0
61.00	1262.0
62.00	1345.0
63.00	892.0
63.80	147.0
64.80	101.0
66.90	114.0
68.00	2601.0
69.00	3108.0
70.00	241.0
71.90	187.0
72.90	1082.0
74.00	4794.0
75.00	14254.0
76.00	1265.0
76.90	215.0
77.90	144.0
78.90	683.0
79.90	221.0
80.90	762.0
81.90	229.0
87.00	1005.0
88.00	1029.0
90.80	141.0
92.00	762.0
93.00	1057.0
94.00	3199.0
95.00	29056.0
96.00	1818.0
103.90	137.0
105.80	126.0
116.90	190.0
118.80	132.0
119.10	135.0
127.80	115.0
129.80	115.0
140.90	291.0
142.90	292.0
171.90	122.0
173.00	248.0
174.00	20072.0
174.90	1604.0
176.00	19608.0
177.00	1220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40