


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110519\
Data File : VV013484.D
Acq On : 05 Nov 2019 08:38
Operator : SY/MD
Sample : BFB55
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB55

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR103119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Nov 06 02:12:23 2019

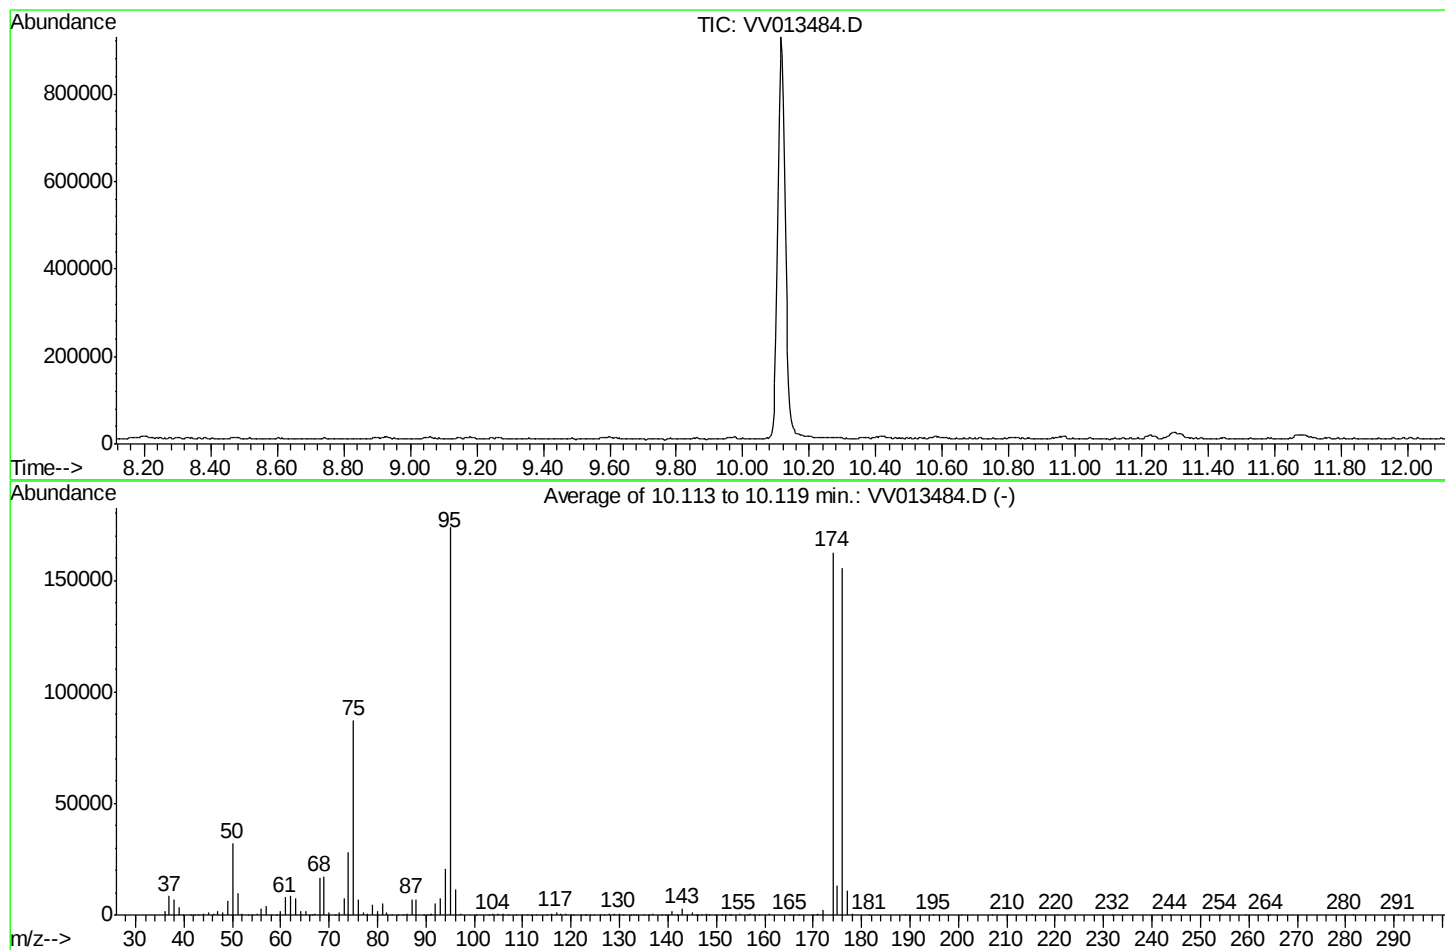

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	31880	PASS
75	95	30	80	50.1	87047	PASS
95	95	100	100	100.0	173717	PASS
96	95	5	9	6.6	11436	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	93.6	162538	PASS
175	174	5	9	8.0	12970	PASS
176	174	95	101	95.5	155242	PASS
177	176	5	9	6.9	10729	PASS

m/z	Abundance
36.00	1458.0
37.00	8571.0
38.00	7316.0
39.10	3375.0
39.90	1370.0
41.00	232.0
42.10	268.0
43.10	195.0
44.00	1905.0
45.00	1398.0
46.00	489.0
47.10	1926.0
48.10	1075.0
49.00	6882.0
50.10	32064.0
51.10	9980.0
52.00	497.0
53.20	319.0
54.00	218.0
55.00	733.0
56.00	2490.0
57.00	4085.0
57.90	270.0
60.00	1826.0
61.00	7844.0
62.00	8548.0
63.00	6947.0
64.10	1577.0
65.00	1766.0
66.00	252.0
67.00	547.0
68.00	16976.0
69.00	17432.0
70.00	1081.0
71.90	1000.0
73.10	7905.0
74.00	27656.0
75.00	86744.0
76.10	6968.0
77.00	1435.0
77.90	807.0
78.90	4799.0
79.90	1607.0
81.00	5464.0
81.90	1379.0
83.20	259.0
84.10	173.0
85.20	173.0
86.00	412.0
87.00	6509.0
88.00	6600.0
89.40	126.0
91.10	694.0
92.00	5107.0
93.00	7601.0
94.00	20544.0
95.00	170688.0
96.00	11614.0
97.00	366.0
103.00	231.0
103.90	661.0
104.80	344.0
105.90	544.0
106.90	262.0
108.50	121.0
109.90	264.0
110.80	137.0
112.80	224.0
114.80	206.0
115.90	646.0
117.00	1170.0
117.90	662.0
118.90	926.0
122.10	125.0
123.00	111.0
123.80	266.0
126.80	137.0
127.90	526.0
128.80	398.0
129.90	754.0
130.80	229.0
132.30	103.0
133.60	153.0
135.00	397.0
136.00	209.0
137.00	322.0
138.80	140.0
140.00	197.0
140.90	1739.0
142.90	2690.0
144.00	312.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

145.00	1101.0
146.10	286.0
146.80	263.0
148.00	550.0
149.90	248.0
151.20	155.0
151.90	143.0
153.00	250.0
153.70	167.0
154.90	541.0
156.40	139.0
156.90	412.0
158.70	244.0
160.80	317.0
165.20	175.0
171.10	634.0
171.90	2253.0
174.00	155264.0
175.00	13148.0
175.90	148928.0
177.00	10771.0
178.20	293.0
181.60	113.0
189.10	104.0
205.20	203.0
207.00	116.0
210.10	130.0
215.00	104.0
220.30	108.0
231.90	104.0
243.70	105.0
263.60	104.0
264.30	117.0
279.80	118.0
290.80	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
35.60	163.0
36.30	151.0
37.10	181.0
38.20	366.0
39.20	214.0
39.90	1146.0
41.00	211.0
42.40	158.0
43.10	187.0
44.00	1218.0
45.00	227.0
45.80	124.0
46.40	148.0
47.10	140.0
48.00	185.0
48.40	153.0
49.70	161.0
51.30	169.0
53.50	144.0
54.50	150.0
55.10	113.0
56.30	165.0
56.70	189.0
57.40	141.0
60.90	105.0
62.00	117.0
62.50	123.0
63.30	102.0
63.70	160.0
65.20	135.0
67.40	120.0
68.30	124.0
68.90	180.0
71.50	130.0
72.60	124.0
75.00	105.0
76.00	107.0
76.70	104.0
77.20	150.0
79.10	138.0
80.10	106.0
81.00	105.0
81.30	101.0
82.10	143.0
83.00	116.0
85.00	126.0
88.30	157.0
89.10	179.0
92.40	110.0
93.80	106.0
97.50	125.0
98.20	111.0
100.70	112.0
101.80	223.0
104.10	192.0
104.80	132.0
105.70	125.0
107.80	120.0
113.40	102.0
114.40	107.0
116.50	170.0
117.40	112.0
119.10	127.0
127.50	107.0
130.10	108.0
130.70	117.0
131.50	104.0
135.00	145.0
153.70	121.0
162.20	109.0
171.60	107.0
198.10	105.0
205.30	122.0
207.00	113.0
209.30	105.0
220.70	110.0
232.70	143.0
249.40	110.0
260.60	114.0
288.00	103.0
294.60	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.10	1646.0
37.00	8248.0
38.00	6578.0
39.00	3704.0
40.00	1489.0
41.40	140.0
42.20	219.0
43.00	213.0
44.00	2273.0
45.00	1398.0
46.10	416.0
47.00	1867.0
47.90	1350.0
49.00	6159.0
50.00	30688.0
51.00	9147.0
52.10	468.0
53.20	248.0
53.90	270.0
55.00	502.0
56.00	2706.0
57.00	3877.0
58.10	307.0
59.10	176.0
60.00	1440.0
61.00	8202.0
62.00	8302.0
63.00	7506.0
64.00	1419.0
65.10	1670.0
66.40	339.0
67.10	737.0
68.00	16182.0
69.00	16528.0
70.00	1162.0
71.20	279.0
71.90	874.0
73.00	7380.0
74.00	28328.0
75.00	84944.0
76.00	7201.0
77.00	1495.0
78.00	930.0
78.90	4708.0
79.90	1539.0
80.90	4874.0
81.90	1065.0
83.00	342.0
84.10	160.0
84.80	111.0
85.90	436.0
87.00	7388.0
88.00	6815.0
89.60	141.0
90.20	145.0
90.80	462.0
91.20	519.0
92.00	5502.0
93.00	7500.0
94.00	20088.0
95.00	171264.0
96.00	10983.0
97.00	507.0
100.30	117.0
103.00	178.0
103.90	788.0
104.80	509.0
105.80	579.0
106.90	225.0
108.40	129.0
109.80	181.0
110.80	108.0
111.80	134.0
112.80	172.0
113.50	135.0
114.80	339.0
115.90	722.0
117.00	1313.0
117.90	657.0
119.00	1064.0
119.90	140.0
122.70	151.0
123.80	228.0
124.80	139.0
126.10	112.0
126.90	178.0
127.90	768.0
128.80	368.0
129.90	785.0
130.70	241.0
131.70	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

132.40	178.0
132.80	138.0
135.00	321.0
136.00	188.0
136.90	309.0
139.40	118.0
139.90	131.0
140.90	1503.0
141.80	281.0
143.00	2879.0
143.90	283.0
144.90	1129.0
145.70	283.0
146.90	178.0
148.00	547.0
148.60	180.0
149.70	225.0
152.60	161.0
154.70	469.0
156.90	482.0
157.80	175.0
158.70	299.0
160.90	346.0
165.90	120.0
167.00	125.0
169.80	116.0
170.60	430.0
171.00	380.0
172.00	2411.0
174.00	164288.0
175.00	12311.0
175.90	156224.0
177.00	10216.0
178.00	385.0
194.80	145.0
200.70	108.0
206.90	126.0
249.60	109.0
254.00	155.0
259.20	103.0
263.60	113.0
281.50	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.10	1652.0
37.00	8931.0
38.00	7188.0
39.00	3597.0
40.00	1472.0
41.00	175.0
41.40	173.0
42.20	273.0
43.10	218.0
44.00	2110.0
45.00	1391.0
46.10	501.0
47.00	1795.0
47.90	1223.0
49.00	6713.0
50.00	32888.0
51.00	10046.0
52.00	482.0
53.20	309.0
54.00	262.0
55.00	664.0
56.00	2797.0
57.00	4099.0
58.00	280.0
59.10	155.0
60.00	1675.0
61.00	8319.0
62.00	8759.0
63.00	7854.0
64.00	1649.0
65.00	1861.0
66.00	314.0
67.00	691.0
68.00	17592.0
69.00	17920.0
70.00	1139.0
71.30	300.0
72.00	956.0
73.00	7968.0
74.00	29256.0
75.00	89768.0
76.10	7288.0
77.00	1641.0
77.90	867.0
78.90	4960.0
79.90	1653.0
80.90	5321.0
81.90	1270.0
83.00	335.0
84.10	194.0
85.20	127.0
85.90	460.0
87.00	7178.0
88.00	7035.0
89.50	125.0
91.10	664.0
92.00	5716.0
93.00	7936.0
94.00	21192.0
95.00	179200.0
96.00	11712.0
97.10	415.0
100.30	119.0
103.00	190.0
103.90	745.0
104.80	486.0
105.90	558.0
106.90	253.0
108.50	128.0
109.90	260.0
110.80	119.0
111.80	126.0
112.80	181.0
113.40	113.0
114.80	294.0
115.90	708.0
117.00	1203.0
117.90	686.0
119.00	1020.0
120.40	121.0
123.00	117.0
123.80	249.0
124.70	125.0
126.90	161.0
127.90	672.0
128.80	429.0
129.80	723.0
130.70	218.0
132.40	139.0
133.40	113.0
135.00	381.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

136.00	214.0
136.90	313.0
138.80	108.0
139.40	107.0
140.00	186.0
140.90	1681.0
143.00	2900.0
143.90	327.0
144.90	1209.0
145.80	229.0
146.20	283.0
146.70	223.0
148.00	560.0
149.80	225.0
151.30	112.0
151.90	145.0
152.90	171.0
153.70	113.0
154.80	510.0
156.90	490.0
158.70	291.0
160.90	339.0
165.20	147.0
167.00	108.0
171.10	492.0
172.00	2436.0
174.00	168064.0
175.00	13452.0
175.90	160576.0
177.00	11202.0
178.00	342.0
181.60	113.0
188.90	103.0
194.80	106.0
205.20	132.0
206.90	100.0
210.10	101.0
231.90	104.0
249.60	107.0
263.70	108.0
290.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55