

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110520\
 Data File : VV019242.D
 Acq On : 04 Nov 2020 12:22
 Operator : SY/MD
 Sample : L4543-16ME 2X
 Misc : 5.70g/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG474ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	82	rVB	89945	97017	12.28%	1.491%
2	1.573	144	150	160	rBV	89539	109092	13.81%	1.676%
3	2.110	305	317	341	rBV	184499	275684	34.91%	4.236%
4	2.431	413	417	419	rBV	245	213	0.03%	0.003%
5	2.515	435	443	450	rVB3	1451	1816	0.23%	0.028%
6	2.859	548	550	556	rVB	293	164	0.02%	0.003%
7	2.884	556	558	560	rBV	223	85	0.01%	0.001%
8	2.897	560	562	565	rVB	247	131	0.02%	0.002%
9	2.929	569	572	575	rBV	326	231	0.03%	0.004%
10	3.026	599	602	605	rVB	305	159	0.02%	0.002%
11	3.048	605	609	614	rVV2	211	245	0.03%	0.004%
12	3.074	614	617	620	rVB	188	116	0.01%	0.002%
13	3.225	662	664	666	rBV2	155	86	0.01%	0.001%
14	3.331	694	697	700	rBV	291	182	0.02%	0.003%
15	3.373	709	710	711	rBV	140	43	0.01%	0.001%
16	3.418	719	724	727	rBV	393	305	0.04%	0.005%
17	3.692	805	809	816	rBV2	325	389	0.05%	0.006%
18	3.720	816	818	821	rVB	250	108	0.01%	0.002%
19	3.737	821	823	828	rBV	160	129	0.02%	0.002%
20	3.791	838	840	843	rBV	236	97	0.01%	0.001%
21	3.846	854	857	859	rBV2	286	190	0.02%	0.003%
22	3.910	865	877	897	rBV	34118	106240	13.45%	1.633%
23	4.367	1004	1019	1052	rVB	126165	314622	39.84%	4.835%
24	4.579	1083	1085	1091	rVB3	513	439	0.06%	0.007%
25	4.614	1092	1096	1100	rBV2	283	280	0.04%	0.004%
26	4.701	1122	1123	1124	rBV2	119	35	0.00%	0.001%
27	4.765	1140	1143	1146	rBV	245	195	0.02%	0.003%
28	4.827	1159	1162	1164	rBV	196	114	0.01%	0.002%
29	4.971	1203	1207	1210	rBV	213	192	0.02%	0.003%
30	5.061	1219	1235	1265	rBV2	309469	789746	100.00%	12.135%
31	5.312	1311	1313	1314	rBV	350	123	0.02%	0.002%
32	5.363	1323	1329	1331	rBV3	713	495	0.06%	0.008%
33	5.376	1331	1333	1334	rBV	287	109	0.01%	0.002%
34	5.560	1388	1390	1392	rVB	174	53	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110520\
 Data File : VV019242.D
 Acq On : 04 Nov 2020 12:22
 Operator : SY/MD
 Sample : L4543-16ME 2X
 Misc : 5.70µ/5.00mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG474ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.579	1392	1396	1400	rBV2	309	315	0.04%	0.005%
36	5.634	1401	1413	1443	rBV	299320	602059	76.23%	9.251%
37	5.884	1486	1491	1494	rVB3	540	454	0.06%	0.007%
38	6.087	1542	1554	1584	rVB	172856	354185	44.85%	5.443%
39	6.357	1635	1638	1641	rVB2	237	148	0.02%	0.002%
40	6.380	1641	1645	1646	rBV	191	120	0.02%	0.002%
41	6.428	1658	1660	1665	rBV	176	108	0.01%	0.002%
42	6.511	1680	1686	1691	rBV	201	294	0.04%	0.005%
43	6.569	1702	1704	1705	rBV	183	47	0.01%	0.001%
44	6.614	1716	1718	1721	rBV	170	132	0.02%	0.002%
45	6.653	1728	1730	1731	rVB	149	40	0.01%	0.001%
46	6.688	1738	1741	1742	rBV	143	56	0.01%	0.001%
47	6.752	1759	1761	1765	rVB2	138	82	0.01%	0.001%
48	6.794	1768	1774	1777	rBV2	279	323	0.04%	0.005%
49	6.916	1809	1812	1814	rBV	223	177	0.02%	0.003%
50	7.003	1828	1839	1869	rBV	97216	184757	23.39%	2.839%
51	7.161	1884	1888	1893	rBV3	469	513	0.06%	0.008%
52	7.215	1904	1905	1906	rBV3	165	41	0.01%	0.001%
53	7.334	1930	1942	1961	rBV	356209	621906	78.75%	9.556%
54	7.640	2027	2037	2061	rBV	68072	129254	16.37%	1.986%
55	7.820	2090	2093	2096	rVB2	421	252	0.03%	0.004%
56	7.881	2110	2112	2113	rBV2	183	73	0.01%	0.001%
57	7.913	2121	2122	2123	rBB	62	27	0.00%	0.000%
58	7.945	2130	2132	2133	rBV	306	133	0.02%	0.002%
59	7.994	2138	2147	2165	rVB	39138	65873	8.34%	1.012%
60	8.122	2175	2187	2229	rBV2	126374	336117	42.56%	5.165%
61	8.489	2298	2301	2305	rBV	361	296	0.04%	0.005%
62	8.666	2351	2356	2360	rVB2	235	235	0.03%	0.004%
63	8.688	2360	2363	2367	rVB	213	175	0.02%	0.003%
64	8.711	2368	2370	2375	rVB	262	182	0.02%	0.003%
65	8.781	2387	2392	2400	rBV2	293	484	0.06%	0.007%
66	8.871	2408	2420	2444	rBV	447888	749374	94.89%	11.515%
67	9.064	2477	2480	2482	rBV	249	189	0.02%	0.003%
68	9.145	2502	2505	2507	rBV2	240	149	0.02%	0.002%
69	9.293	2544	2551	2556	rBV2	547	968	0.12%	0.015%
70	9.373	2573	2576	2580	rBV	292	234	0.03%	0.004%
71	9.453	2598	2601	2604	rBV	271	200	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110520\
 Data File : VV019242.D
 Acq On : 04 Nov 2020 12:22
 Operator : SY/MD
 Sample : L4543-16ME 2X
 Misc : 5.70g/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG474ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	9.646	2659	2661	2664	rBV	164	87	0.01%	0.001%
73	9.797	2707	2708	2711	rBV	202	124	0.02%	0.002%
74	9.846	2718	2723	2725	rBV	225	210	0.03%	0.003%
75	10.019	2774	2777	2780	rBV2	237	187	0.02%	0.003%
76	10.080	2794	2796	2798	rBV	156	53	0.01%	0.001%
77	10.241	2832	2846	2867	rBV	211680	348087	44.08%	5.349%
78	10.376	2886	2888	2890	rBV	306	165	0.02%	0.003%
79	10.585	2952	2953	2955	rBV	218	113	0.01%	0.002%
80	10.739	2998	3001	3002	rBV	164	90	0.01%	0.001%
81	10.810	3020	3023	3025	rBV2	376	253	0.03%	0.004%
82	11.061	3096	3101	3107	rVB2	506	677	0.09%	0.010%
83	11.167	3129	3134	3138	rBV2	687	751	0.10%	0.012%
84	11.270	3155	3166	3186	rBV	497825	771170	97.65%	11.850%
85	11.498	3235	3237	3238	rBV	243	92	0.01%	0.001%
86	11.646	3271	3283	3305	rBV	408873	635888	80.52%	9.771%
87	12.112	3425	3428	3429	rBV2	271	128	0.02%	0.002%
88	12.302	3485	3487	3489	rBV	262	144	0.02%	0.002%
89	13.026	3707	3712	3716	rBV2	345	441	0.06%	0.007%


Sum of corrected areas: 6507757

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110520\
Data File : VV019242.D
Acq On : 04 Nov 2020 12:22
Operator : SY/MD
Sample : L4543-16ME 2X
Misc : 5.70uL/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG474ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

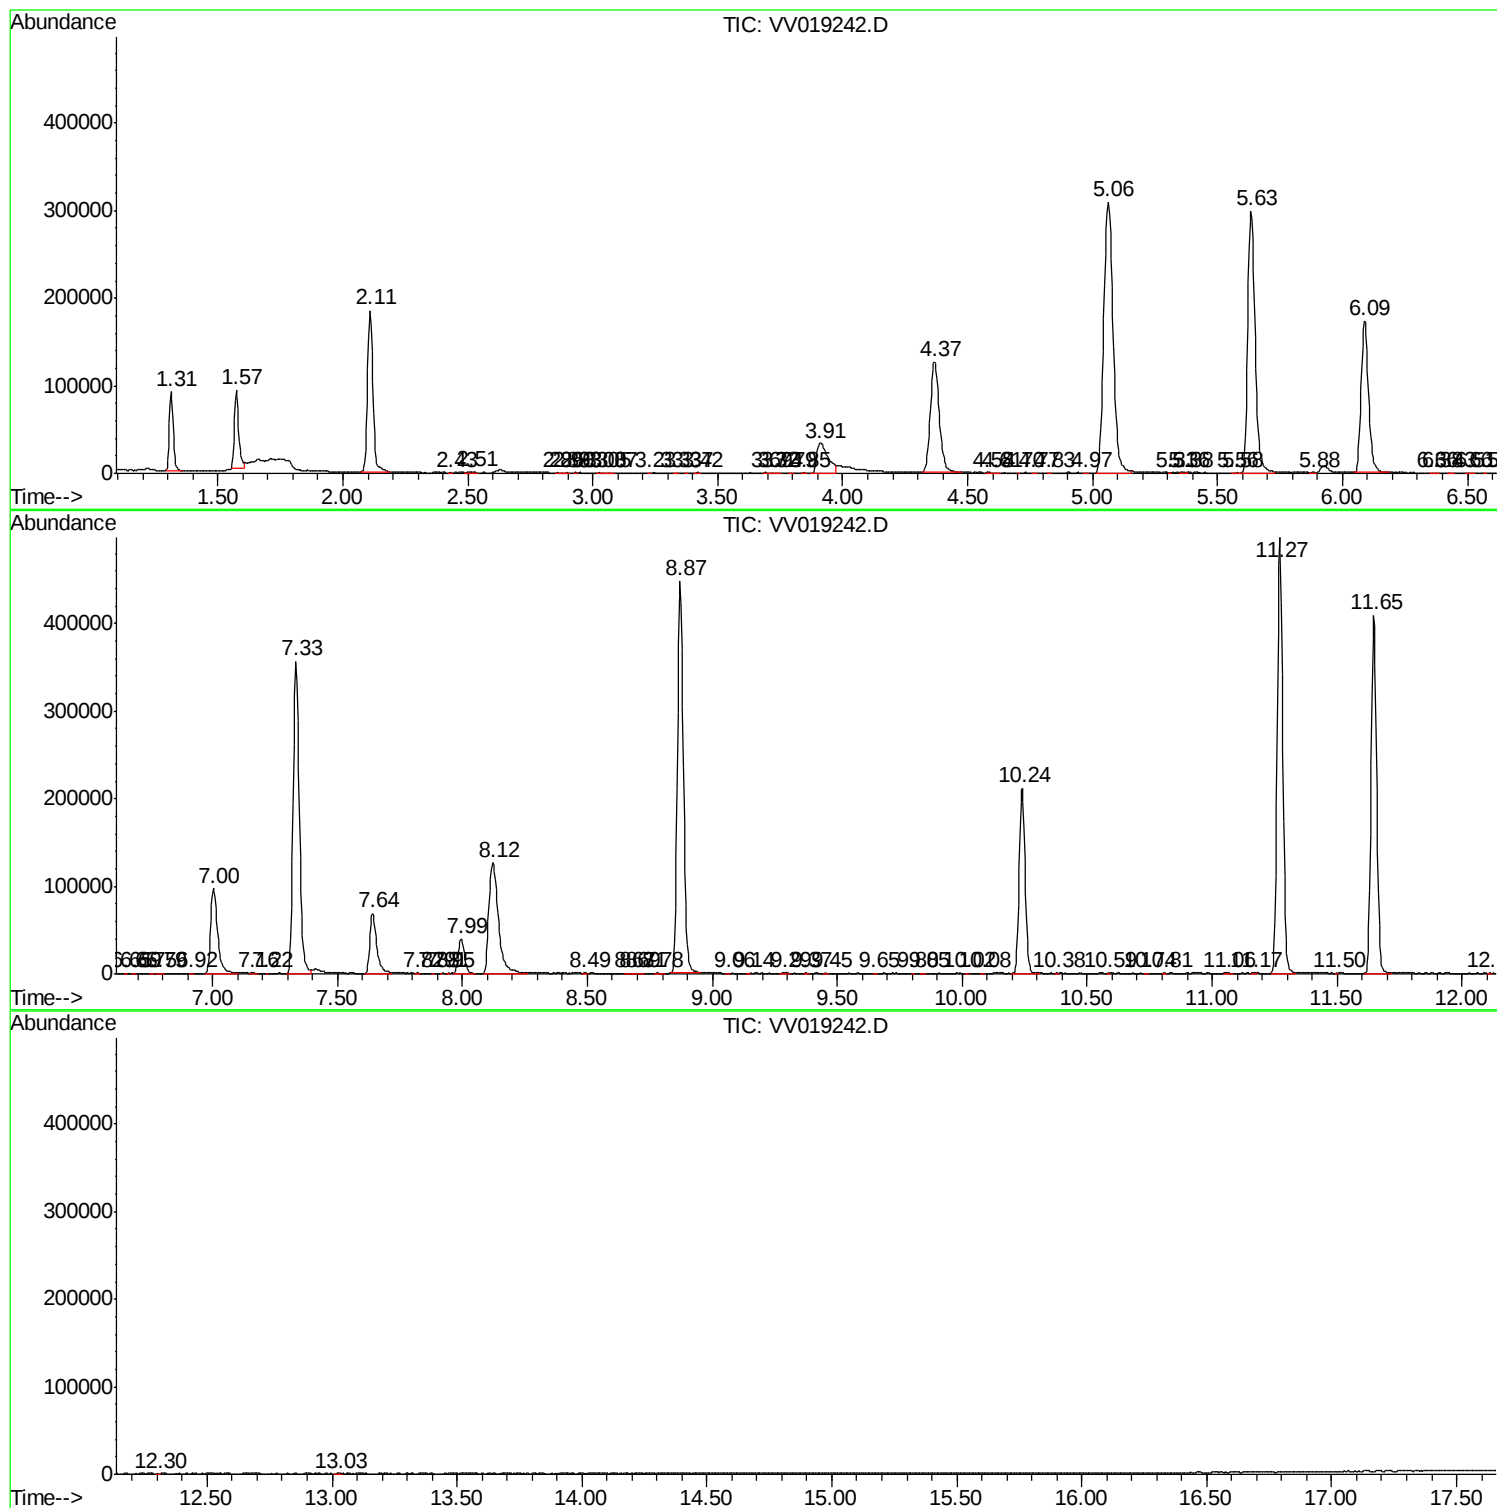

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110520\
Data File : VV019242.D
Acq On : 04 Nov 2020 12:22
Operator : SY/MD
Sample : L4543-16ME 2X
Misc : 5.70g/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG474ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV110520\
Data File : VV019242.D
Acq On : 04 Nov 2020 12:22
Operator : SY/MD
Sample : L4543-16ME 2X
Misc : 5.70g/5.00mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG474ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc