

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110520\
 Data File : VV019244.D
 Acq On : 04 Nov 2020 13:12
 Operator : SY/MD
 Sample : L4615-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG462

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	172316	168552	15.58%	2.192%
2	1.579	145	152	164	rVB	142079	156271	14.44%	2.033%
3	2.123	311	321	336	rBV	282760	417402	38.57%	5.429%
4	2.364	393	396	398	rBV2	513	319	0.03%	0.004%
5	2.579	459	463	467	rBV2	372	383	0.04%	0.005%
6	2.676	491	493	496	rBV2	323	271	0.03%	0.004%
7	2.724	506	508	509	rBV	225	80	0.01%	0.001%
8	2.756	515	518	523	rVB	213	171	0.02%	0.002%
9	2.782	523	526	528	rBV	235	138	0.01%	0.002%
10	2.888	558	559	560	rVB	136	26	0.00%	0.000%
11	2.930	569	572	573	rBV	160	82	0.01%	0.001%
12	3.094	621	623	626	rVB	271	113	0.01%	0.001%
13	3.106	626	627	630	rBV	132	53	0.00%	0.001%
14	3.222	660	663	666	rBV2	206	111	0.01%	0.001%
15	3.270	676	678	681	rVB	253	103	0.01%	0.001%
16	3.296	681	686	689	rBV2	251	231	0.02%	0.003%
17	3.322	689	694	697	rBV2	220	234	0.02%	0.003%
18	3.428	724	727	728	rBV	148	77	0.01%	0.001%
19	3.492	743	747	749	rBV	278	183	0.02%	0.002%
20	3.682	802	806	809	rBV2	247	218	0.02%	0.003%
21	3.701	809	812	813	rBV	257	110	0.01%	0.001%
22	3.743	822	825	827	rBV	199	116	0.01%	0.002%
23	3.836	850	854	857	rBV2	253	198	0.02%	0.003%
24	3.907	866	876	912	rBV	68858	196001	18.11%	2.550%
25	4.373	1006	1021	1048	rBV	172386	426968	39.46%	5.554%
26	4.679	1113	1116	1118	rBV3	441	283	0.03%	0.004%
27	4.733	1128	1133	1137	rBV2	313	349	0.03%	0.005%
28	4.756	1137	1140	1143	rBV2	164	126	0.01%	0.002%
29	4.836	1161	1165	1167	rBV	259	194	0.02%	0.003%
30	4.981	1207	1210	1212	rBV	179	133	0.01%	0.002%
31	5.071	1221	1238	1271	rBV2	425553	1082072	100.00%	14.075%
32	5.399	1338	1340	1342	rBV	196	74	0.01%	0.001%
33	5.431	1342	1350	1352	rVV2	389	399	0.04%	0.005%
34	5.595	1398	1401	1402	rBV2	205	135	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110520\
 Data File : VV019244.D
 Acq On : 04 Nov 2020 13:12
 Operator : SY/MD
 Sample : L4615-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG462

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.640	1403	1415	1446	rVV	256705	512007	47.32%	6.660%
36	5.929	1495	1505	1526	rVB3	11245	23590	2.18%	0.307%
37	6.093	1542	1556	1584	rBV	238406	480773	44.43%	6.254%
38	6.238	1598	1601	1602	rBV2	511	337	0.03%	0.004%
39	6.315	1622	1625	1627	rBV2	164	117	0.01%	0.002%
40	6.380	1642	1645	1649	rBV	246	154	0.01%	0.002%
41	6.437	1661	1663	1665	rBV	210	125	0.01%	0.002%
42	6.576	1704	1706	1708	rBV2	270	119	0.01%	0.002%
43	6.640	1723	1726	1727	rBV2	198	127	0.01%	0.002%
44	6.798	1773	1775	1781	rVB2	422	281	0.03%	0.004%
45	6.830	1783	1785	1787	rBV	136	61	0.01%	0.001%
46	6.865	1794	1796	1800	rVB	297	191	0.02%	0.002%
47	6.913	1808	1811	1813	rVB	235	139	0.01%	0.002%
48	6.929	1813	1816	1820	rVB	318	256	0.02%	0.003%
49	6.952	1820	1823	1824	rBV	171	103	0.01%	0.001%
50	6.965	1824	1827	1829	rBV	144	84	0.01%	0.001%
51	7.007	1829	1840	1866	rBV	139400	251355	23.23%	3.270%
52	7.338	1931	1943	1960	rBV	509436	868271	80.24%	11.294%
53	7.640	2028	2037	2074	rBV	99245	173508	16.03%	2.257%
54	7.839	2095	2099	2100	rBV2	332	243	0.02%	0.003%
55	7.878	2109	2111	2114	rBV	214	180	0.02%	0.002%
56	8.052	2161	2165	2170	rBV2	341	443	0.04%	0.006%
57	8.106	2172	2182	2221	rVV	239651	434375	40.14%	5.650%
58	8.447	2286	2288	2289	rBV	284	99	0.01%	0.001%
59	8.569	2323	2326	2330	rBV2	189	146	0.01%	0.002%
60	8.704	2363	2368	2371	rBV	214	271	0.03%	0.004%
61	8.727	2373	2375	2379	rVV	147	110	0.01%	0.001%
62	8.871	2406	2420	2440	rBV	389456	621266	57.41%	8.081%
63	9.138	2501	2503	2506	rBV	196	120	0.01%	0.002%
64	9.216	2523	2527	2531	rBV	314	331	0.03%	0.004%
65	9.270	2538	2544	2547	rBV2	381	398	0.04%	0.005%
66	9.315	2555	2558	2560	rBV	197	142	0.01%	0.002%
67	9.498	2612	2615	2620	rBV2	241	250	0.02%	0.003%
68	9.595	2643	2645	2648	rBV	220	129	0.01%	0.002%
69	9.759	2693	2696	2698	rBV2	238	140	0.01%	0.002%
70	9.900	2736	2740	2743	rBV	250	268	0.02%	0.003%
71	9.945	2752	2754	2760	rBV2	164	148	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110520\
 Data File : VV019244.D
 Acq On : 04 Nov 2020 13:12
 Operator : SY/MD
 Sample : L4615-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG462

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	9.984	2763	2766	2768	rBV	138	91	0.01%	0.001%
73	10.000	2768	2771	2773	rBV2	243	166	0.02%	0.002%
74	10.145	2810	2816	2824	rVB5	2063	3114	0.29%	0.041%
75	10.177	2824	2826	2828	rBV	187	97	0.01%	0.001%
76	10.235	2833	2844	2865	rVV	277991	438452	40.52%	5.703%
77	10.695	2984	2987	2988	rBV2	171	100	0.01%	0.001%
78	10.855	3034	3037	3040	rBV	337	203	0.02%	0.003%
79	10.932	3054	3061	3065	rBV3	1535	2103	0.19%	0.027%
80	11.167	3130	3134	3140	rBV3	723	832	0.08%	0.011%
81	11.228	3150	3153	3155	rBV	270	172	0.02%	0.002%
82	11.270	3155	3166	3185	rVV	401970	610491	56.42%	7.941%
83	11.402	3200	3207	3212	rBV4	839	1221	0.11%	0.016%
84	11.514	3236	3242	3244	rBV	308	311	0.03%	0.004%
85	11.646	3270	3283	3308	rBV	513965	805899	74.48%	10.483%
86	11.817	3333	3336	3338	rBV2	725	367	0.03%	0.005%
87	11.955	3377	3379	3382	rBV	250	135	0.01%	0.002%
88	12.103	3422	3425	3427	rBV2	147	118	0.01%	0.002%
89	12.190	3449	3452	3455	rBV	195	168	0.02%	0.002%
90	12.630	3586	3589	3590	rBV	358	206	0.02%	0.003%
91	12.923	3677	3680	3683	rVB	270	180	0.02%	0.002%
92	13.534	3867	3870	3873	rBV	256	161	0.01%	0.002%
93	13.556	3873	3877	3880	rBV2	336	307	0.03%	0.004%


Sum of corrected areas: 7687727

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110520\
Data File : VV019244.D
Acq On : 04 Nov 2020 13:12
Operator : SY/MD
Sample : L4615-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG462

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

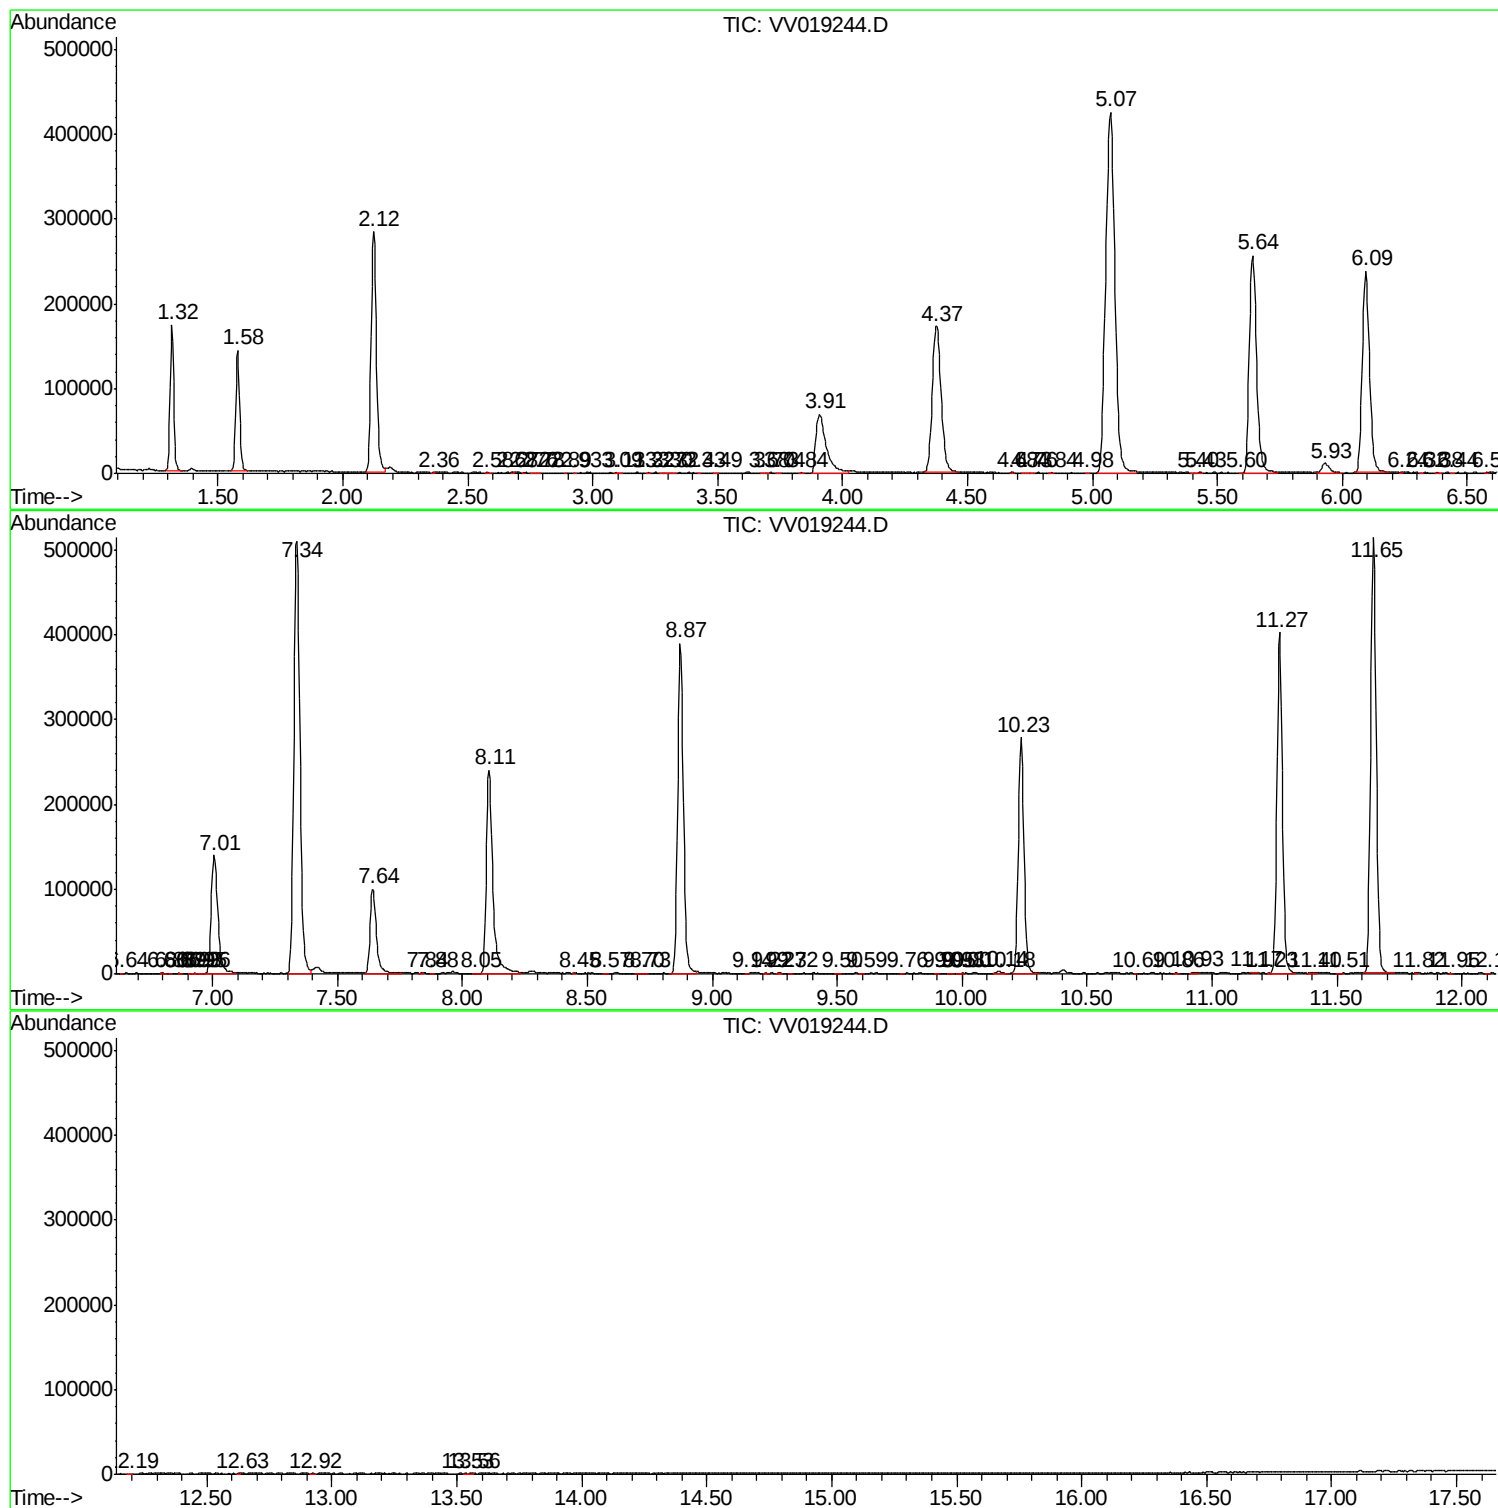

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110520\
Data File : VV019244.D
Acq On : 04 Nov 2020 13:12
Operator : SY/MD
Sample : L4615-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG462

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110520\
Data File : VV019244.D
Acq On : 04 Nov 2020 13:12
Operator : SY/MD
Sample : L4615-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG462

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc