


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV110520\
 Data File : VV019238.D
 Acq On : 04 Nov 2020 08:41
 Operator : SY/MD
 Sample : BFB88
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB88

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 06 01:20:06 2020

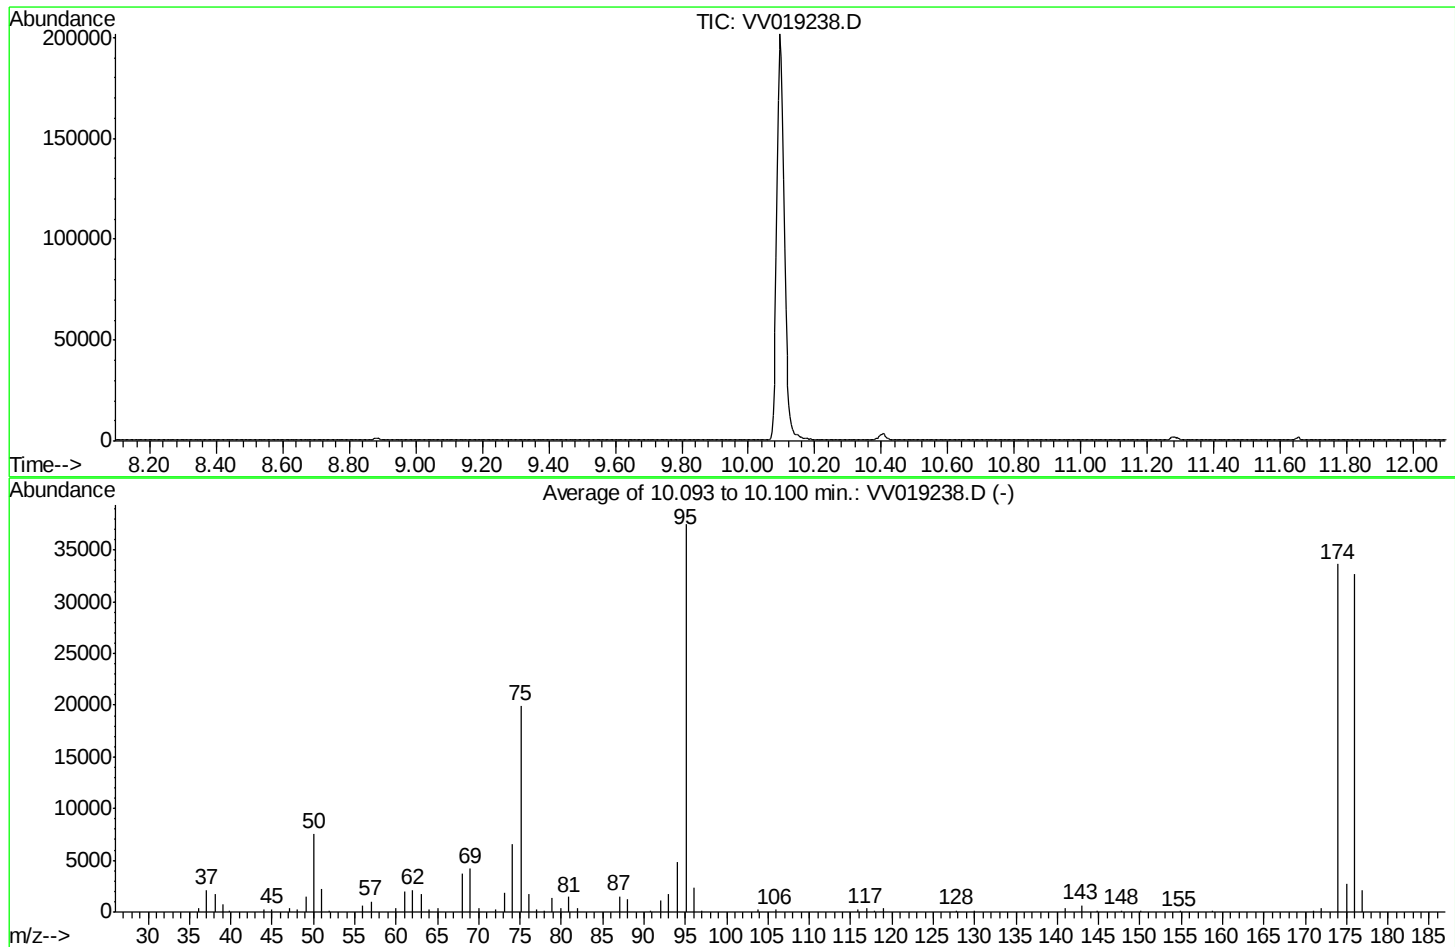

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	7564	PASS
75	95	30	80	53.3	19973	PASS
95	95	100	100	100.0	37496	PASS
96	95	5	9	6.4	2416	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.8	33661	PASS
175	174	5	9	8.0	2686	PASS
176	174	95	101	97.3	32744	PASS
177	176	5	9	6.5	2138	PASS

m/z	Abundance
36.00	389.0
37.10	2082.0
38.00	1561.0
39.10	749.0
39.80	131.0
44.00	854.0
45.00	285.0
47.10	417.0
48.00	246.0
49.00	1427.0
50.10	7031.0
51.00	2197.0
51.90	129.0
56.00	561.0
57.00	1009.0
59.90	386.0
61.00	1859.0
62.00	1983.0
63.10	1758.0
63.90	301.0
65.00	319.0
68.00	3713.0
69.00	4091.0
70.00	344.0
72.10	196.0
73.10	1800.0
74.00	6276.0
75.10	19200.0
76.10	1684.0
77.10	194.0
77.90	107.0
78.90	1406.0
79.90	428.0
80.90	1495.0
81.90	311.0
87.00	1396.0
88.00	1191.0
90.90	110.0
92.00	1093.0
93.00	1622.0
94.00	4702.0
95.10	36608.0
96.00	2306.0
97.00	107.0
103.90	189.0
105.90	259.0
115.90	201.0
116.90	346.0
117.90	121.0
118.90	300.0
127.80	186.0
130.00	140.0
141.00	419.0
142.90	619.0
144.80	125.0
147.80	127.0
158.70	110.0
170.90	181.0
171.80	396.0
174.00	33304.0
175.00	2724.0
176.00	32384.0
177.00	2028.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
36.10	399.0
37.00	2234.0
38.10	1761.0
39.10	721.0
39.90	128.0
44.00	811.0
45.00	280.0
47.00	442.0
48.00	322.0
49.00	1567.0
50.10	7794.0
51.00	2392.0
51.90	117.0
56.00	612.0
57.00	1074.0
59.90	379.0
61.00	2045.0
62.00	2213.0
63.10	1775.0
64.00	308.0
65.00	327.0
68.00	3879.0
69.00	4333.0
70.00	440.0
72.10	243.0
73.10	1989.0
74.10	6843.0
75.10	20624.0
76.10	1703.0
77.00	240.0
77.90	142.0
78.90	1478.0
80.00	445.0
80.90	1476.0
81.90	379.0
87.00	1543.0
88.00	1322.0
90.80	127.0
92.00	1153.0
93.00	1781.0
94.00	4987.0
95.10	38632.0
96.00	2467.0
97.00	108.0
103.90	203.0
105.90	239.0
115.90	216.0
116.90	362.0
117.90	156.0
119.00	336.0
127.80	205.0
129.90	139.0
141.00	385.0
142.90	696.0
144.90	149.0
147.80	129.0
150.10	124.0
154.80	140.0
158.80	102.0
171.00	158.0
171.90	441.0
174.00	34848.0
175.00	2775.0
176.00	33816.0
177.00	2194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
36.10	369.0
37.00	2167.0
38.00	1773.0
39.00	643.0
39.90	132.0
44.00	751.0
45.00	268.0
47.00	427.0
48.00	334.0
49.10	1560.0
50.10	7869.0
51.00	2279.0
56.00	597.0
57.00	1014.0
59.90	345.0
61.00	2014.0
62.00	2270.0
63.10	1618.0
64.00	271.0
65.00	302.0
68.00	3633.0
69.00	4135.0
70.00	418.0
72.10	254.0
73.10	1906.0
74.10	6663.0
75.10	20096.0
76.00	1661.0
77.00	263.0
77.90	192.0
78.90	1344.0
79.90	422.0
80.90	1410.0
81.90	402.0
87.00	1589.0
88.00	1371.0
90.80	149.0
92.00	1103.0
93.00	1786.0
94.00	4933.0
95.10	37248.0
96.00	2477.0
97.00	101.0
103.80	213.0
105.90	182.0
115.90	167.0
116.90	347.0
117.90	178.0
118.90	309.0
127.80	166.0
129.80	144.0
140.90	370.0
142.90	694.0
144.90	131.0
147.80	140.0
150.00	117.0
154.90	165.0
171.10	137.0
172.00	449.0
174.00	32832.0
175.00	2560.0
176.00	32032.0
176.90	2194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
44.00	578.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88