


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023220.D
Acq On : 05 Nov 2021 10:29
Operator : SY/MD
Sample : VV1105WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sampled :
VBLK242

Quant Time: Nov 09 02:04:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 02:04:24 2021
Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/10/2021
Supervised By : Mahesh Dadoda 11/10/2021

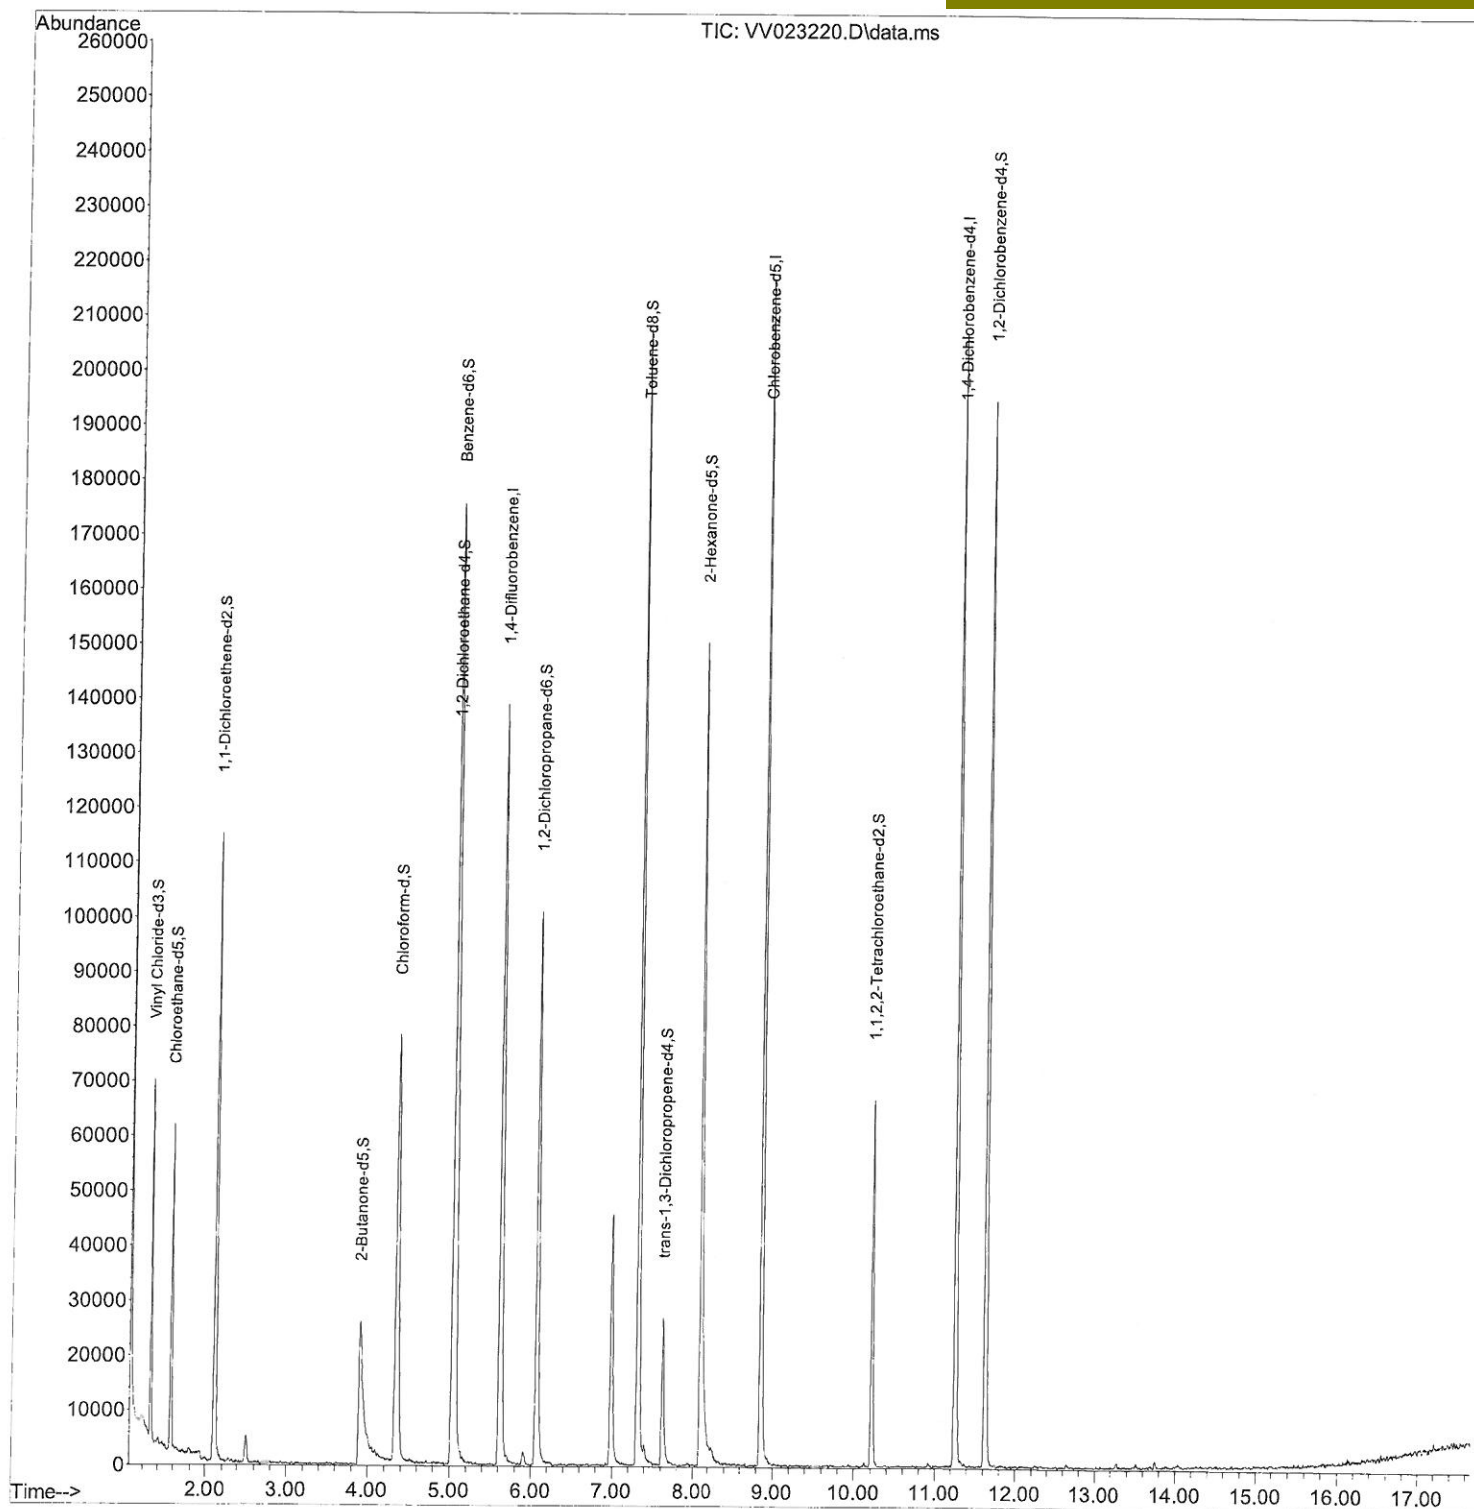

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023220.D
 Acq On : 05 Nov 2021 10:29
 Operator : SY/MD
 Sample : VV1105WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK242

Quant Time: Nov 09 02:04:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 02:04:24 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/10/2021
 Supervised By :Mahesh Dadoda 11/10/2021

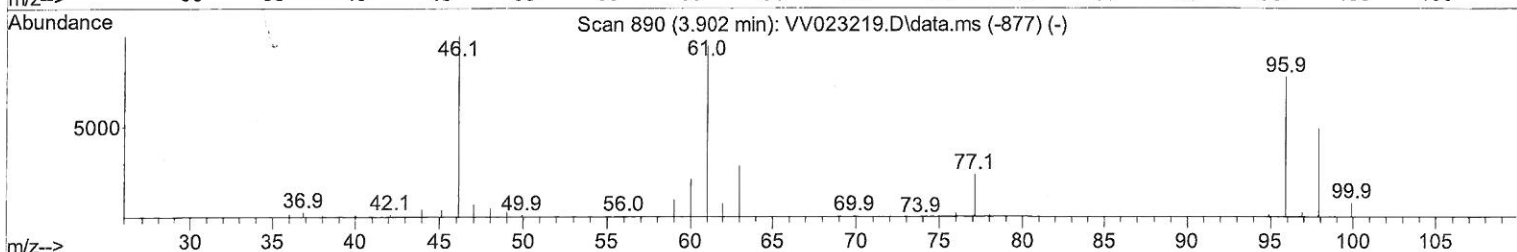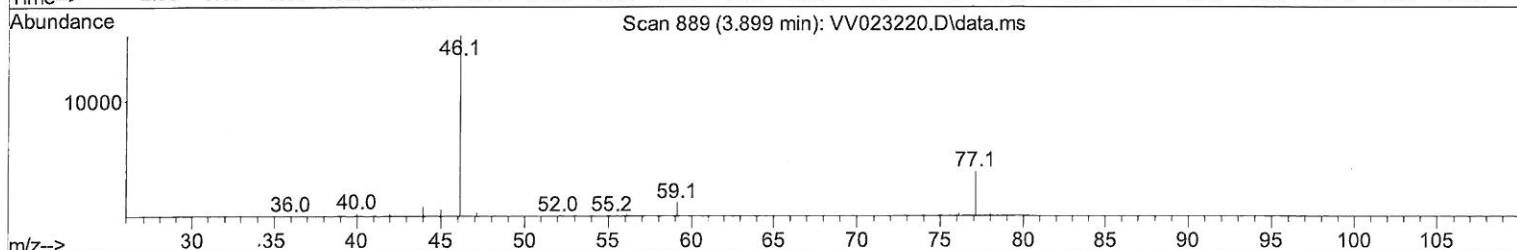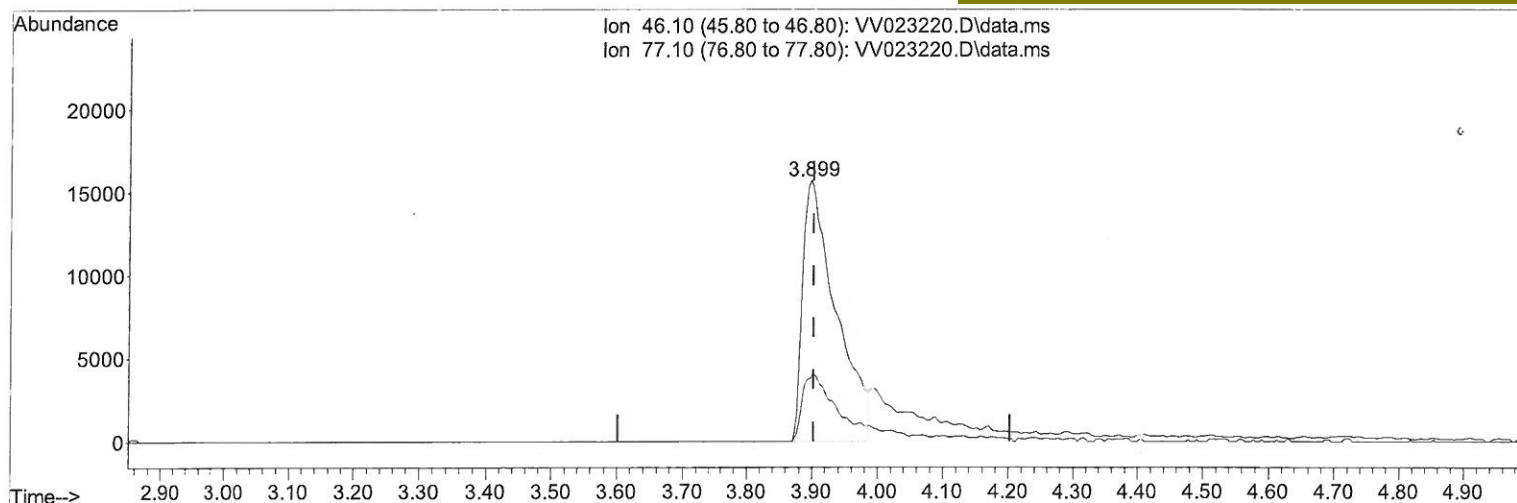

TIC: VV023220.D\data.ms

(20) 2-Butanone-d5 (S)

3.899min (-0.003) 41.61 ug/L

response 55274

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	24.15
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023220.D
 Acq On : 05 Nov 2021 10:29
 Operator : SY/MD
 Sample : VV1105WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 VBLK242

Quant Time: Nov 09 02:04:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 02:04:24 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/10/2021
 Supervised By : Mahesh Dadoda 11/10/2021

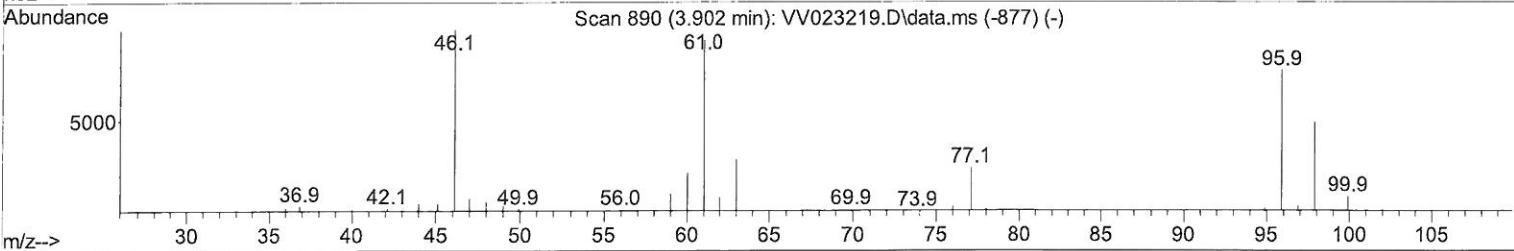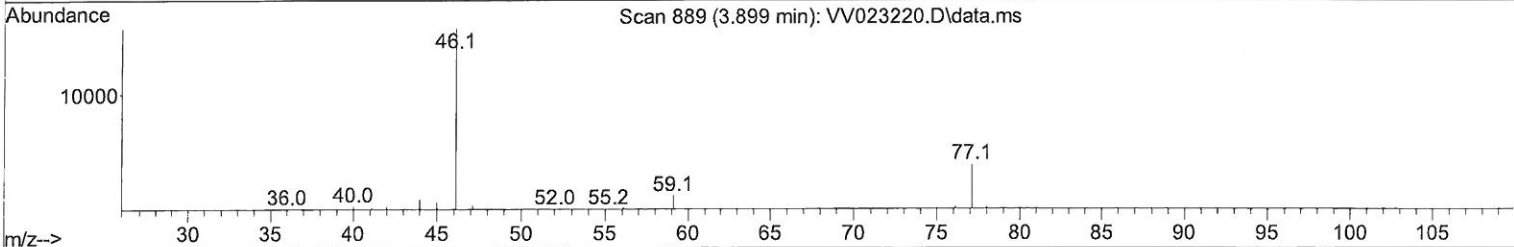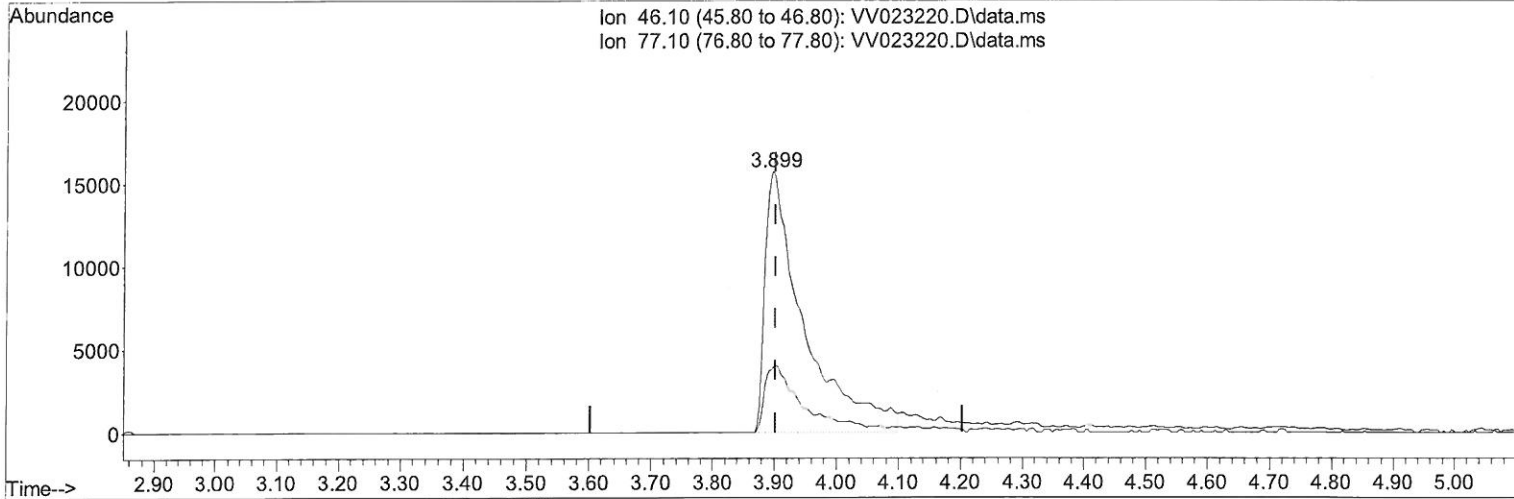

TIC: VV023220.D\data.ms

(20) 2-Butanone-d5 (S)

3.899min (-0.003) 51.22 ug/L m

response 68040

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	19.62
0.00	0.00	0.00
0.00	0.00	0.00

MD
 11/10/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\WV110521\
 Data File : WV023220.D
 Acq On : 05 Nov 2021 10:29
 Operator : SY/MD
 Sample : WV1105WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 VBLK242

Quant Time: Nov 09 02:04:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 02:04:24 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/10/2021
 Supervised By : Mahesh Dadoda 11/10/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	123076	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	122019	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56063	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	40451	5.246	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	= 105.000%	
7) Chloroethane-d5	1.564	69	34391	5.473	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	= 109.400%	
11) 1,1-Dichloroethene-d2	2.105	63	57853	4.008	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	= 80.200%	
20) 2-Butanone-d5	3.899	46	68040m	51.222	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	= 102.440%	
24) Chloroform-d	4.346	84	83596	5.087	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 101.800%	
26) 1,2-Dichloroethane-d4	5.031	65	39642	5.365	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 107.200%	
32) Benzene-d6	5.047	84	162451	5.189	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 103.800%	
36) 1,2-Dichloropropane-d6	6.066	67	48867	5.302	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	= 106.000%	
41) Toluene-d8	7.313	98	138058	4.706	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 94.200%	
43) trans-1,3-Dichloroprop...	7.622	79	17179	4.916	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	= 98.400%	
46) 2-Hexanone-d5	8.088	63	54411	42.318	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	= 84.640%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31418	4.740	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	= 94.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	51794	5.548	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	= 111.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed