

# Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110521\  
 Data File : VV023268.D  
 Acq On : 06 Nov 2021 05:37  
 Operator : SY/MD  
 Sample : M4545-04  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 Client Sampled :  
 H4606

Quant Time: Nov 09 04:50:53 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Tue Nov 09 03:48:20 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/10/2021  
 Supervised By : Mahesh Dadoda 11/10/2021

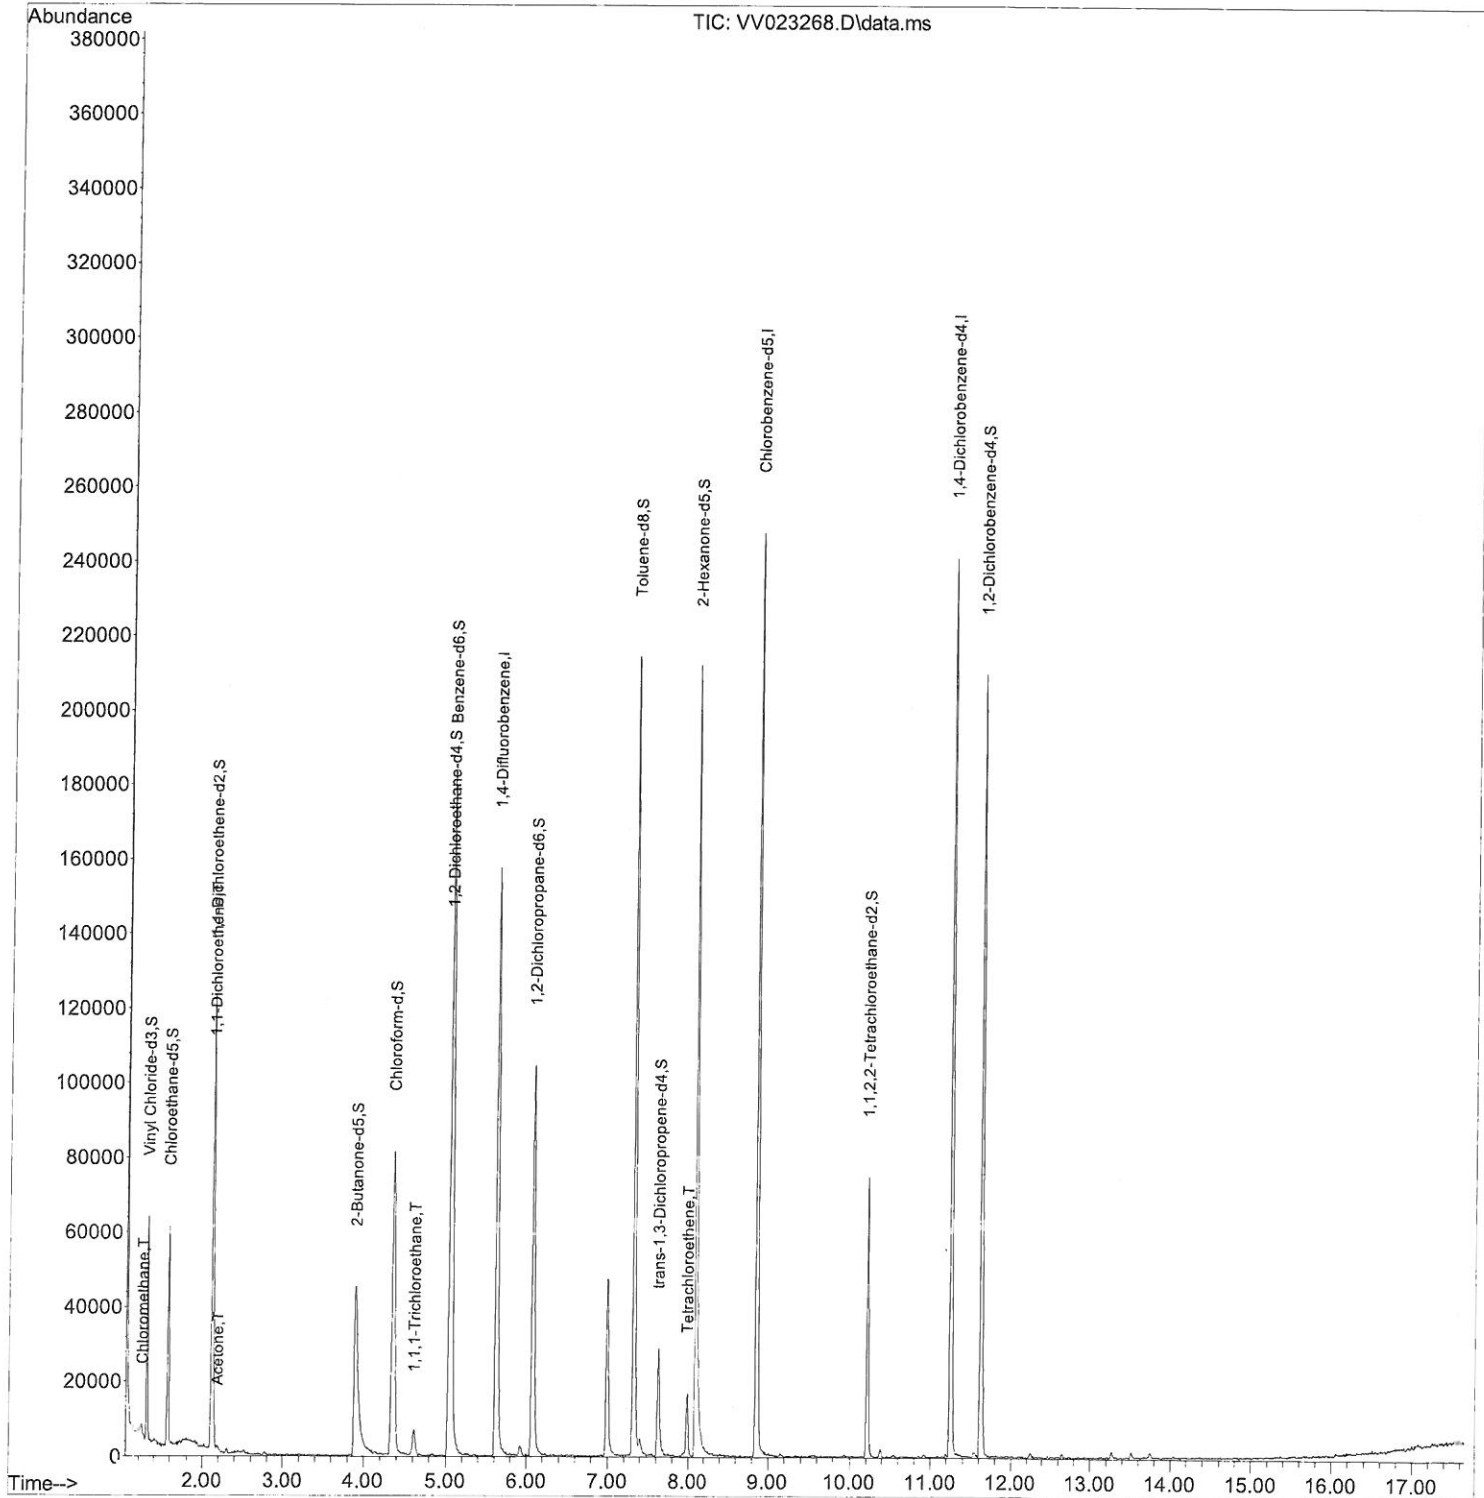

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110521\  
 Data File : VV023268.D  
 Acq On : 06 Nov 2021 05:37  
 Operator : SY/MD  
 Sample : M4545-04  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 Client Sampled :  
 H4606

Quant Time: Nov 09 04:50:53 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Tue Nov 09 03:48:20 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/10/2021  
 Supervised By : Mahesh Dadoda 11/10/2021

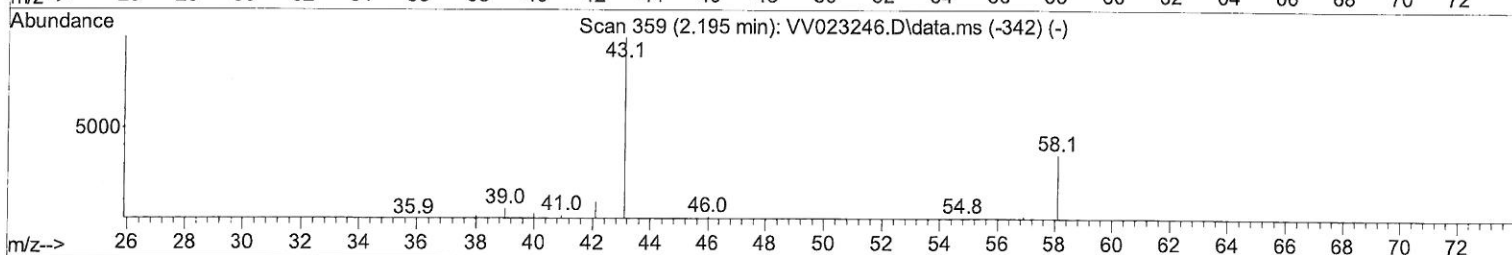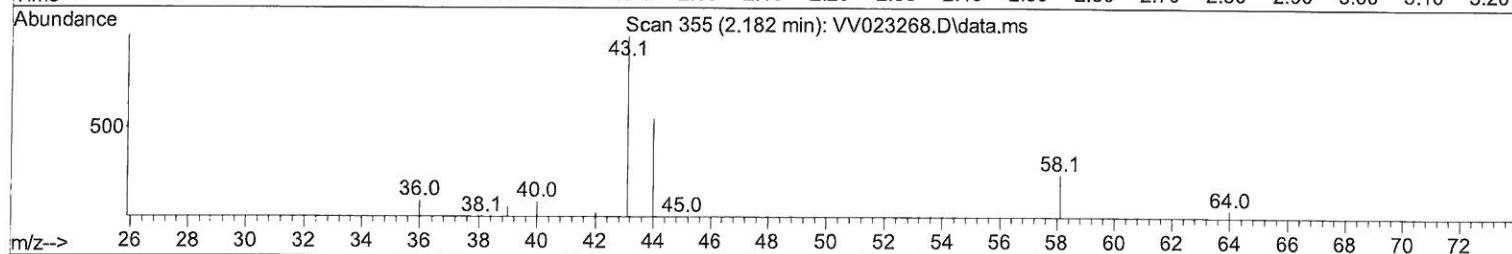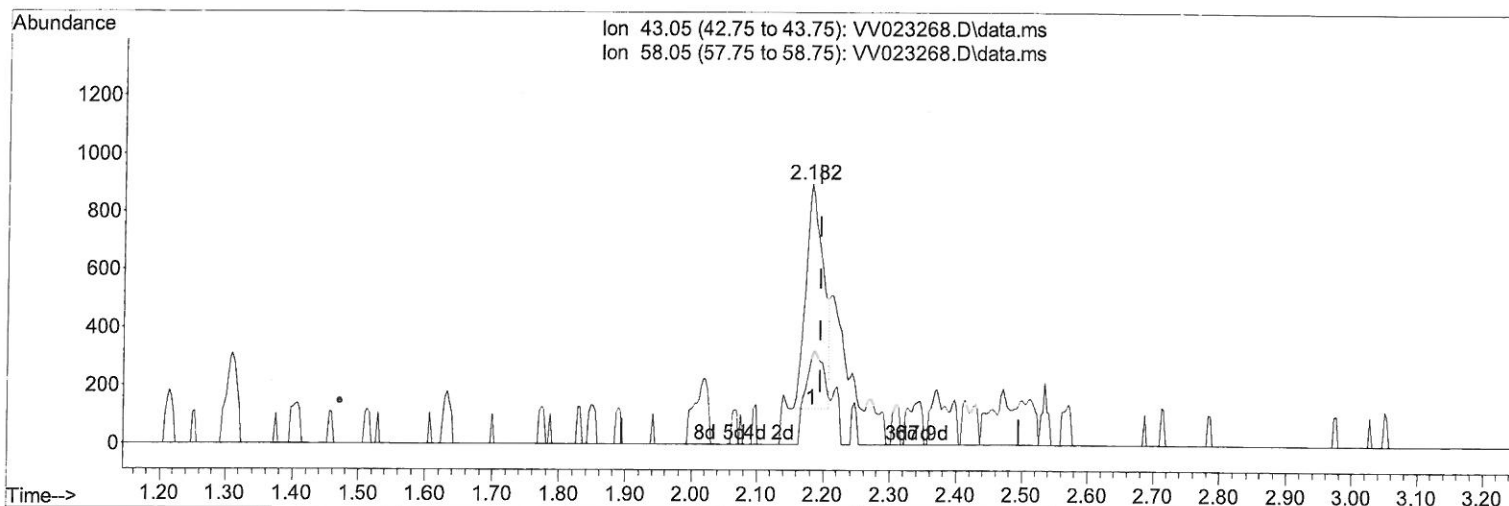

TIC: VV023268.D\data.ms

(13) Acetone (T)

2.182min (-0.013) 1.55 ug/L

response 1416

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	47.81
0.00	0.00	0.00
0.00	0.00	0.00

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110521\  
 Data File : VV023268.D  
 Acq On : 06 Nov 2021 05:37  
 Operator : SY/MD  
 Sample : M4545-04  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampled :  
 H4606

Quant Time: Nov 09 04:50:53 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Tue Nov 09 03:48:20 2021  
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/10/2021  
 Supervised By :Mahesh Dadoda 11/10/2021

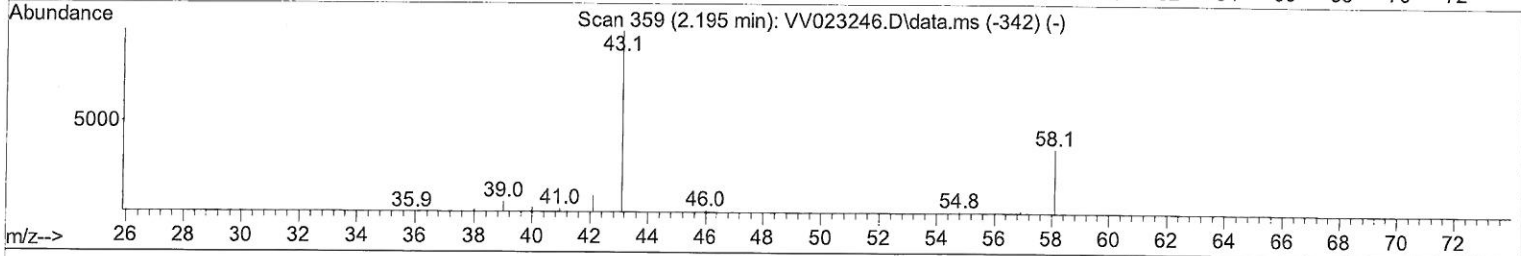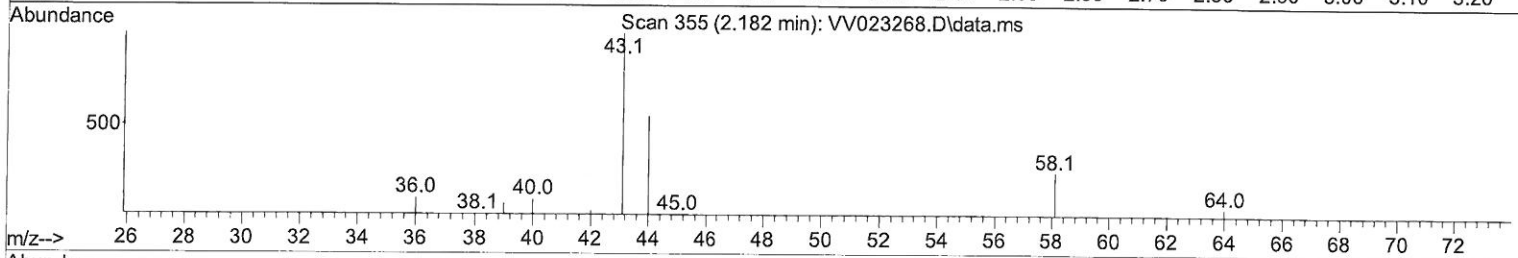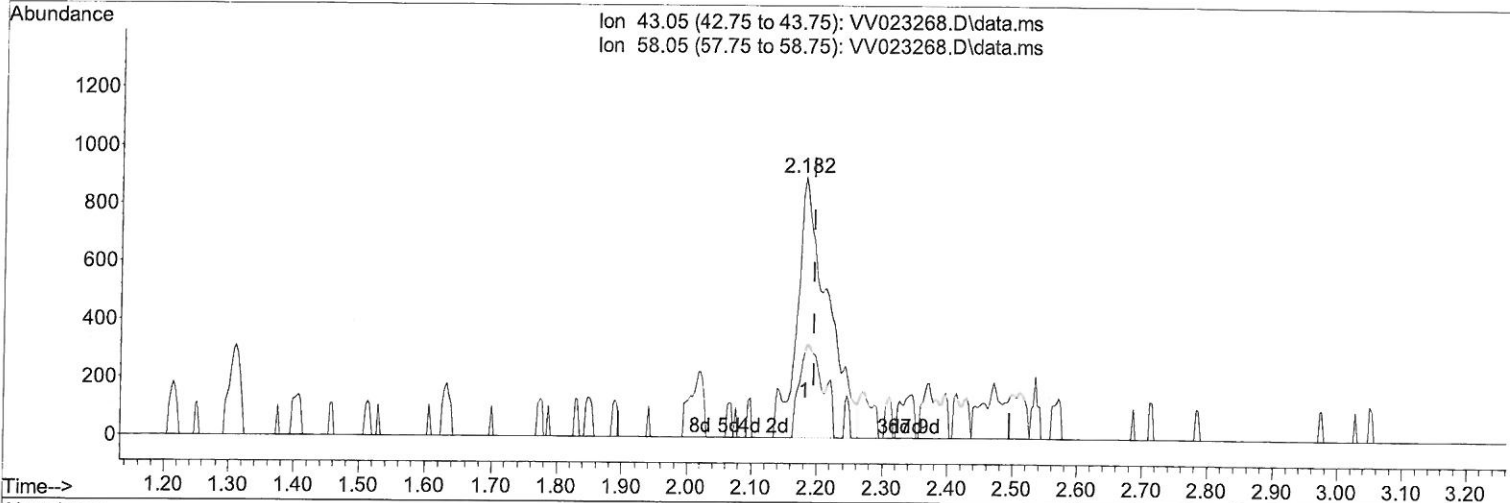

TIC: VV023268.D\data.ms

(13) Acetone (T)

2.182min (-0.013) 3.20 ug/L m

response 2926

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	23.14
0.00	0.00	0.00
0.00	0.00	0.00

> MD  
 11/10/21

## Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110521\  
 Data File : VV023268.D  
 Acq On : 06 Nov 2021 05:37  
 Operator : SY/MD  
 Sample : M4545-04  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 Client Sampled :  
 H4606

Quant Time: Nov 09 04:50:53 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Tue Nov 09 03:48:20 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/10/2021  
 Supervised By : Mahesh Dadoda 11/10/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	138716	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	136563	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65201	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	37226	4.284	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	85.600%		
7) Chloroethane-d5	1.571	69	35193	4.969	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	99.400%		
11) 1,1-Dichloroethene-d2	2.111	63	58599	3.602	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	72.000%		
20) 2-Butanone-d5	3.896	46	95568	63.834	ug/L	-0.01
Spiked Amount 50.000	Range 40 - 130		Recovery =	127.660%		
24) Chloroform-d	4.352	84	84950	4.587	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	91.800%		
26) 1,2-Dichloroethane-d4	5.037	65	40644	4.880	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.600%		
32) Benzene-d6	5.053	84	167505	4.780	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	95.600%		
36) 1,2-Dichloropropane-d6	6.072	67	51255	4.969	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	99.400%		
41) Toluene-d8	7.317	98	144883	4.412	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	88.200%		
43) trans-1,3-Dichloroprop...	7.625	79	17681	4.521	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	90.400%		
46) 2-Hexanone-d5	8.088	63	71782	49.883	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	99.760%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34899	4.705	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	94.000%		
66) 1,2-Dichlorobenzene-d4	11.625	152	56086	5.166	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	103.400%		
Target Compounds						Qvalue
3) Chloromethane	1.243	50	1441	0.125	ug/L	91
12) 1,1-Dichloroethene	2.121	96	9724	1.176	ug/L #	1
13) Acetone	2.182	43	2926m	3.199	ug/L	94
29) 1,1,1-Trichloroethane	4.609	97	5387	0.325	ug/L	96
47) Tetrachloroethene	7.979	164	3930	0.447	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed